
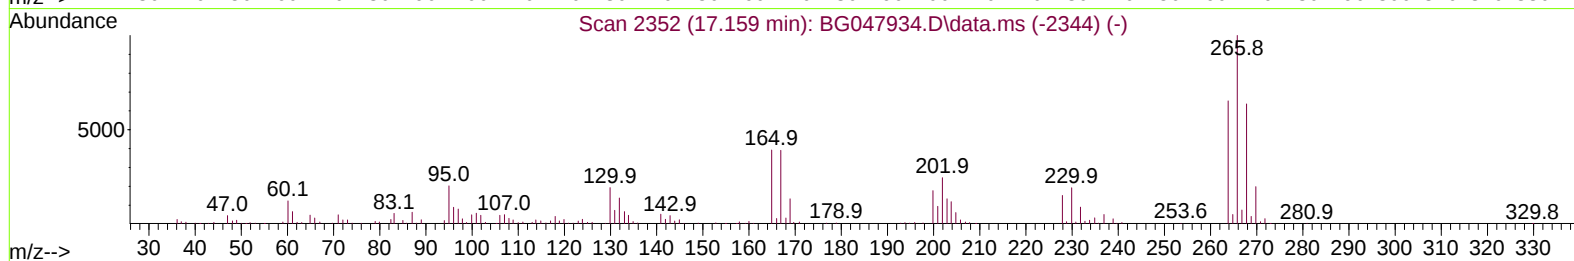
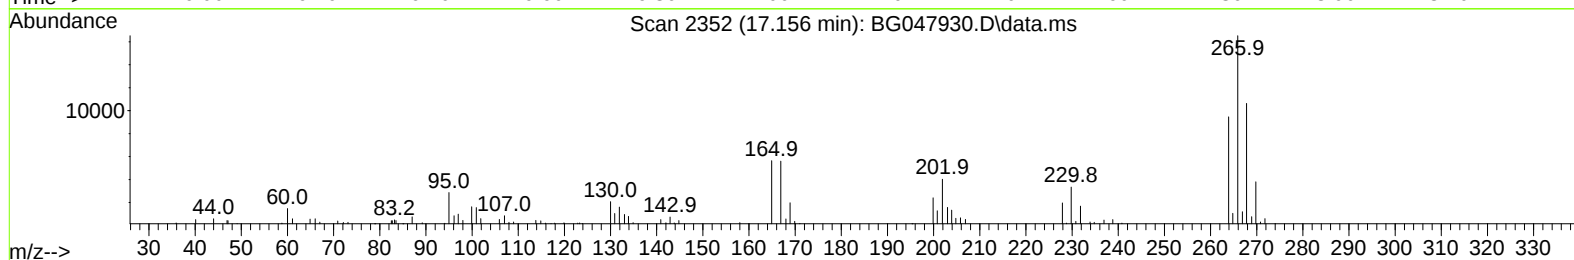


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012021\
Data File : BG047930.D
Acq On : 20 Jan 2021 9:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 00:43:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 16:06:10 2021
Response via : Initial Calibration

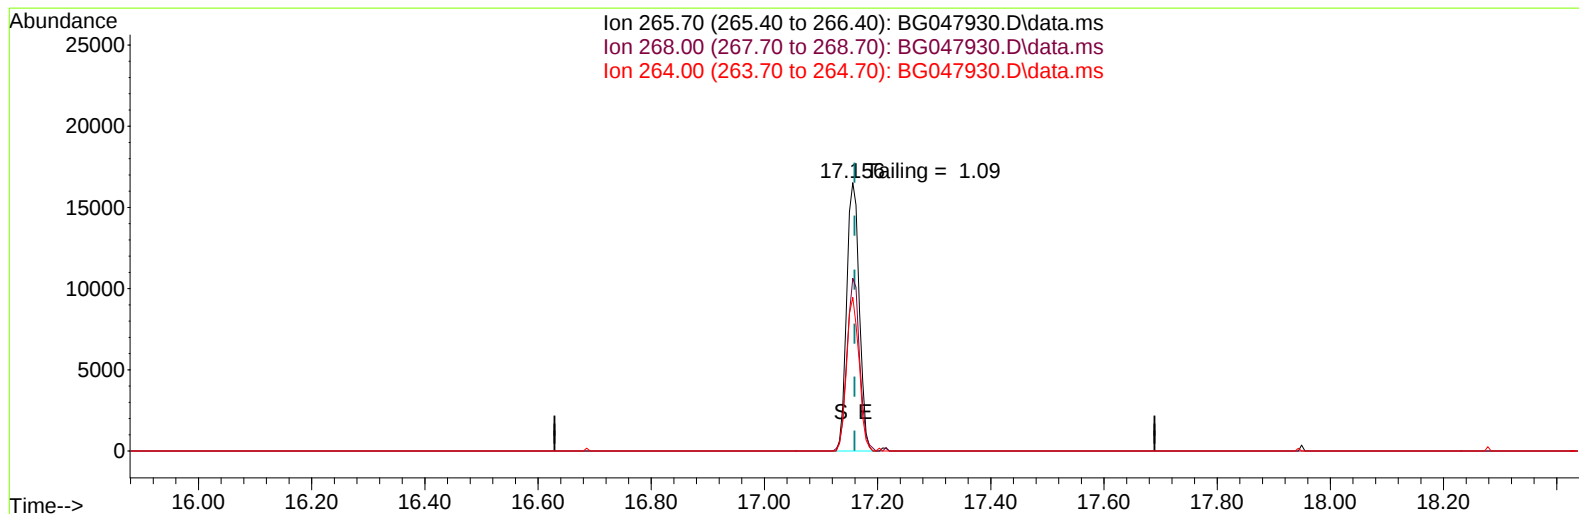

TIC: BG047930.D\data.ms

(70) Pentachlorophenol (C)




17.156min (-0.003) 24148.96 ng

response 25474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.31
264.00	61.60	57.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012021\
Data File : BG047930.D
Acq On : 20 Jan 2021 9:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 00:43:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 16:06:10 2021
Response via : Initial Calibration

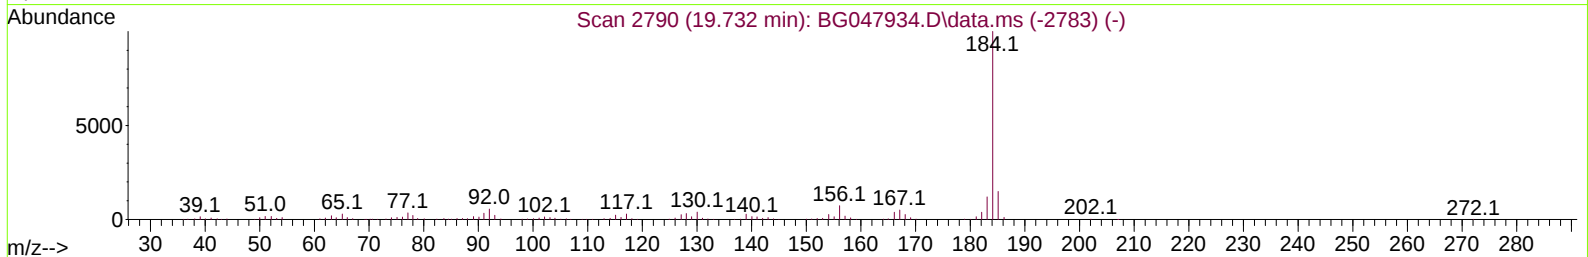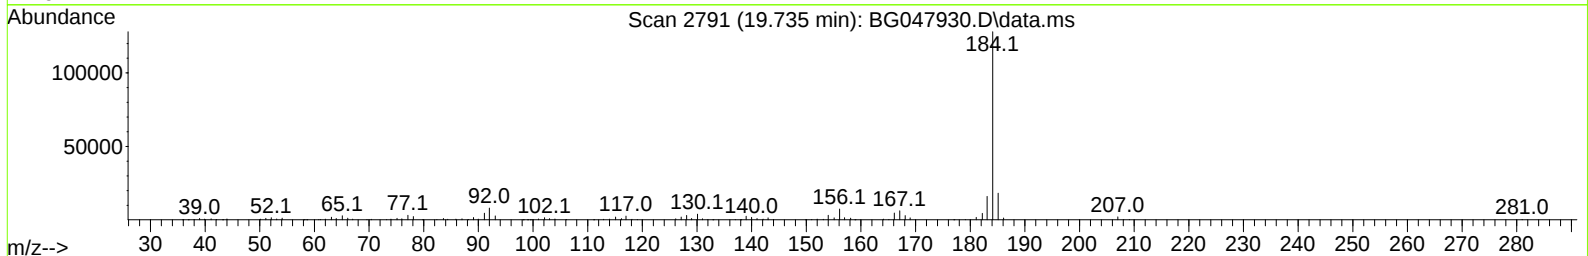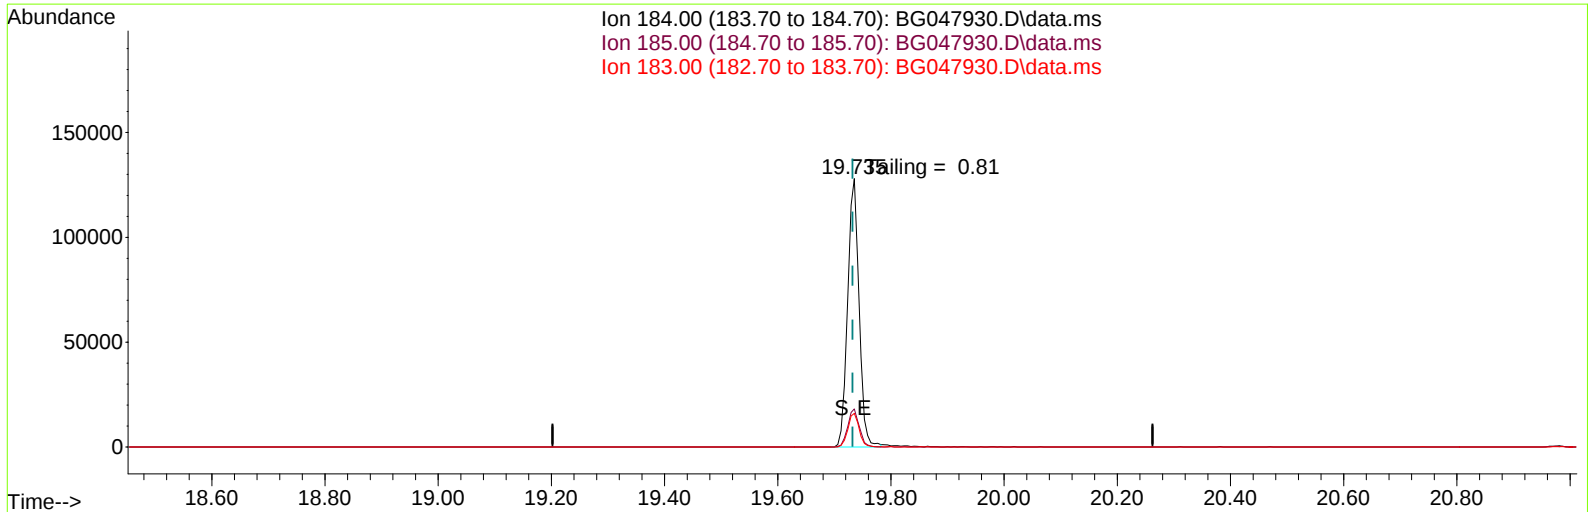

TIC: BG047930.D\data.ms

(77) Benzidine

19.735min (+ 0.003) 0.00 ng

response 181699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.22
183.00	13.20	12.53
0.00	0.00	0.00