

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012021\
 Data File : BG047940.D
 Acq On : 20 Jan 2021 16:53
 Operator : CG/JU
 Sample : M1160-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BASIN-4

Quant Time: Jan 20 17:29:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 20 16:06:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.149	152	44701	20.00	ng	0.00
21) Naphthalene-d8	10.963	136	170755	20.00	ng	# 0.00
39) Acenaphthene-d10	14.770	164	120945	20.00	ng	0.00
64) Phenanthrene-d10	17.514	188	305895	20.00	ng	0.00
76) Chrysene-d12	21.797	240	354350	20.00	ng	# 0.00
86) Perylene-d12	25.099	264	344730	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.704	112	275801	112.22	ng	0.00
7) Phenol-d6	7.291	99	382876	101.93	ng	0.00
23) Nitrobenzene-d5	9.312	82	246698	70.89	ng	0.00
42) 2,4,6-Tribromophenol	16.251	330	165570	103.08	ng	0.00
45) 2-Fluorobiphenyl	13.401	172	551728	60.72	ng	0.00
79) Terphenyl-d14	20.117	244	1015678	52.86	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.218	163	45136	5.00	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012021\
Data File : BG047940.D
Acq On : 20 Jan 2021 16:53
Operator : CG/JU
Sample : M1160-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BASIN-4

Quant Time: Jan 20 17:29:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 16:06:10 2021
Response via : Initial Calibration




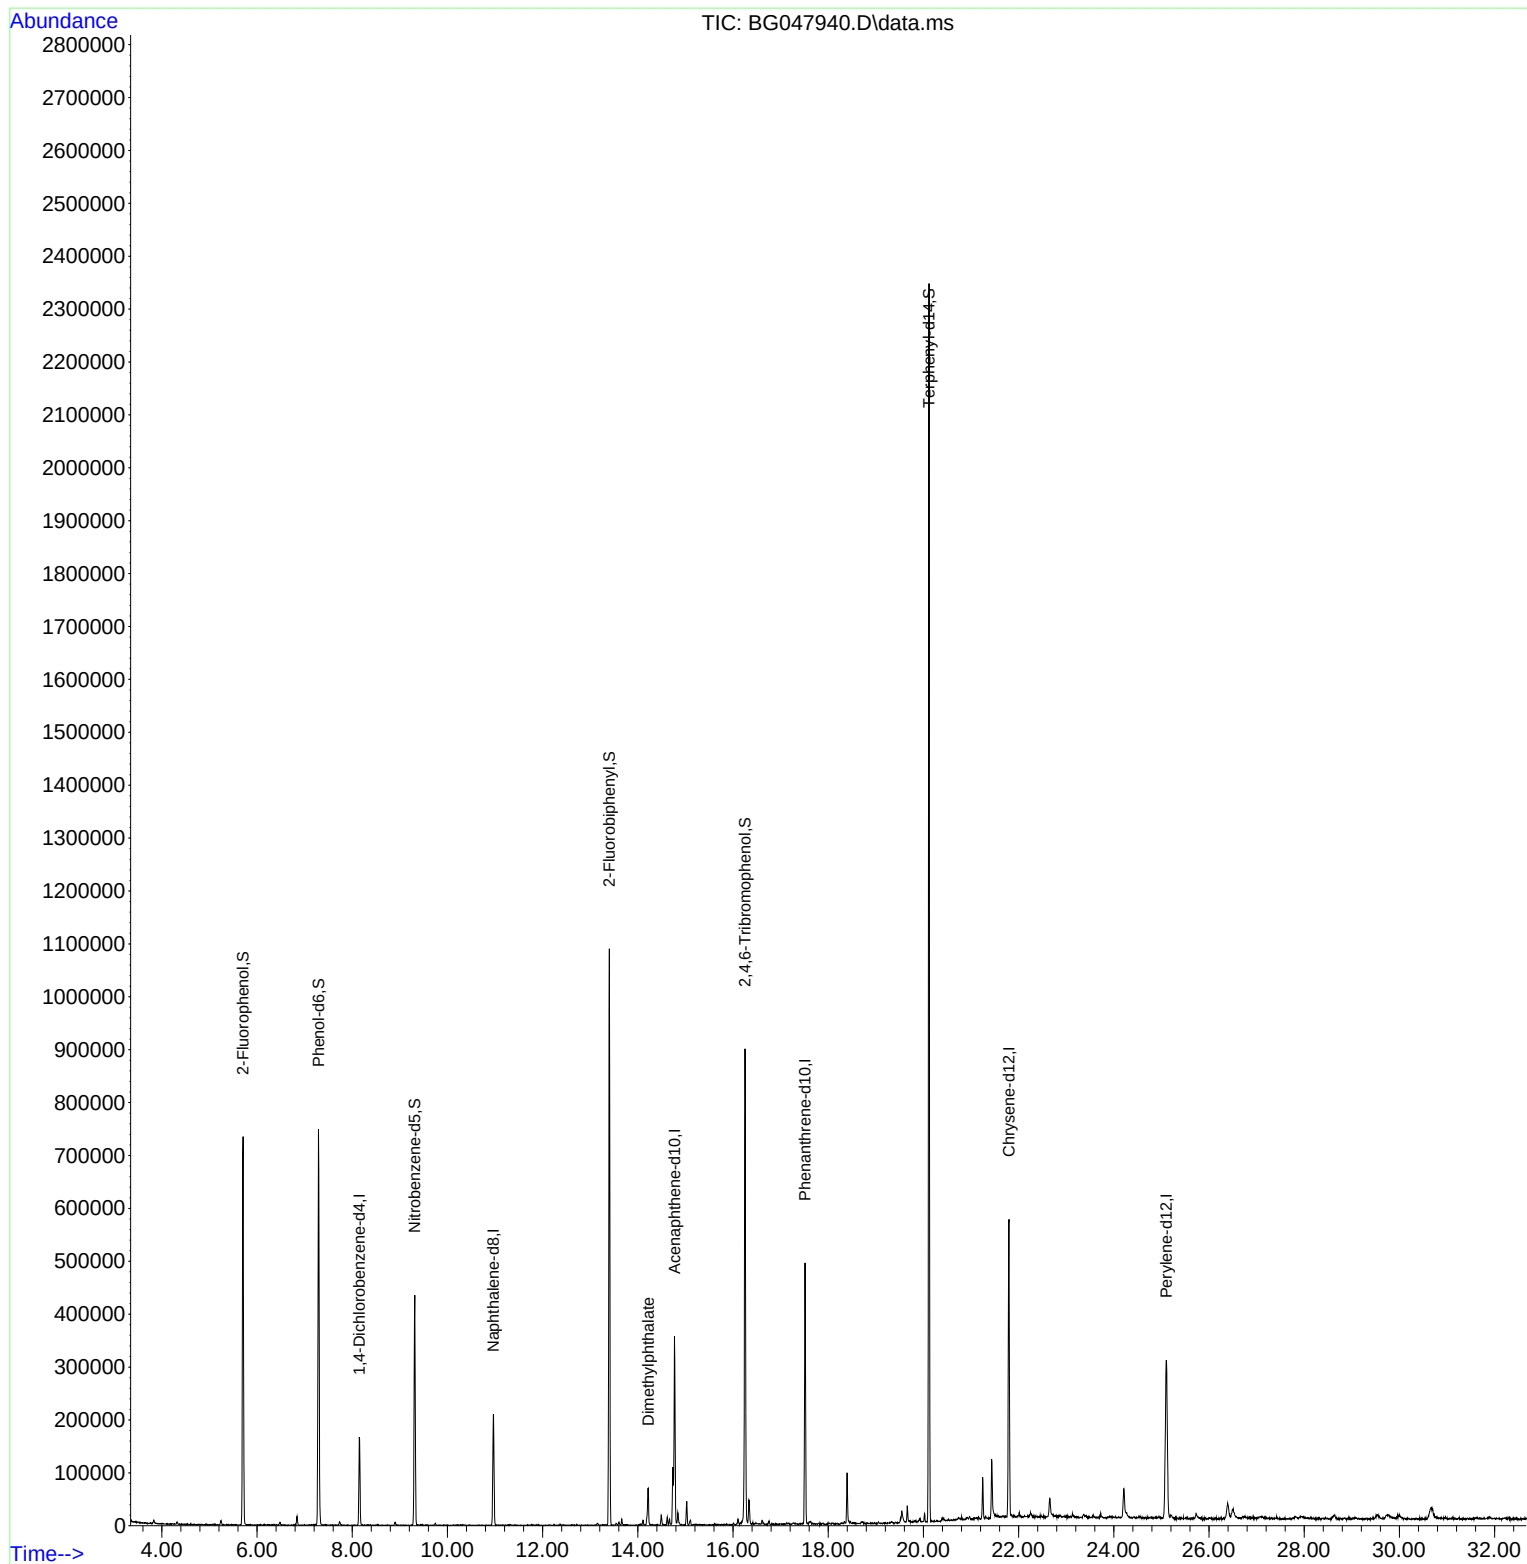




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.149 min Scan# 819
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53




Instrument :
BNA_G
ClientSampleId :
BASIN-4


Tgt Ion:152 Resp: 44701
Ion Ratio Lower Upper
152 100
150 144.7 125.0 187.6
115 49.5 41.8 62.6

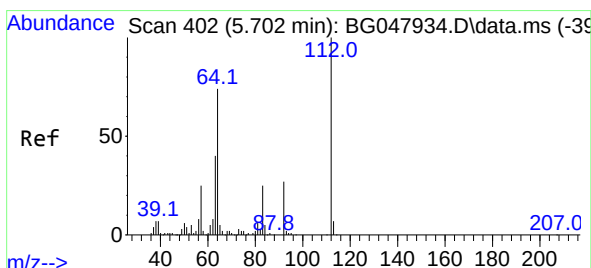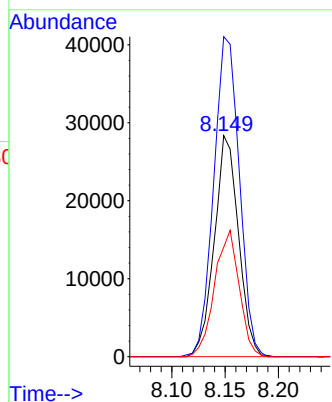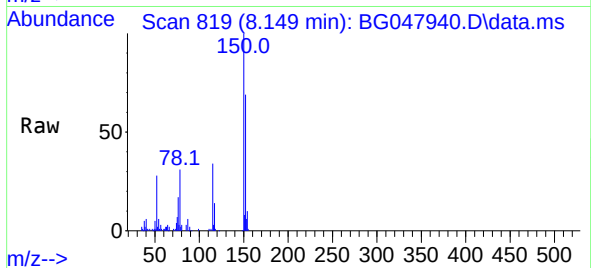

#5
2-Fluorophenol
Concen: 112.22 ng
RT: 5.704 min Scan# 403
Delta R.T. 0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion:112 Resp: 275801
Ion Ratio Lower Upper
112 100
64 77.5 46.7 70.1#
63 41.0 22.8 34.2#

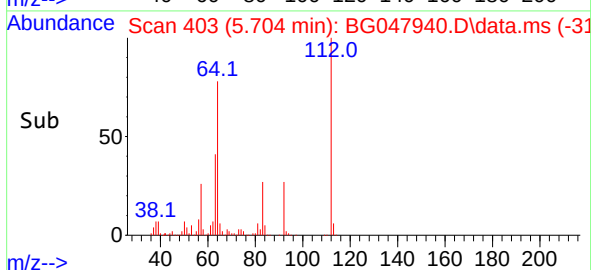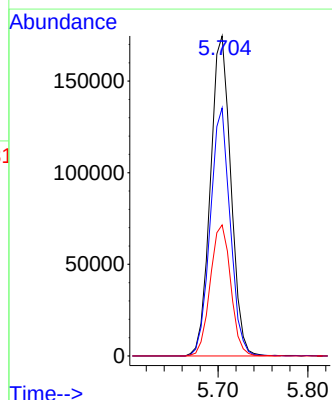




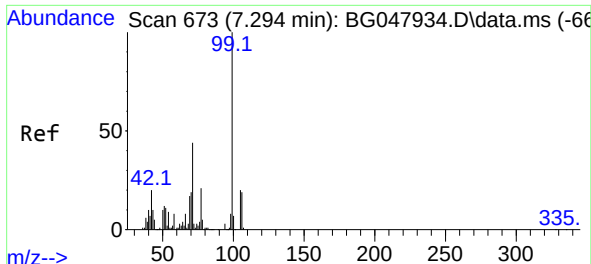


#7
Phenol-d6
Concen: 101.93 ng
RT: 7.291 min Scan# 673
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Instrument :
BNA_G
ClientSampleId :
BASIN-4

Tgt Ion: 99 Resp: 382876




Ion	Ratio	Lower	Upper
99	100		
42	22.8	12.8	19.2#
71	42.7	24.6	36.8#

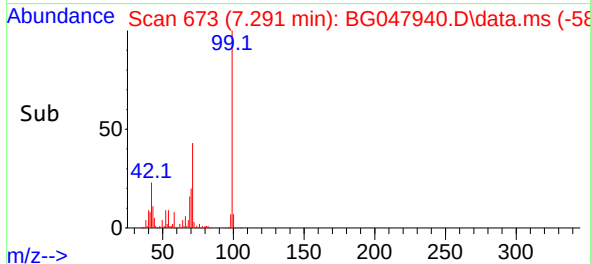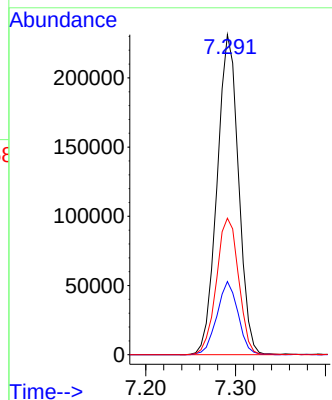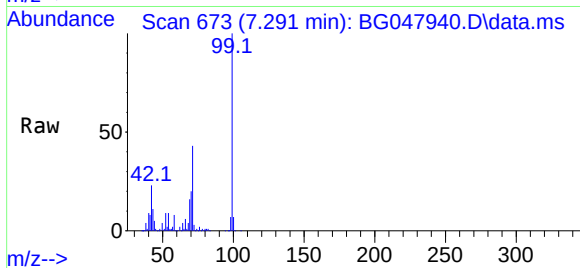


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.963 min Scan# 1298
Delta R.T. -0.009 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion: 136 Resp: 170755

Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.1	13.7
54	10.2	6.2	9.4#
68	5.3	5.0	7.4


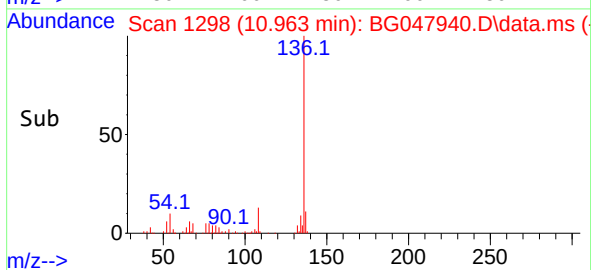
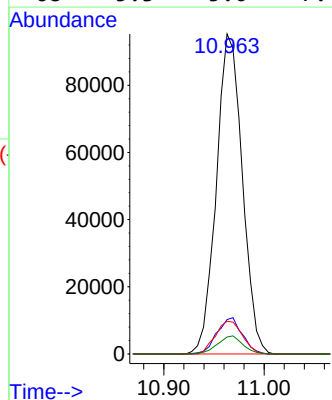
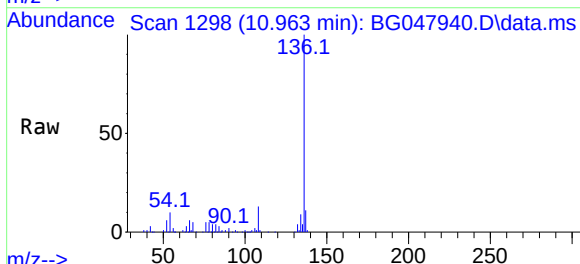




#23
Nitrobenzene-d5
Concen: 70.89 ng
RT: 9.312 min Scan# 1017
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53




Instrument :
BNA_G
ClientSampleId :
BASIN-4


Tgt Ion: 82 Resp: 246698
Ion Ratio Lower Upper
82 100
128 35.3 37.0 55.6#
54 57.1 39.0 58.4

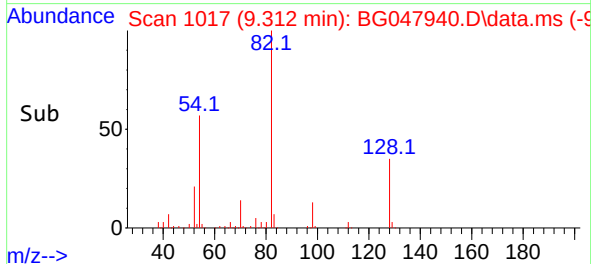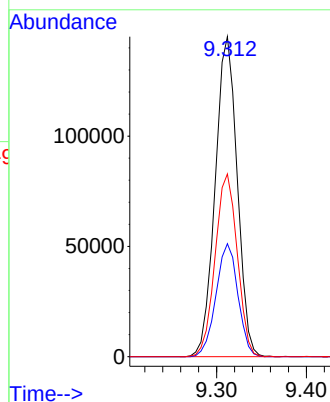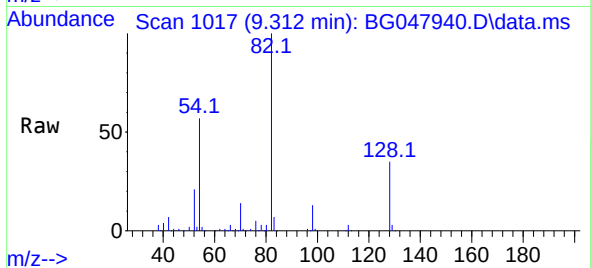

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.770 min Scan# 1946
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion:164 Resp: 120945
Ion Ratio Lower Upper
164 100
162 101.8 82.3 123.5
160 44.1 35.3 52.9


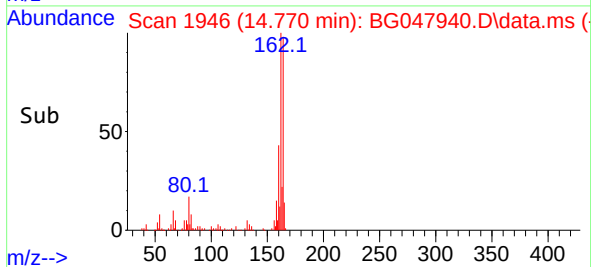
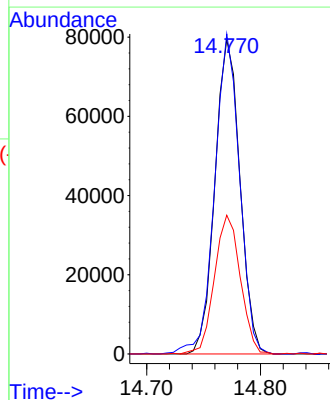
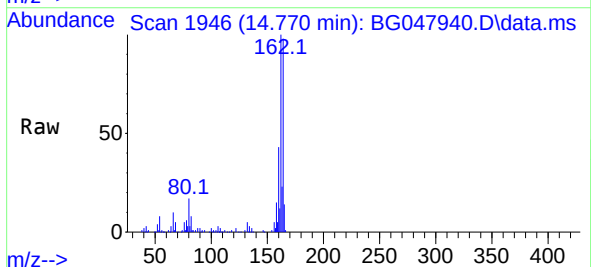




#42
2,4,6-Tribromophenol
Concen: 103.08 ng
RT: 16.251 min Scan# 2198
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53




Instrument :
BNA_G
ClientSampleId :
BASIN-4


Tgt Ion:330 Resp: 165570
Ion Ratio Lower Upper
330 100
332 97.2 76.5 114.7
141 33.7 26.0 39.0

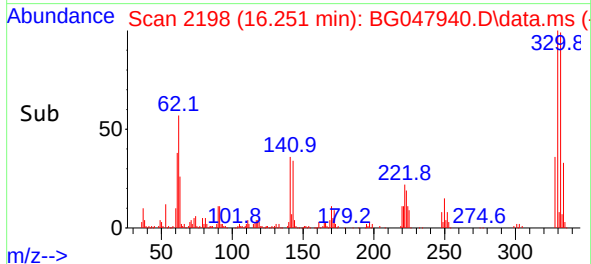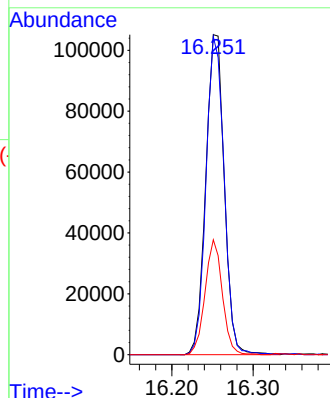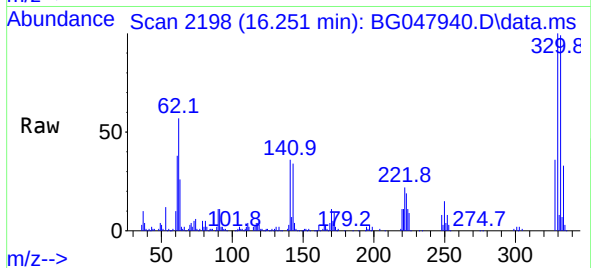

#45
2-Fluorobiphenyl
Concen: 60.72 ng
RT: 13.401 min Scan# 1713
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion:172 Resp: 551728
Ion Ratio Lower Upper
172 100
171 36.2 31.3 46.9
170 23.3 20.8 31.2


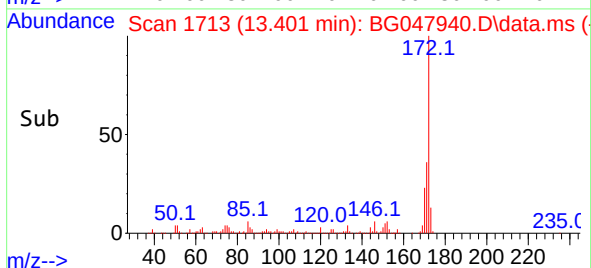
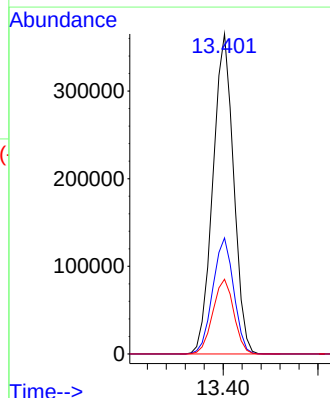
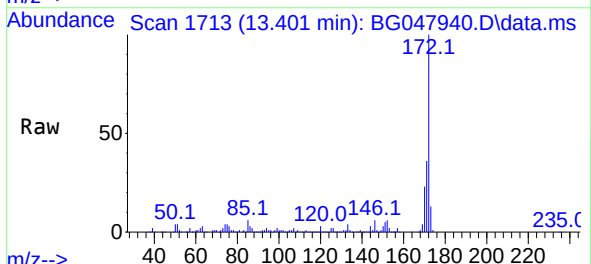




#50
Dimethylphthalate
Concen: 5.00 ng
RT: 14.218 min Scan# 1852
Delta R.T. -0.009 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53




Instrument :
BNA_G
ClientSampleId :
BASIN-4


Tgt Ion:163	Resp:	45136
Ion Ratio	Lower	Upper
163	100	
194	4.6	3.8 5.8
164	9.1	8.8 13.2

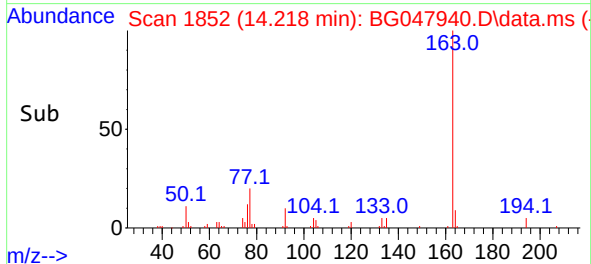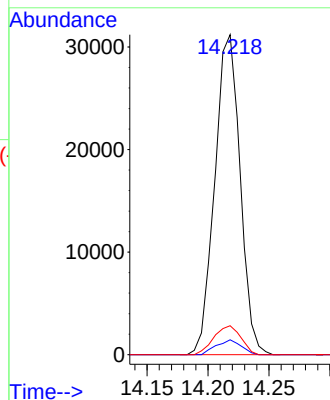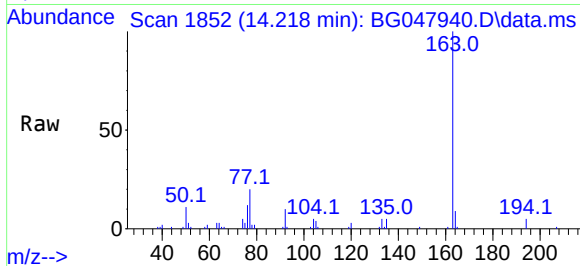

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.514 min Scan# 2413
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion:188	Resp:	305895
Ion Ratio	Lower	Upper
188	100	
94	6.6	6.3 9.5
80	7.2	7.0 10.6


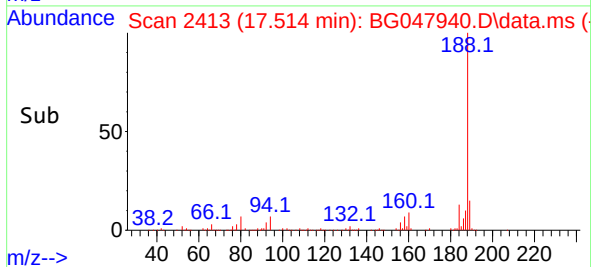
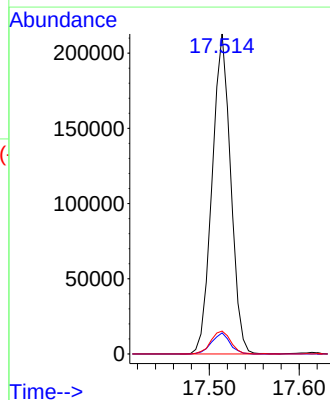
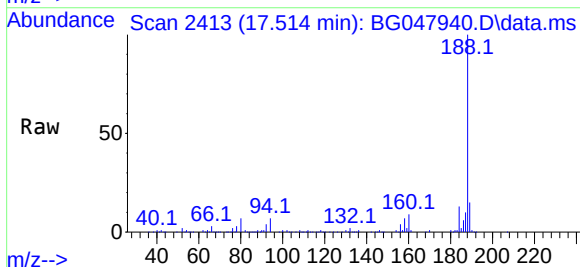




#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.797 min Scan# 3142
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53




Instrument :
BNA_G
ClientSampleId :
BASIN-4


Tgt Ion:240 Resp: 354350
Ion Ratio Lower Upper
240 100
120 5.3 6.2 9.4#
236 26.1 20.5 30.7

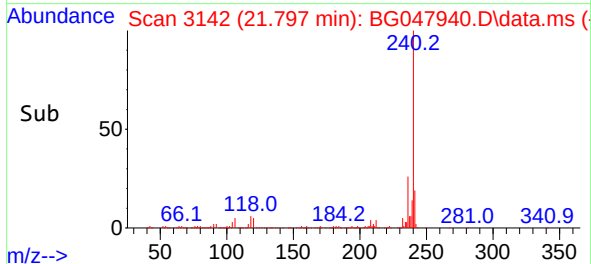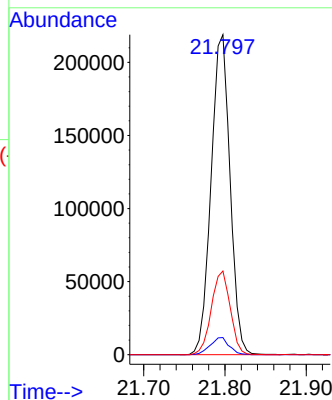

#79
Terphenyl-d14
Concen: 52.86 ng
RT: 20.117 min Scan# 2856
Delta R.T. -0.003 min
Lab File: BG047940.D
Acq: 20 Jan 2021 16:53

Tgt Ion:244 Resp: 1015678
Ion Ratio Lower Upper
244 100
212 7.6 6.7 10.1
122 6.9 7.8 11.6#

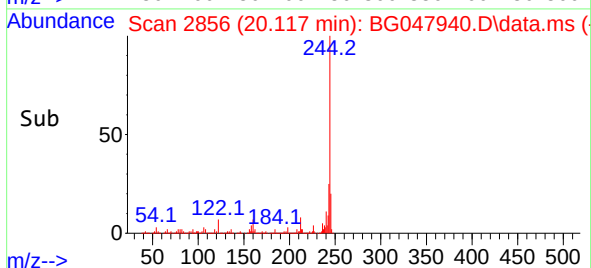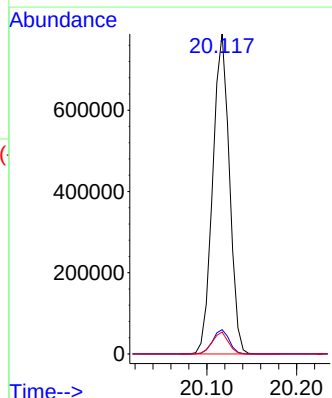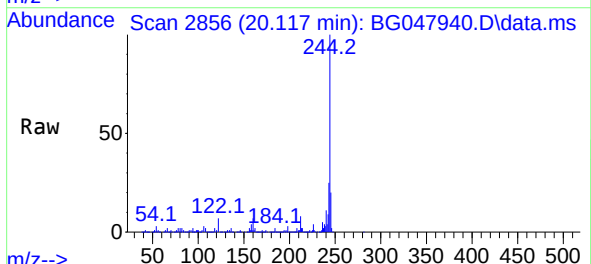

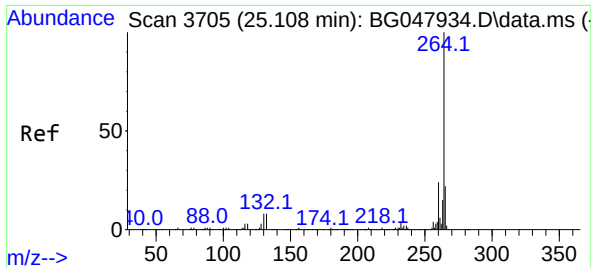

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.099 min Scan# 3704
 Delta R.T. -0.009 min
 Lab File: BG047940.D
 Acq: 20 Jan 2021 16:53

Instrument :
 BNA_G
 ClientSampleId :
 BASIN-4

Tgt Ion:264 Resp: 344730
 Ion Ratio Lower Upper
 264 100
 260 24.7 18.8 28.2
 265 21.6 17.8 26.8

