


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012021\
 Data File : BG047930.D
 Acq On : 20 Jan 2021 9:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 21 10:00:28 2021

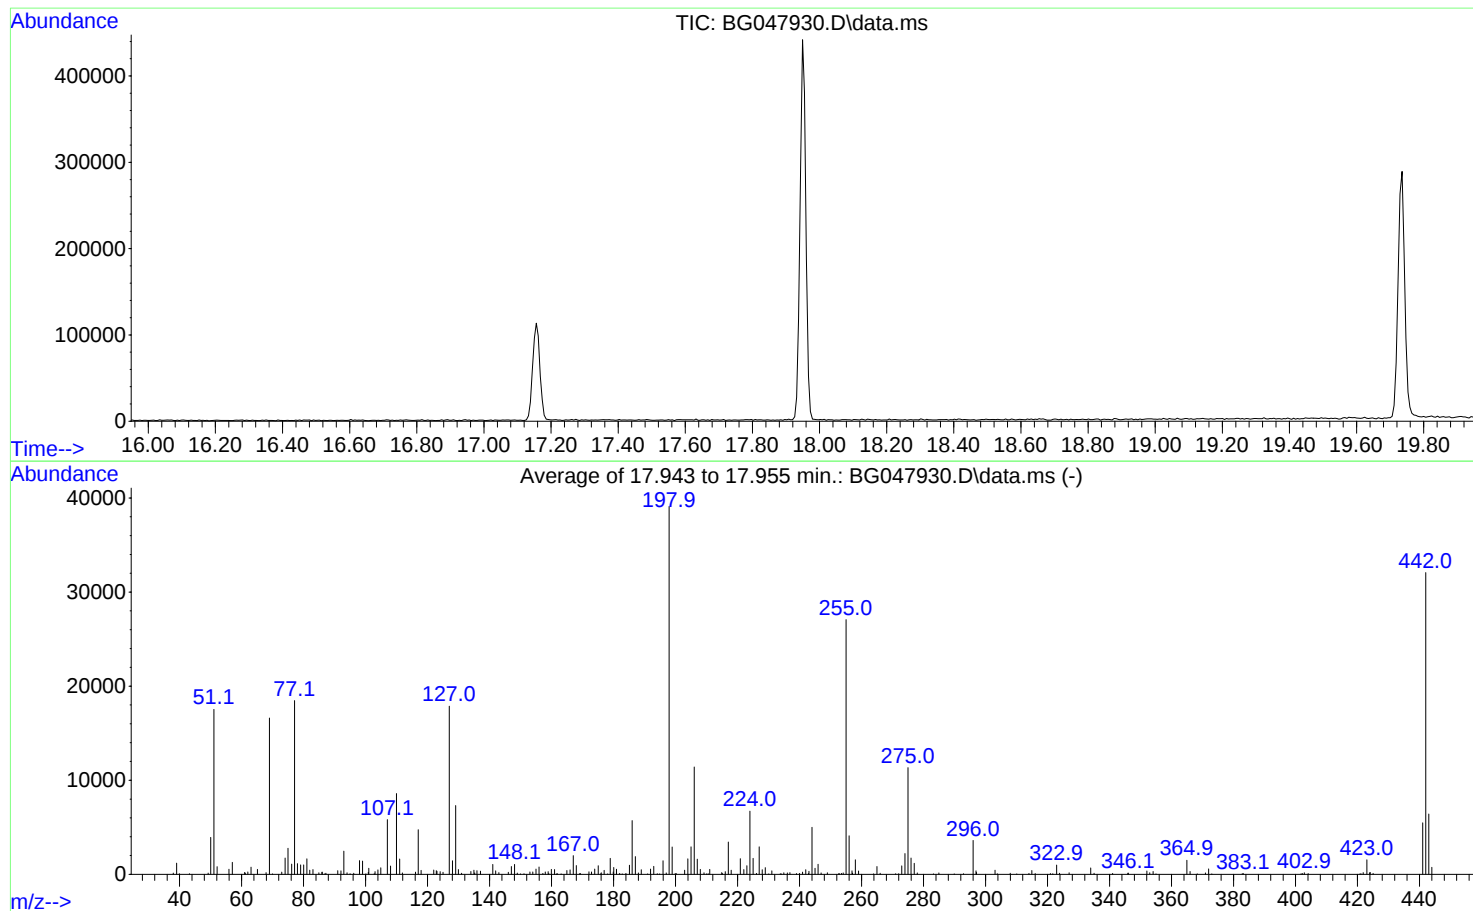

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	17536	PASS
68	69	0.00	2	1.1	184	PASS
69	198	0.00	100	42.5	16617	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	45.7	17867	PASS
197	198	0.00	2	0.4	148	PASS
198	198	100	100	100.0	39093	PASS
199	198	5	9	7.4	2905	PASS
275	198	10	60	29.0	11343	PASS
365	198	1	100	3.8	1495	PASS
441	198	0.01	100	14.0	5470	PASS
442	198	50	100	82.0	32064	PASS
443	442	15	24	20.0	6416	PASS