


Data Path : Z:\HPCHEM1\BNA G\Data\BG012115\  
 Data File : BG015906.D  
 Acq On : 21 Jan 2015 15:38  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG012015.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jan 20 17:47:40 2015

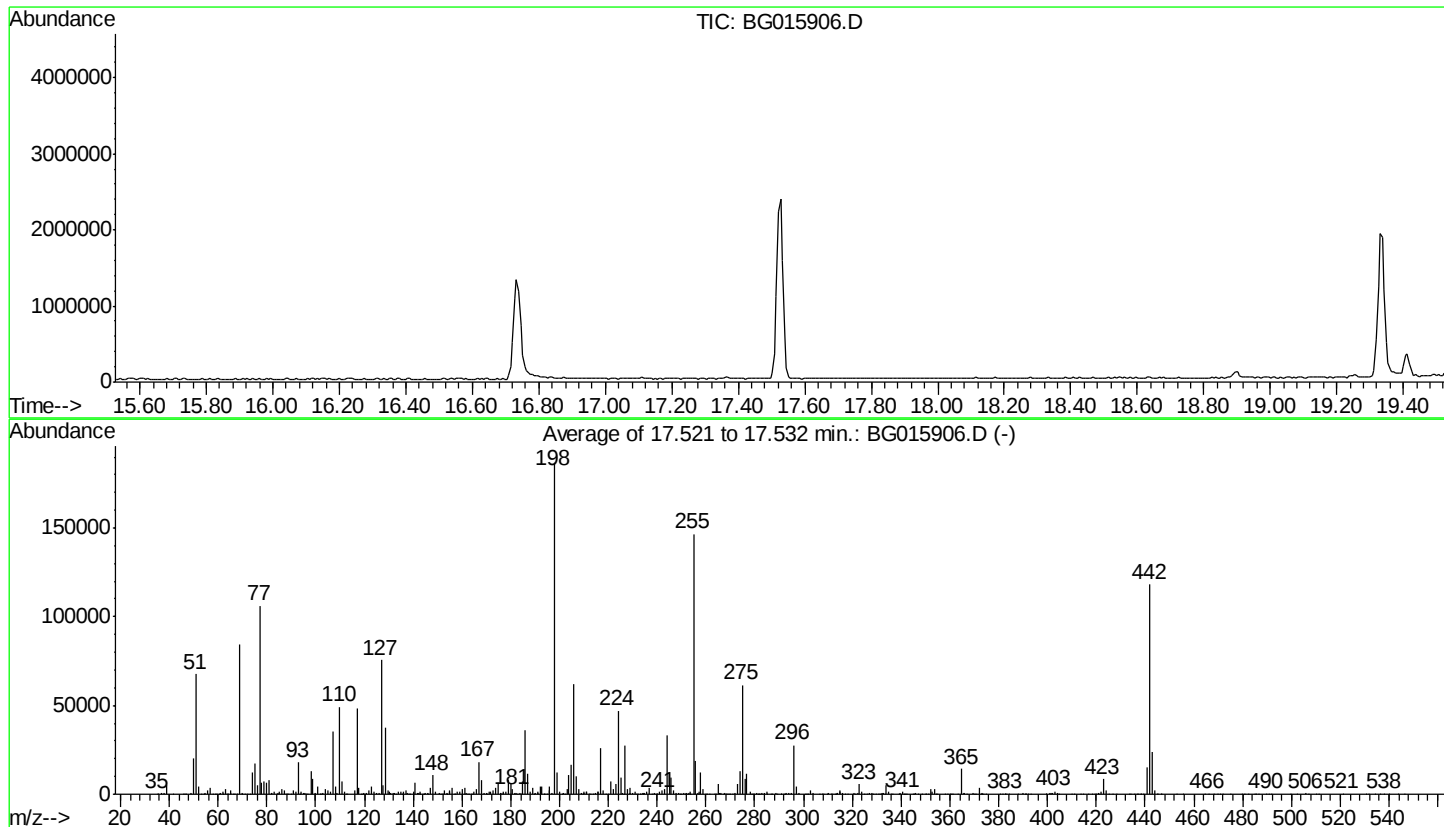

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.2      | 67704   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 4       | PASS             |
| 69          | 198          | 0.00         | 100          | 45.2      | 84488   | PASS             |
| 70          | 69           | 0.00         | 2            | 1.1       | 913     | PASS             |
| 127         | 198          | 10           | 80           | 40.4      | 75504   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 1022    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 186773  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 12540   | PASS             |
| 275         | 198          | 10           | 60           | 32.9      | 61392   | PASS             |
| 365         | 198          | 1            | 100          | 7.6       | 14273   | PASS             |
| 441         | 442          | 0.01         | 24           | 12.8      | 15128   | PASS             |
| 442         | 198          | 50           | 100          | 63.2      | 118128  | PASS             |
| 443         | 442          | 15           | 24           | 20.4      | 24096   | PASS             |