
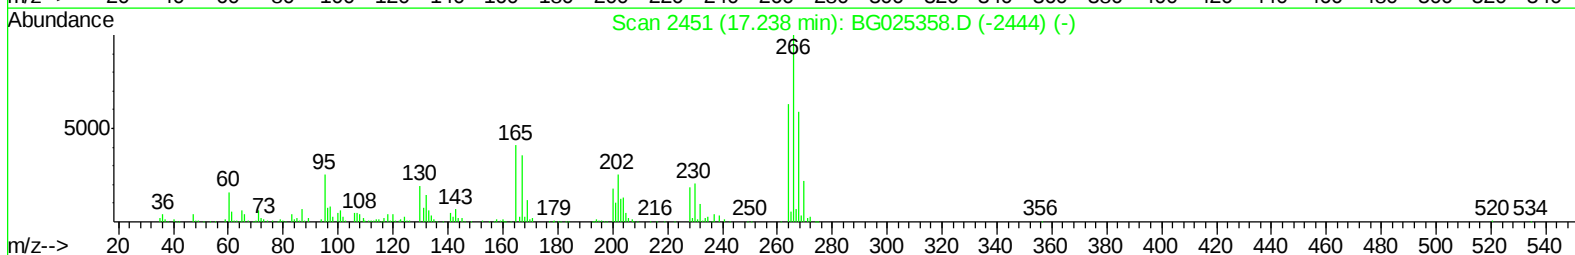
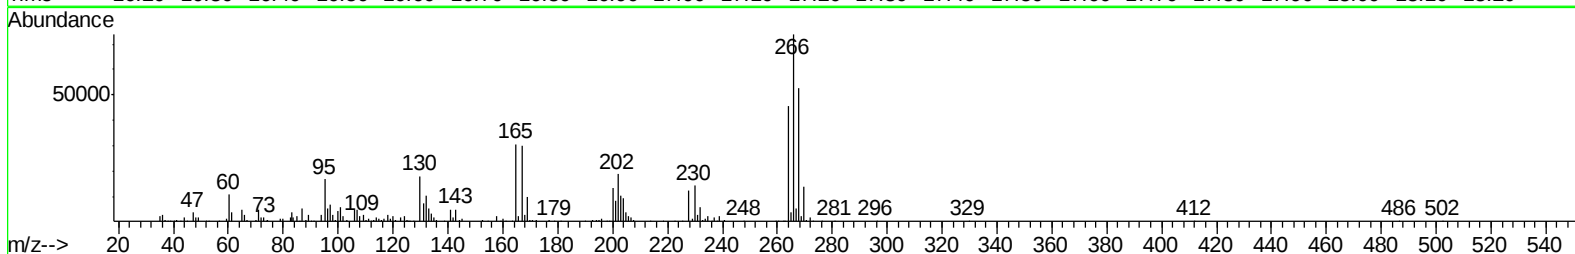


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012117\
Data File : BG025567.D
Acq On : 21 Jan 2017 10:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 08:01:47 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

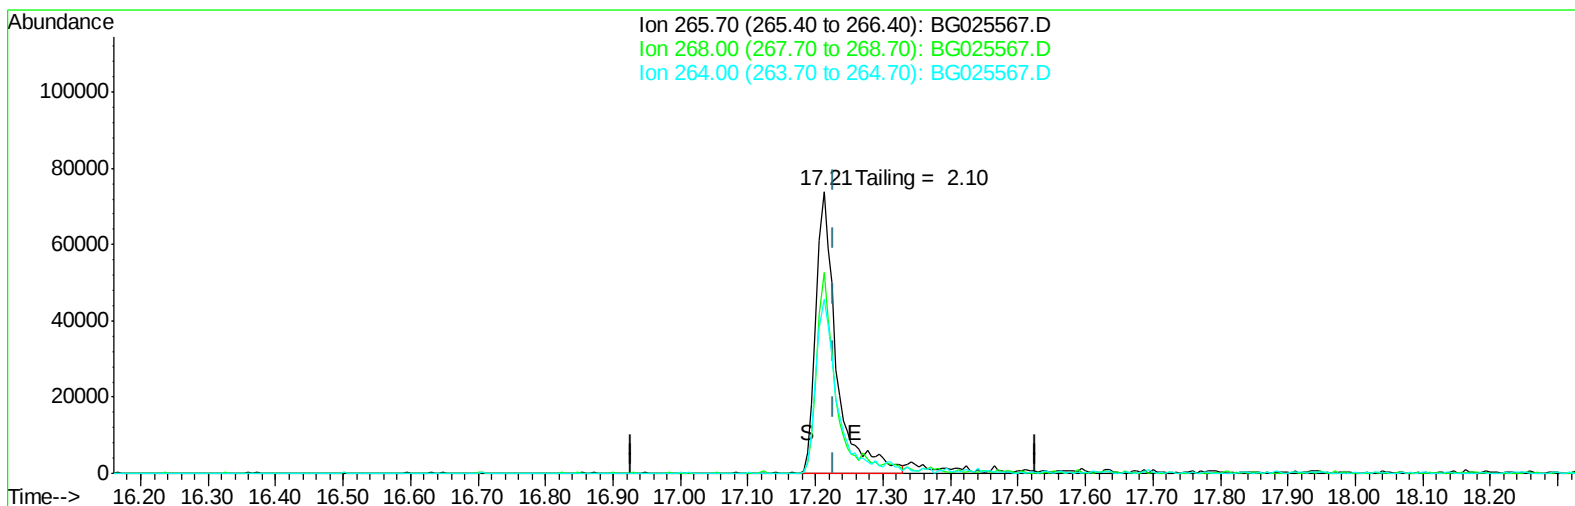

TIC: BG025567.D

(69) Pentachlorophenol (C)




17.212min (-0.016) 241039.21ng

response 155677

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	71.23
264.00	62.60	61.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG012117\
Data File : BG025567.D
Acq On : 21 Jan 2017 10:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 08:01:47 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

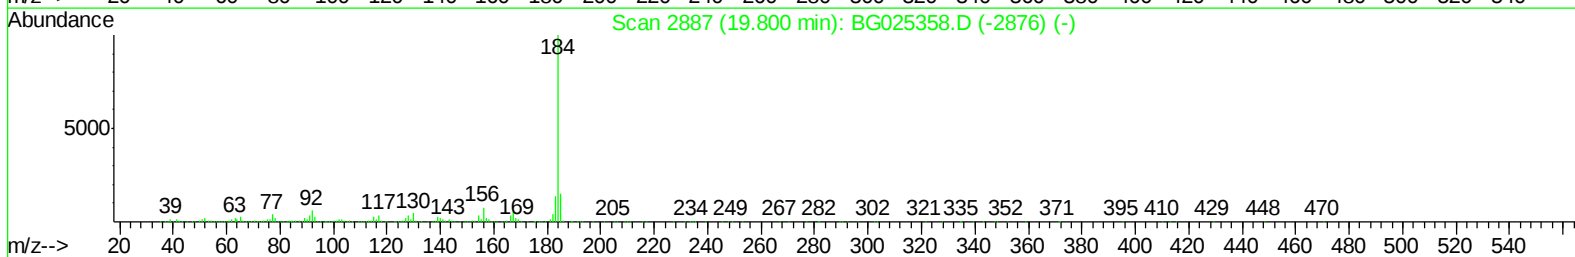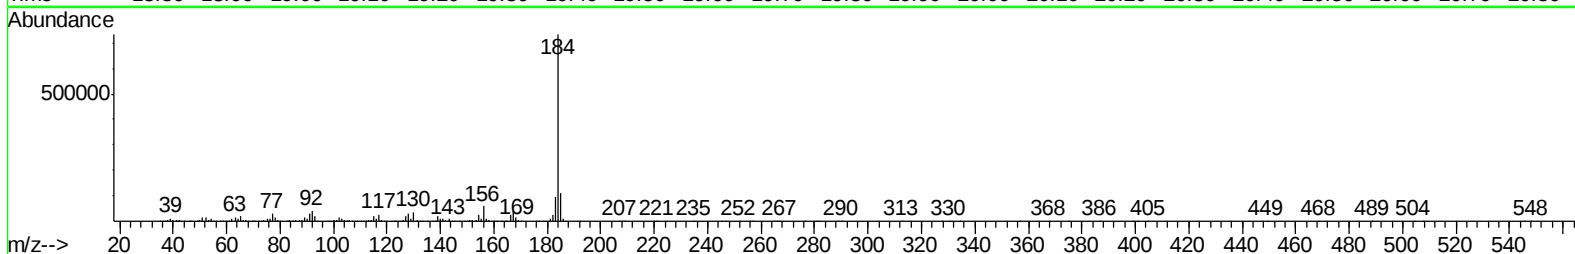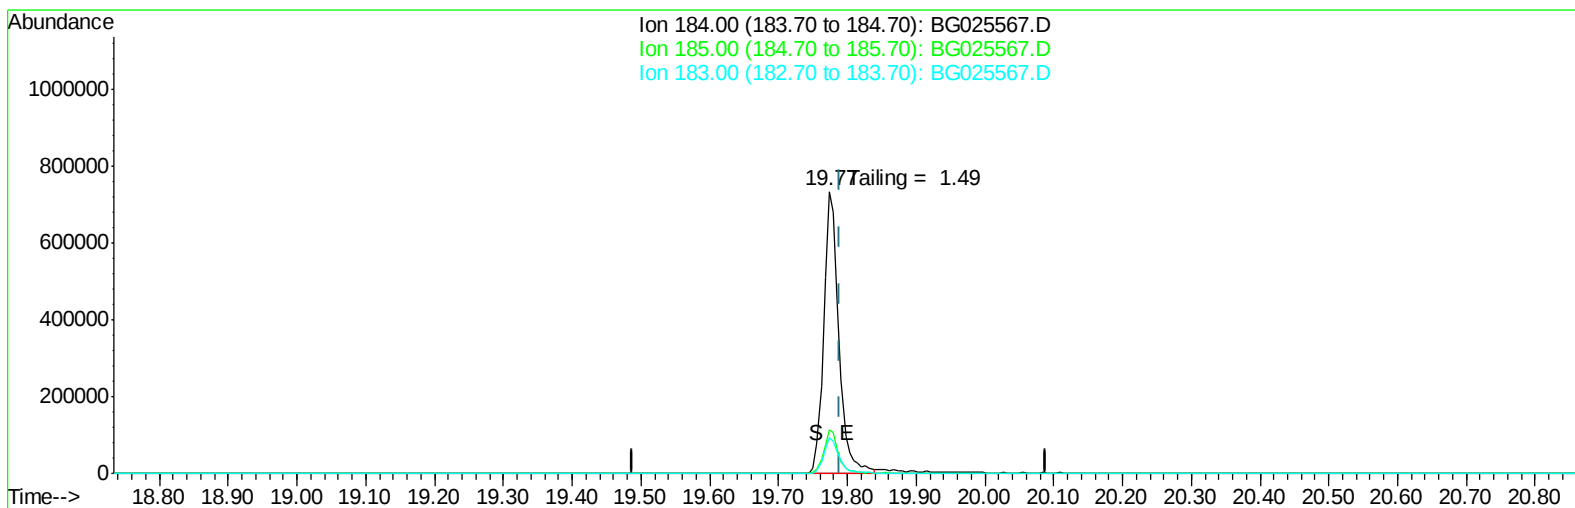

TIC: BG025567.D

(76) Benzidine

19.774min (-0.016) 463504.11ng

response 1144630

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.31
183.00	13.80	12.96
0.00	0.00	0.00