


Data Path : Z:\HPCHEM1\BNA G\DATA\BG012117\
 Data File : BG025567.D
 Acq On : 21 Jan 2017 10:43
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 10 11:26:22 2017

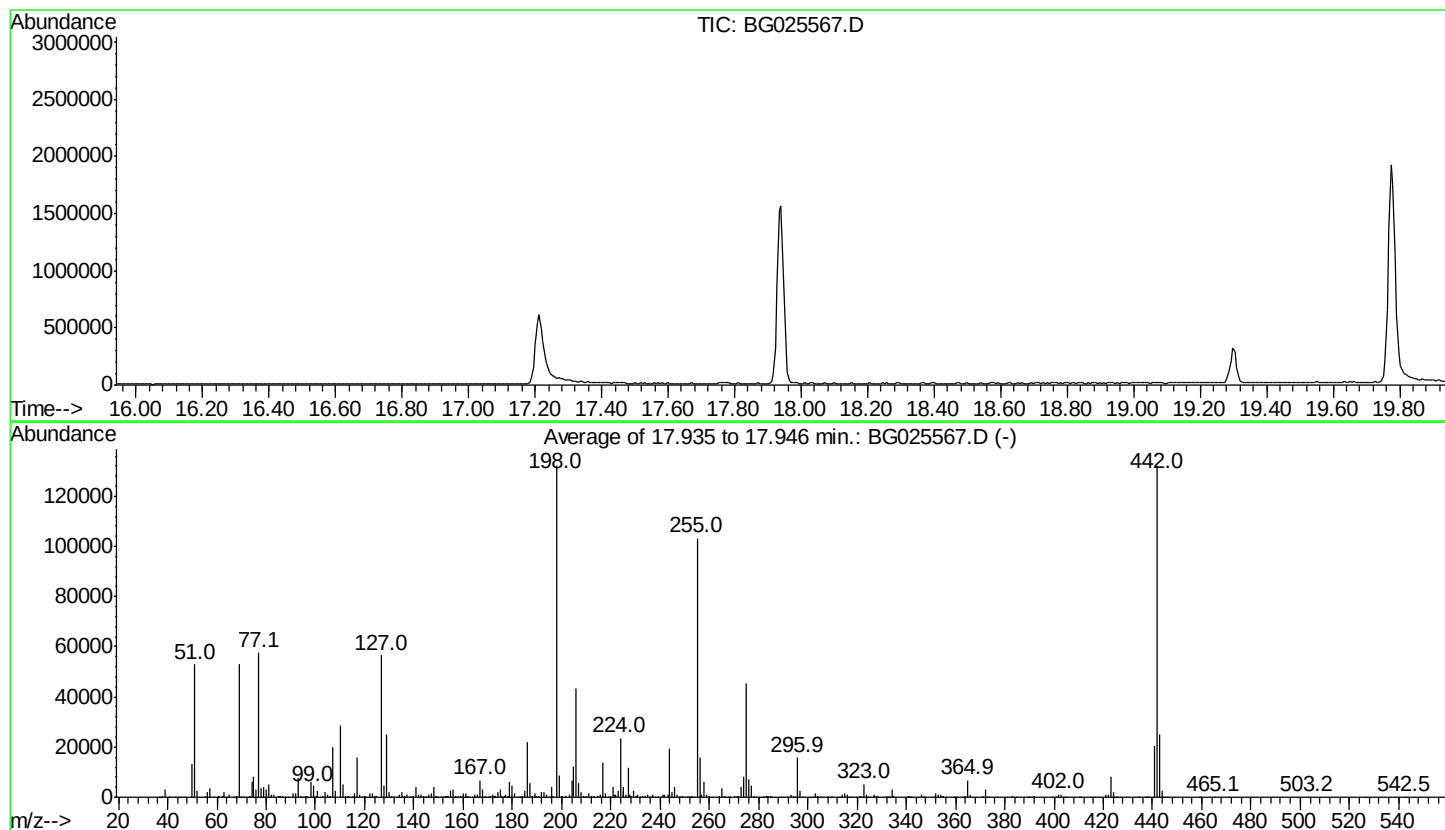

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	52918	PASS
68	69	0.00	2	1.0	555	PASS
69	198	0.00	100	40.3	53226	PASS
70	69	0.00	2	0.5	241	PASS
127	198	10	80	42.7	56472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132213	PASS
199	198	5	9	6.6	8671	PASS
275	198	10	60	34.5	45552	PASS
365	198	1	100	5.0	6658	PASS
441	442	0.01	24	15.4	20392	PASS
442	198	50	100	100.0	132152	PASS
443	442	15	24	19.0	25157	PASS