
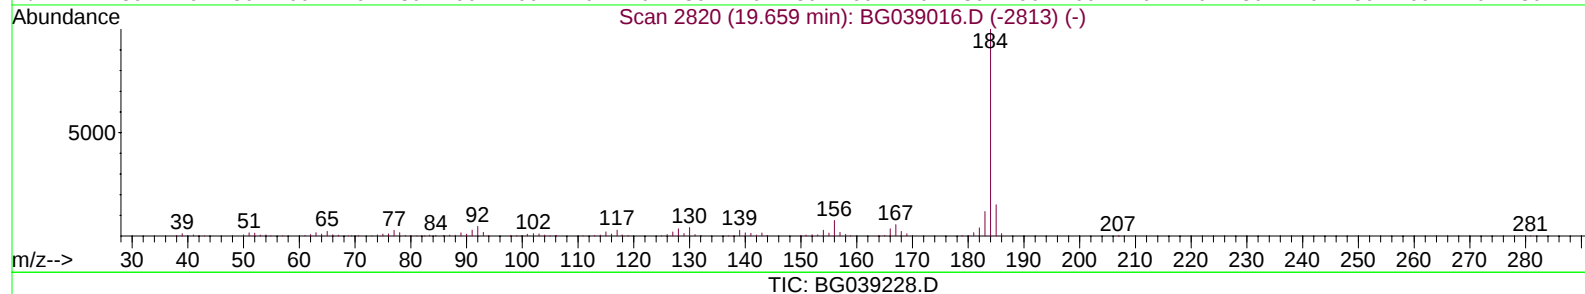
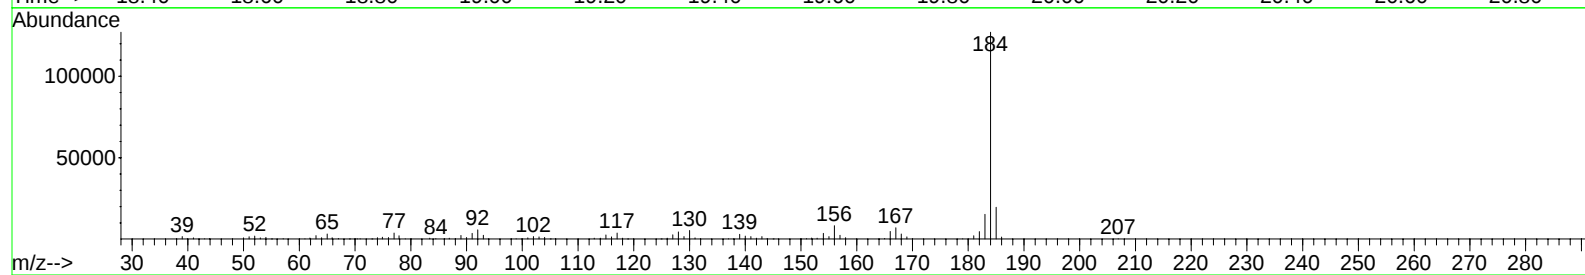


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012119\
Data File : BG039228.D
Acq On : 21 Jan 2019 11:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 17:07:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

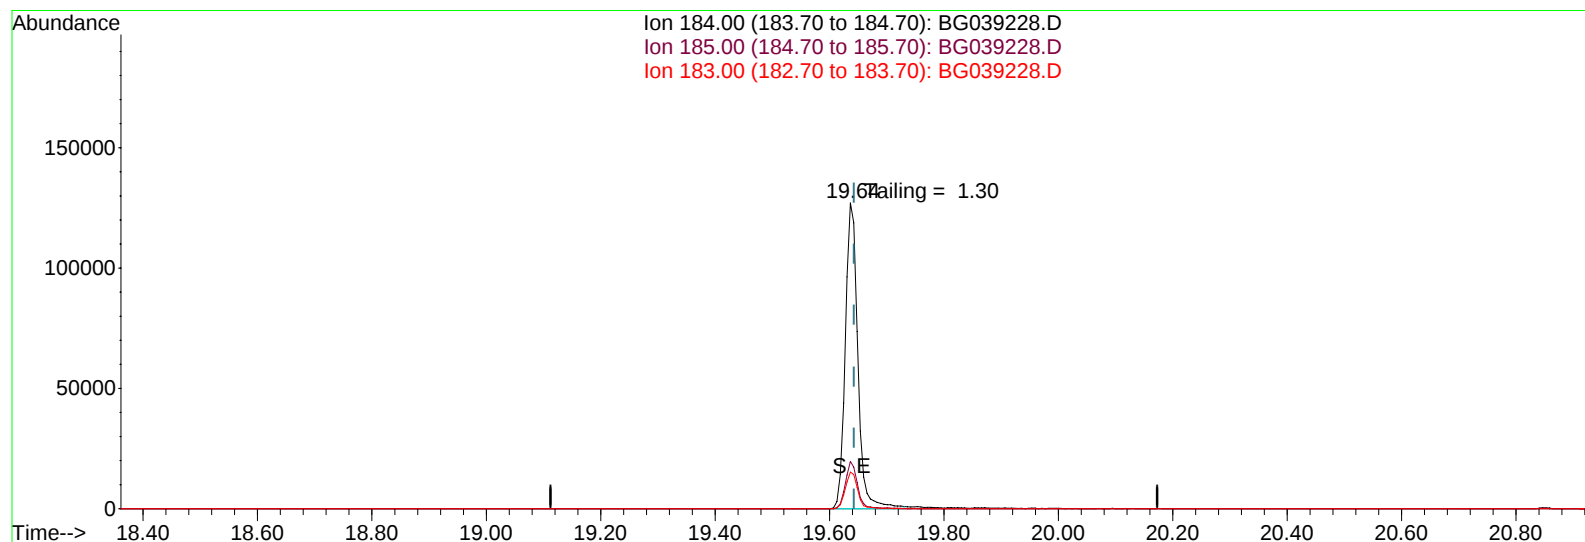

(77) Benzidine




19.636min (-0.006) 0.00ng

response 194857

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.47
183.00	11.90	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012119\
Data File : BG039228.D
Acq On : 21 Jan 2019 11:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 17:07:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

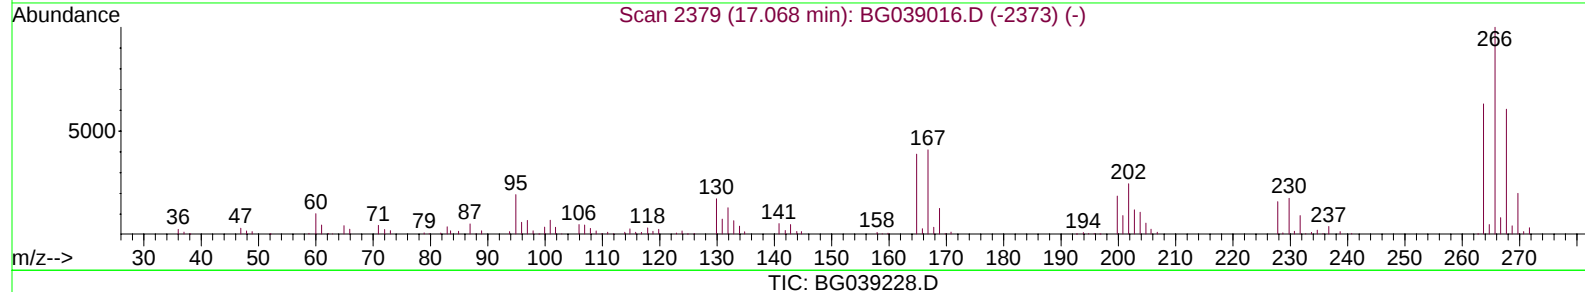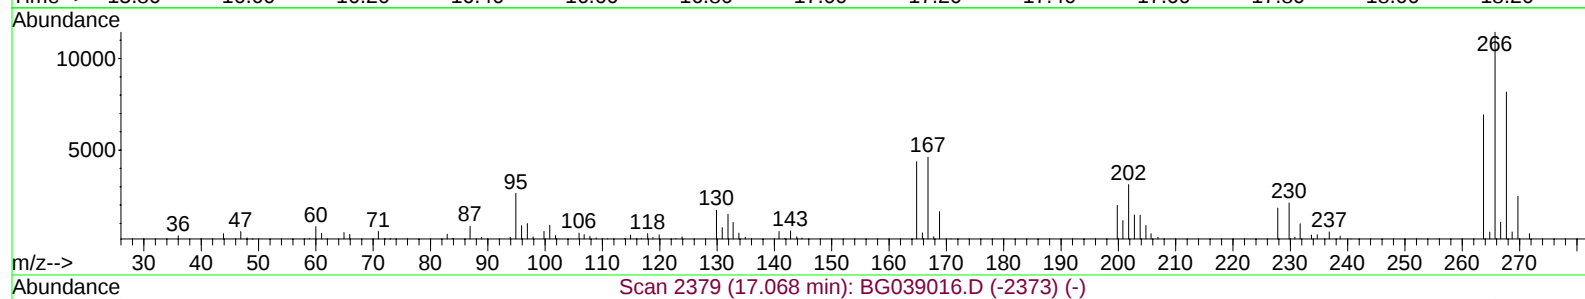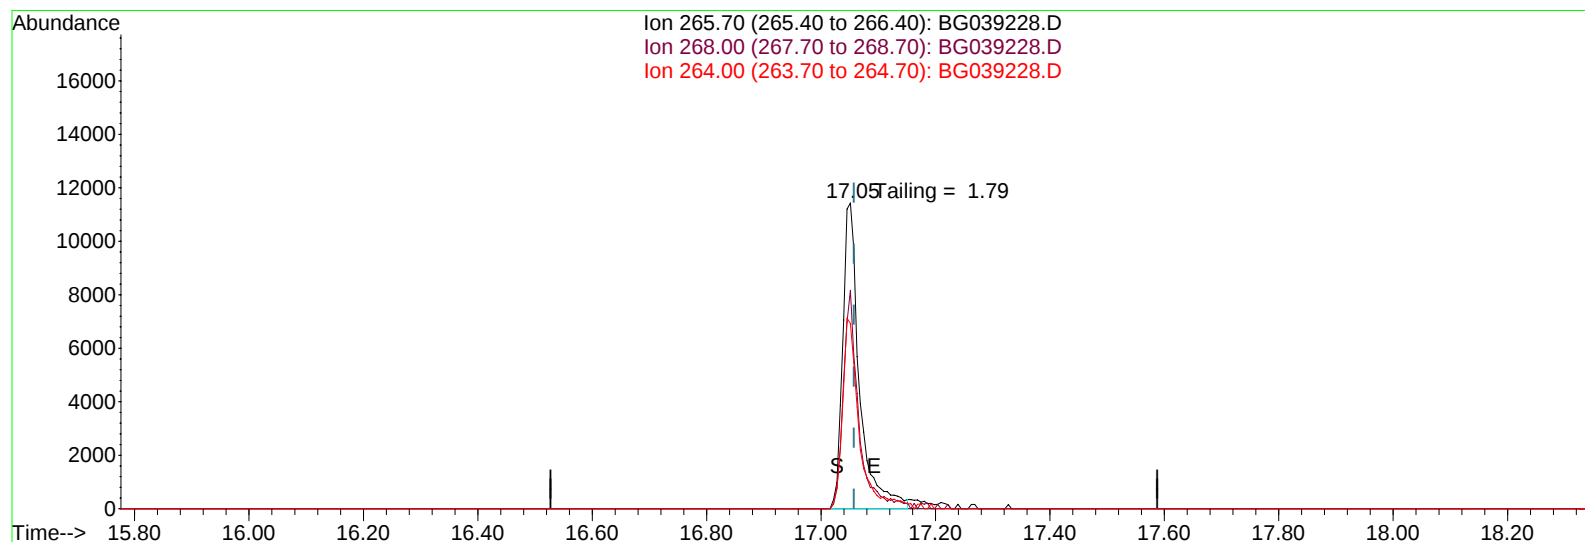

(70) Pentachlorophenol (C)

17.051min (-0.006) 45250.14ng

response 23674

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	76.15
264.00	68.20	60.58
0.00	0.00	0.00