

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012119\
 Data File : BG039242.D
 Acq On : 21 Jan 2019 20:38
 Operator : JU/SJ
 Sample : K1009-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-011819-A

Quant Time: Jan 22 00:17:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	14987	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	59416	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	45383	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	114138	20.00	ng	0.00
76) Chrysene-d12	21.67	240	119347	20.00	ng	-0.01
87) Perylene-d12	24.93	264	127235	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	101637	128.65	ng	0.00
7) Phenol-d6	7.17	99	122454	107.70	ng	0.00
23) Nitrobenzene-d5	9.19	82	100126	92.21	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	97475	128.13	ng	0.00
45) 2-Fluorobiphenyl	13.27	172	285126	85.98	ng	0.00
79) Terphenyl-d14	20.00	244	583755	90.48	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012119\
Data File : BG039242.D
Acq On : 21 Jan 2019 20:38
Operator : JU/SJ
Sample : K1009-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-01-011819-A

Quant Time: Jan 22 00:17:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

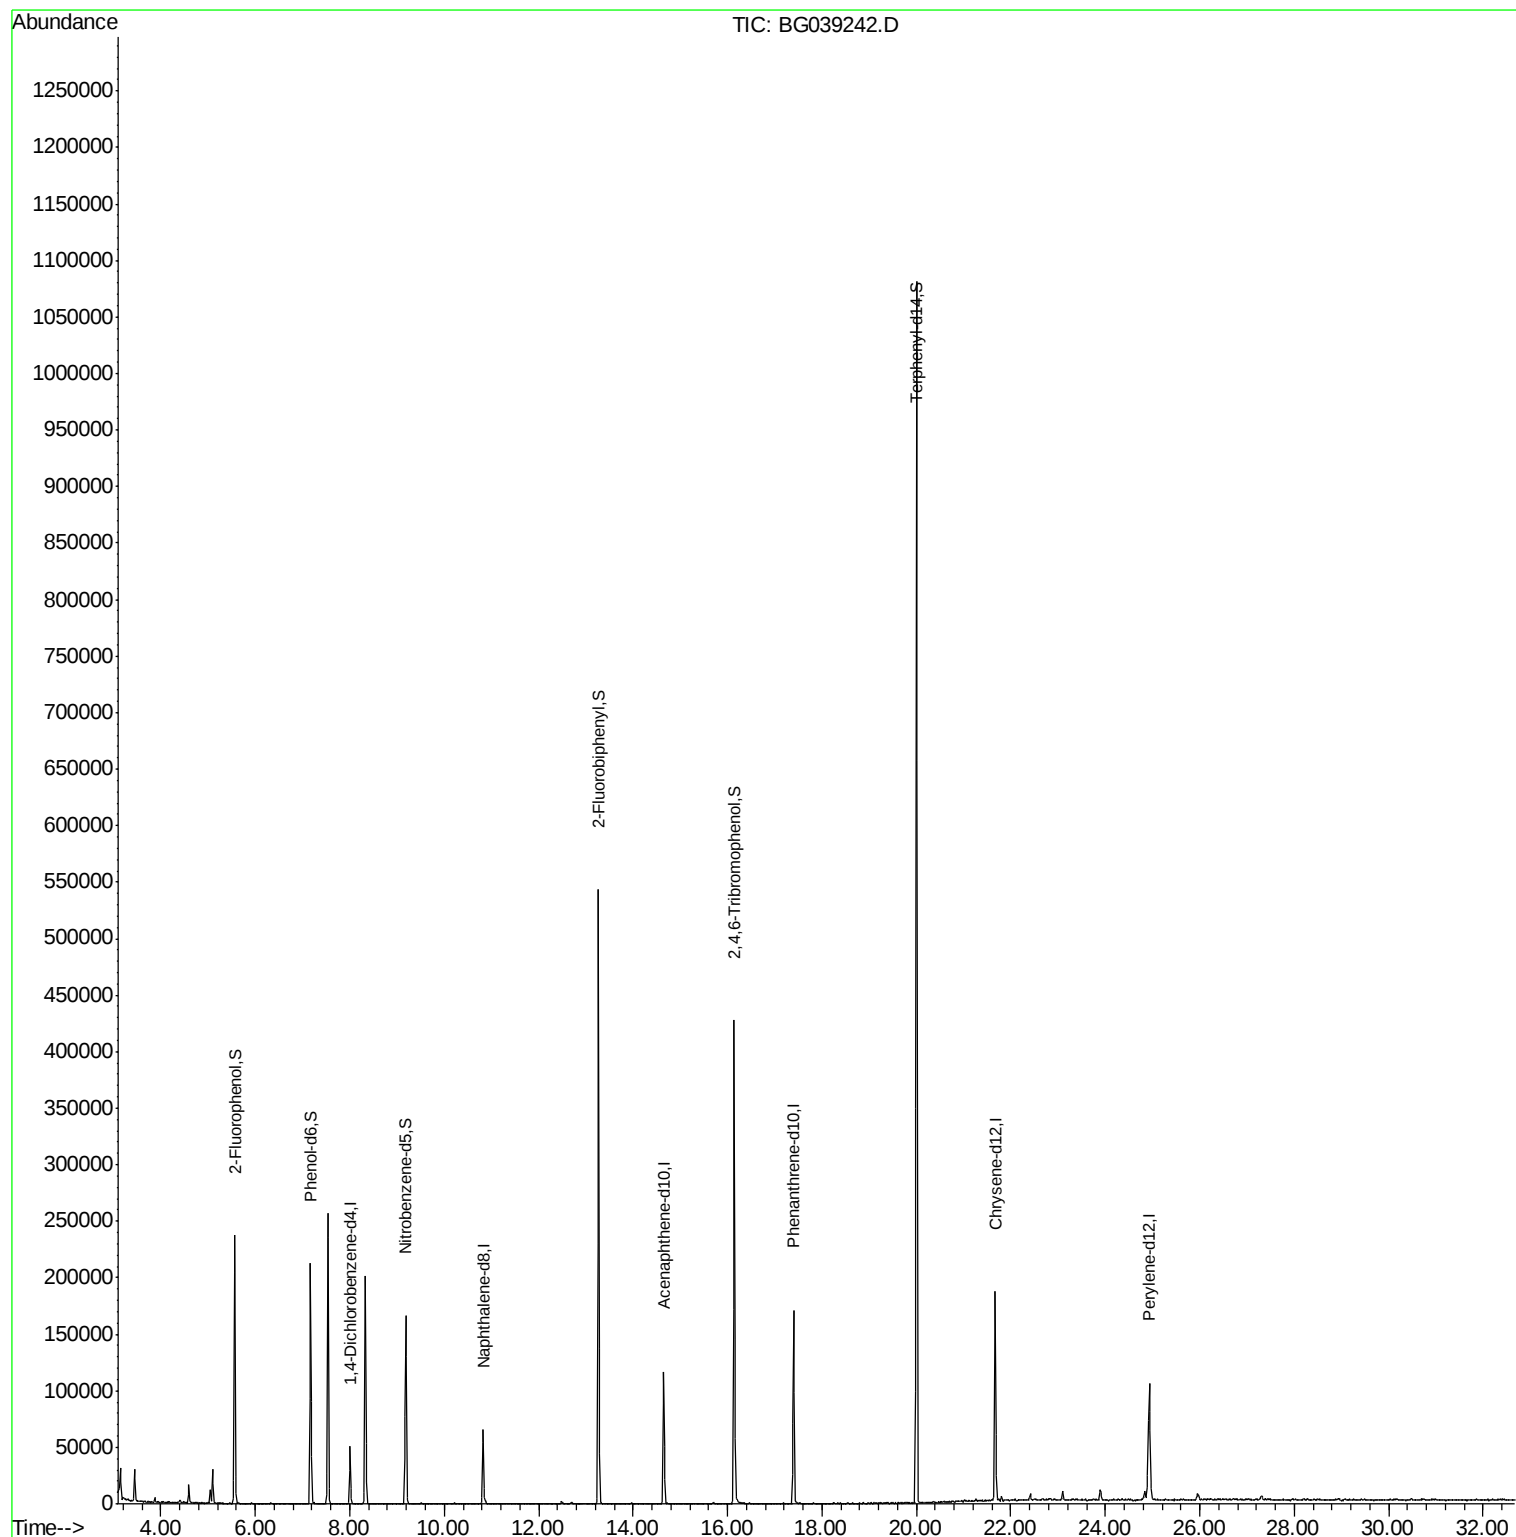




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039242.D
Acq: 21 Jan 2019 20:38

Instrument :
BNA_G
ClientSampleId :
CL-01-011819-A

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.3	124.7	187.1
115	55.1	46.5	69.7

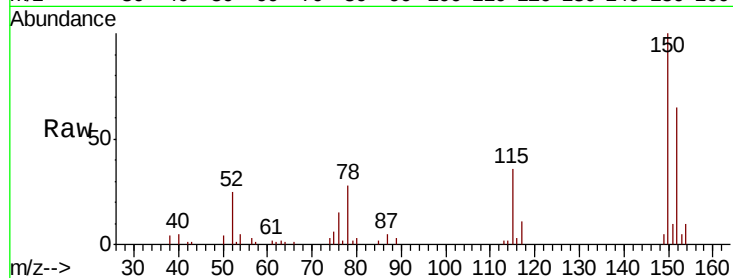


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

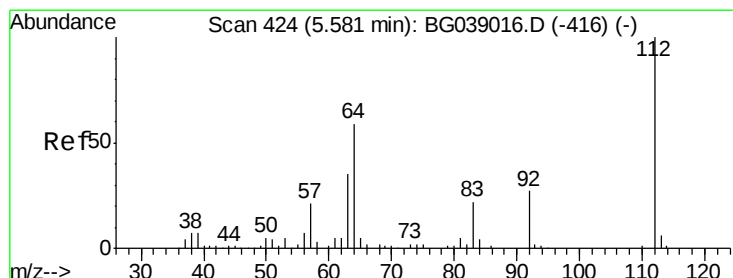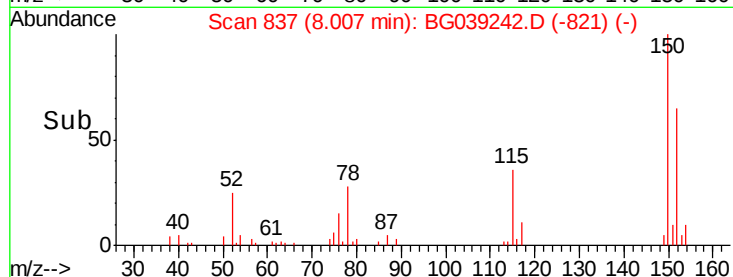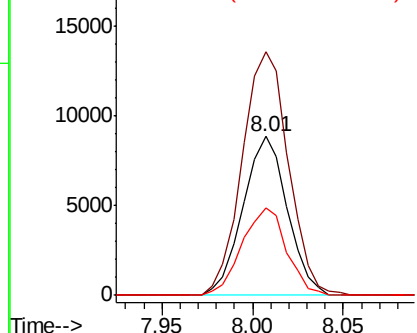



#5


2-Fluorophenol
Concen: 128.647 ng
RT: 5.56 min Scan# 421
Delta R.T. -0.00 min
Lab File: BG039242.D
Acq: 21 Jan 2019 20:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.5	47.0	70.6
63	33.6	28.0	42.0

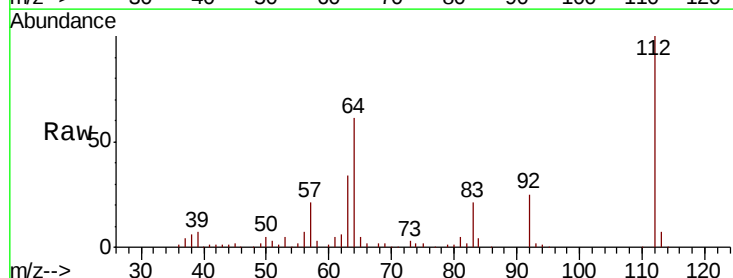

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

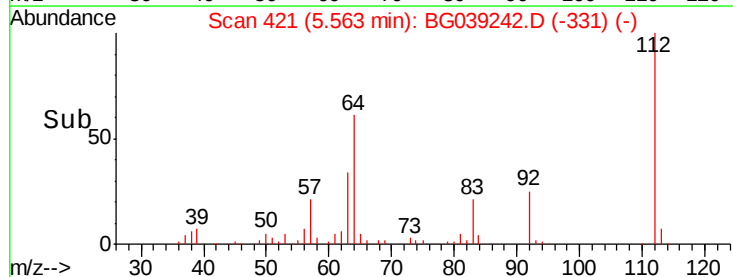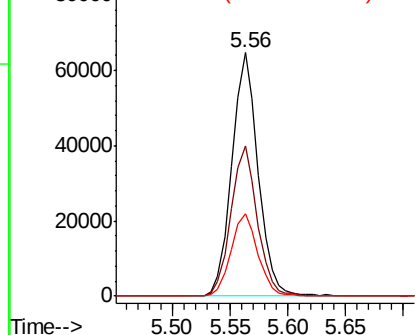

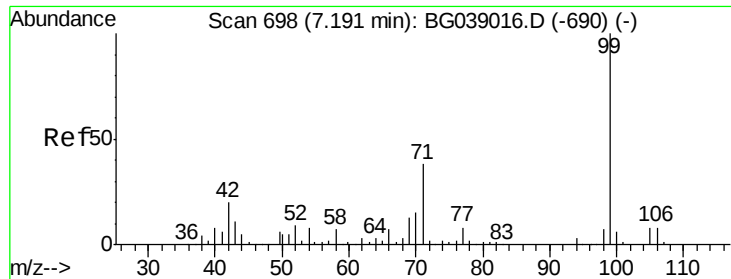

#7

Phenol-d6

Concen: 107.701 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.00 min

Lab File: BG039242.D

Acq: 21 Jan 2019 20:38

Instrument :

BNA_G

ClientSampleId :

CL-01-011819-A


Tot Ion: 99 Resp: 122454

Ion Ratio Lower Upper

99 100

42 20.0 15.8 23.6

71 38.1 30.2 45.4



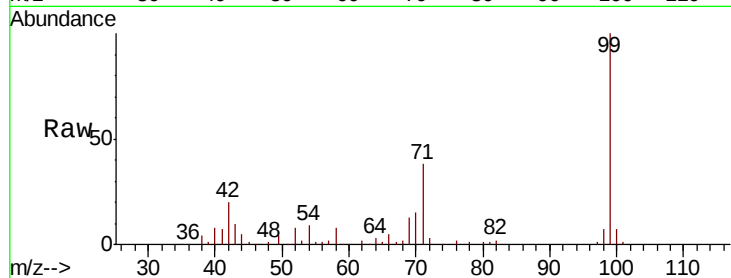


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

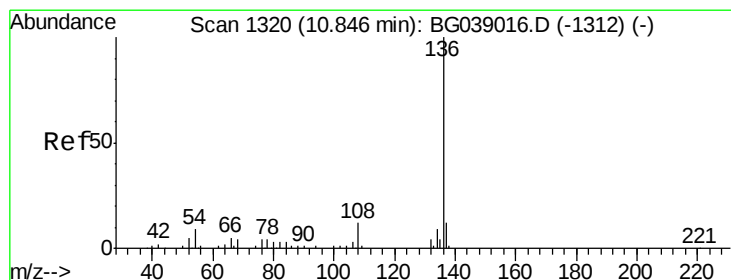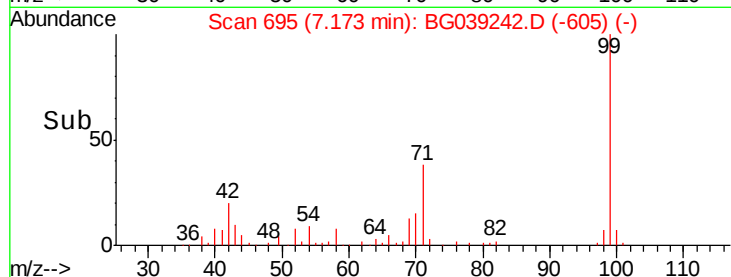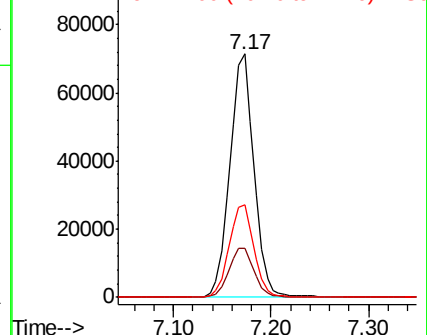

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG039242.D

Acq: 21 Jan 2019 20:38

Tgt Ion: 136 Resp: 59416


Ion Ratio Lower Upper

136 100

137 9.7 9.4 14.2

54 10.2 7.2 10.8

68 4.8 3.5 5.3

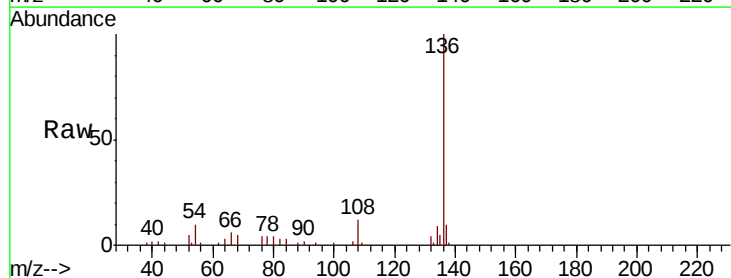



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

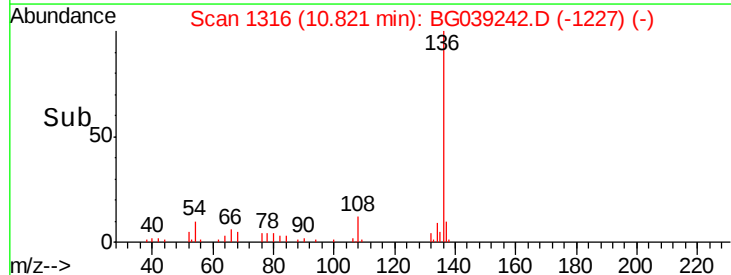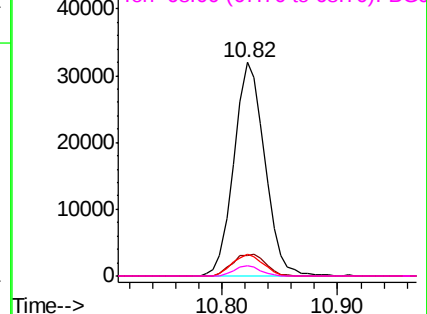


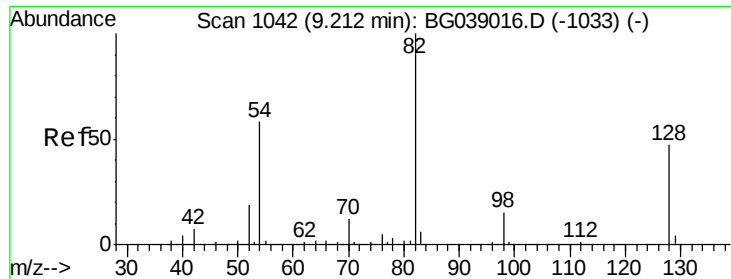




#23
 Nitrobenzene-d5
 Concen: 92.212 ng
 RT: 9.19 min Scan# 1038
 Delta R.T. -0.00 min
 Lab File: BG039242.D
 Acq: 21 Jan 2019 20:38

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-011819-A

Tot Ion: 82 Resp: 100126
 Ion Ratio Lower Upper
 82 100
 128 44.0 37.3 55.9
 54 58.9 46.4 69.6

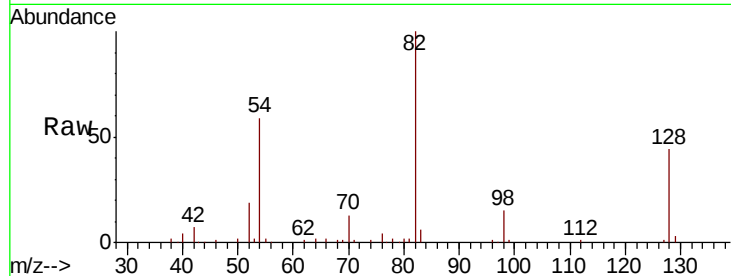


Abundance Ion 82.00 (81.70 to 82.70): BG
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BG

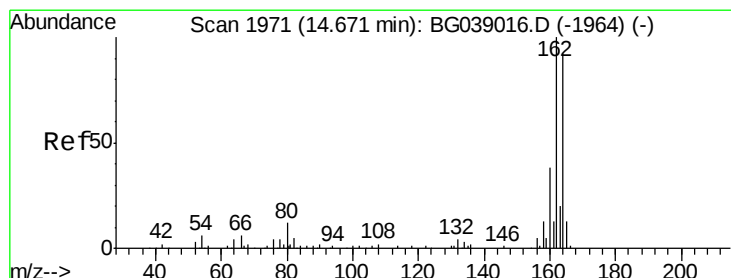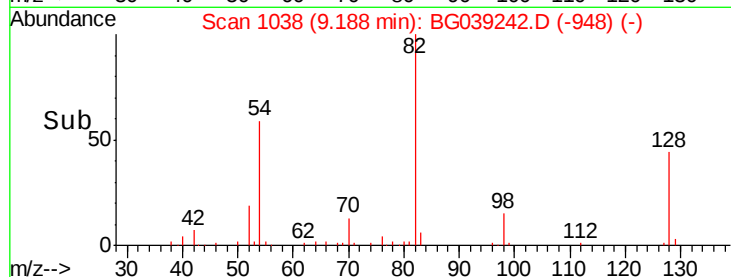
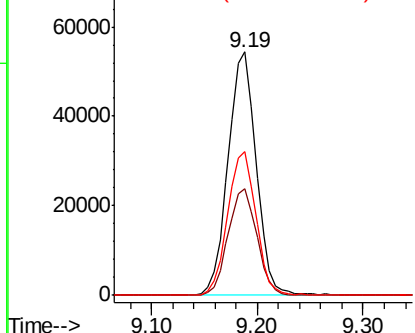



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.65 min Scan# 1967
 Delta R.T. -0.01 min
 Lab File: BG039242.D
 Acq: 21 Jan 2019 20:38

Tgt Ion:164 Resp: 45383
 Ion Ratio Lower Upper
 164 100
 162 104.6 87.2 130.8
 160 44.1 33.3 49.9

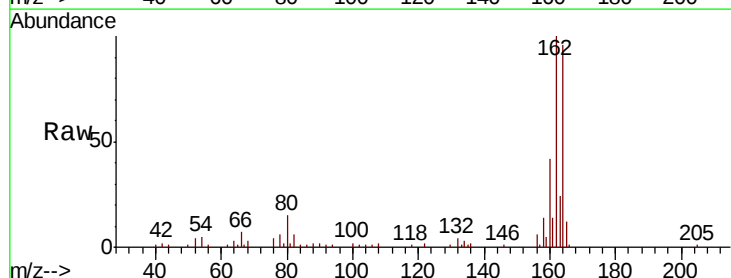

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

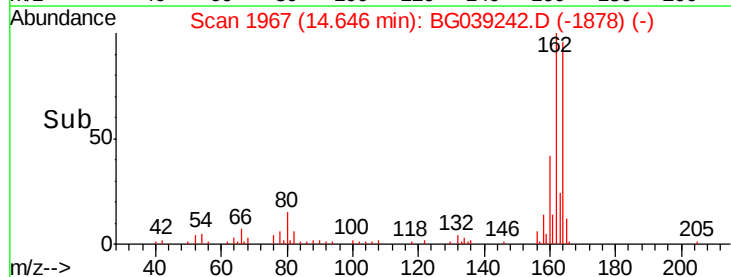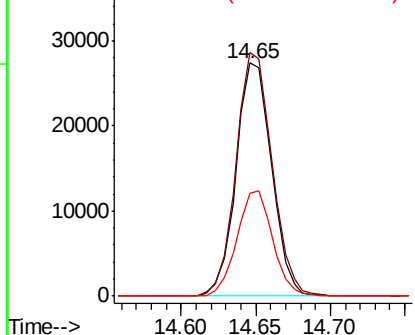


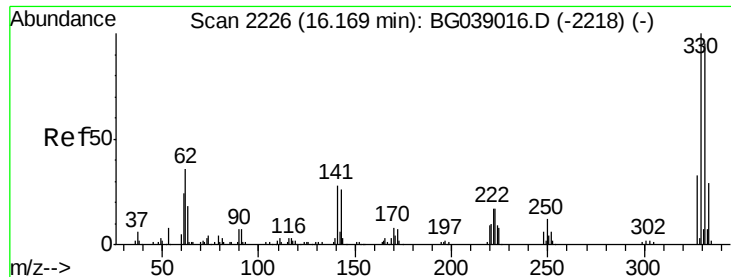

#42
 2,4,6-Tribromophenol
 Concen: 128.131 ng
 RT: 16.14 min Scan# 2222
 Delta R.T. -0.01 min
 Lab File: BG039242.D
 Acq: 21 Jan 2019 20:38

Instrument :
 BNA_G
 ClientSampleId :
 CL-01-011819-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	75.7	113.5
141	32.5	24.9	37.3



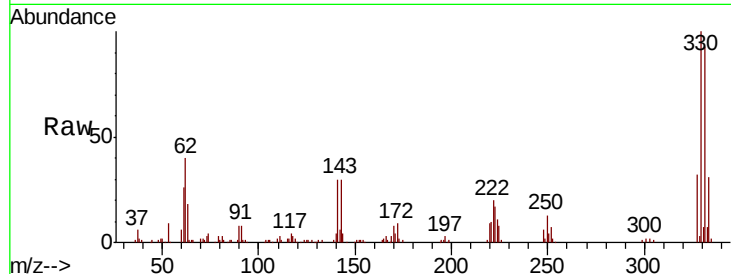


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

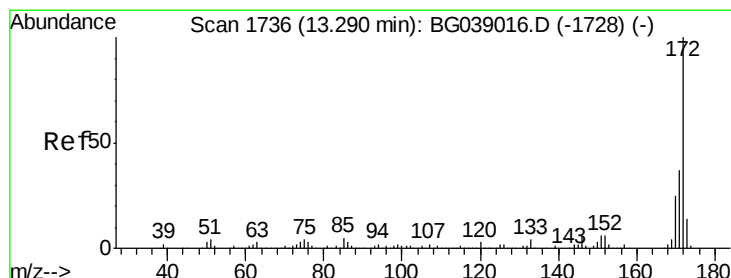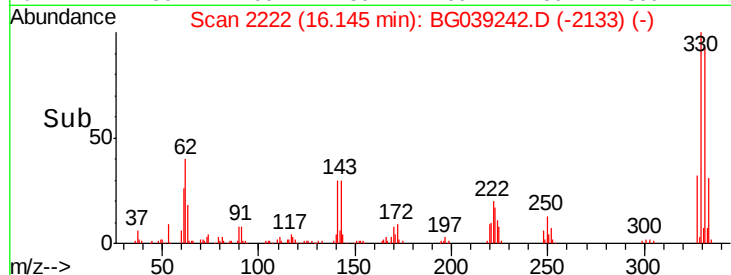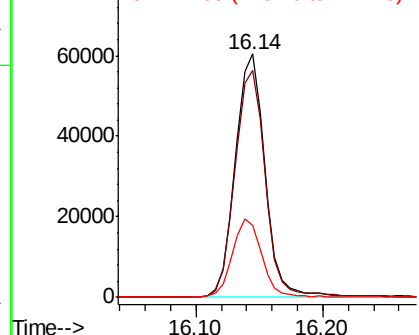

#45
 2-Fluorobiphenyl
 Concen: 85.982 ng
 RT: 13.27 min Scan# 1732
 Delta R.T. -0.01 min
 Lab File: BG039242.D
 Acq: 21 Jan 2019 20:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.4	44.0
170	24.7	20.1	30.1


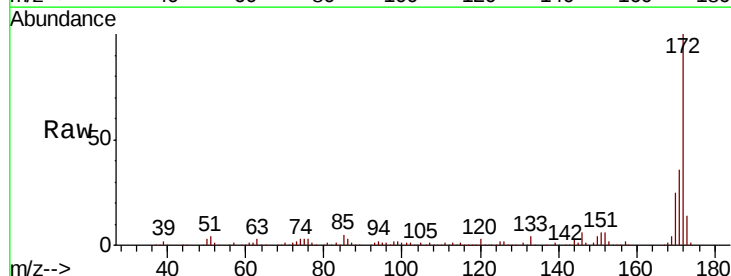


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

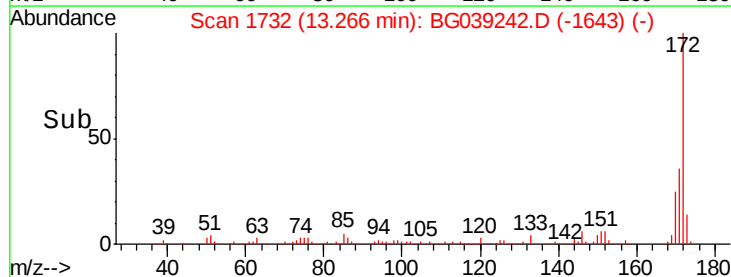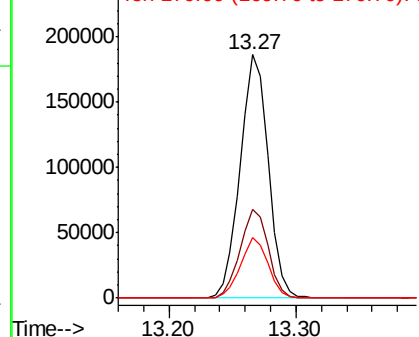







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.40 min Scan# 2435
Delta R.T. -0.01 min
Lab File: BG039242.D
Acq: 21 Jan 2019 20:38

Instrument :
BNA_G
ClientSampleId :
CL-01-011819-A

Tot Ion:188 Resp: 114138
Ion Ratio Lower Upper
188 100
94 6.5 5.0 7.4
80 6.8 4.7 7.1

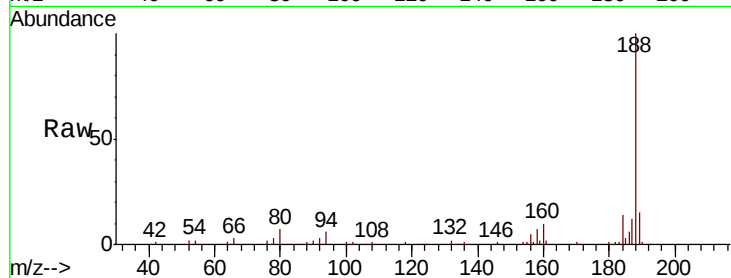


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

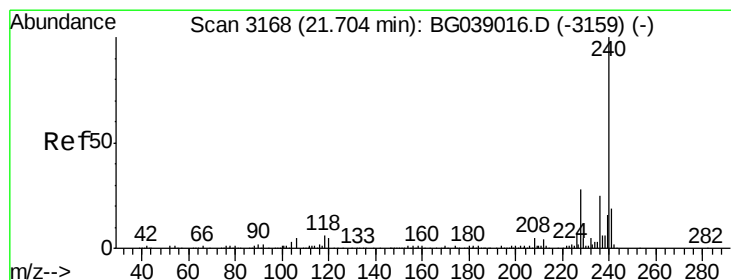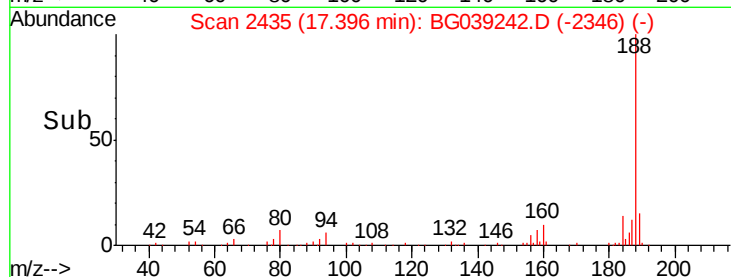
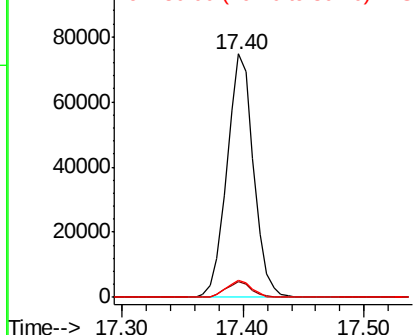



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.67 min Scan# 3162
Delta R.T. -0.01 min
Lab File: BG039242.D
Acq: 21 Jan 2019 20:38

Tgt Ion:240 Resp: 119347
Ion Ratio Lower Upper
240 100
120 6.6 4.3 6.5#
236 26.2 20.1 30.1

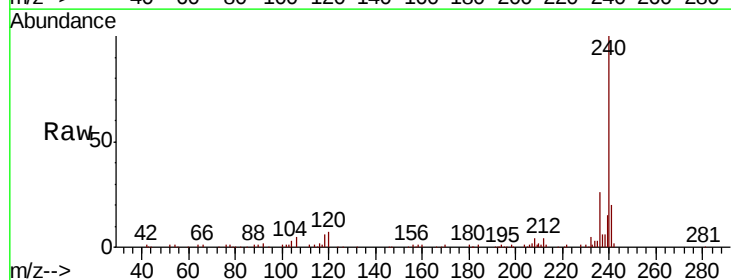

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

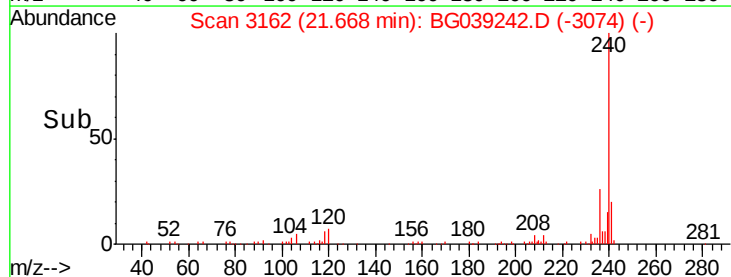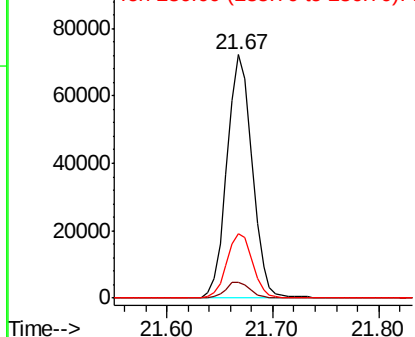

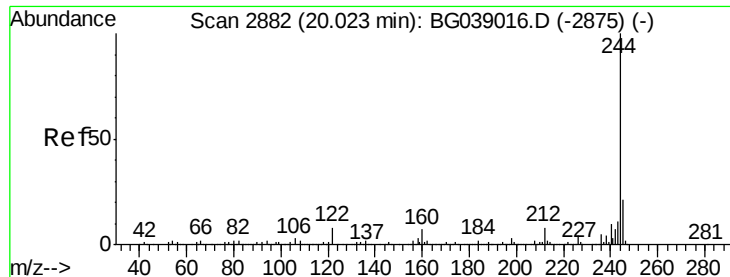

#79

Terphenyl-d14

Concen: 90.483 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG039242.D

Acq: 21 Jan 2019 20:38

Instrument :

BNA_G

ClientSampleId :

CL-01-011819-A


Tot Ion:244 Resp: 583755

Ion Ratio Lower Upper

244 100

212 7.4 6.1 9.1




122 6.5 6.1 9.1

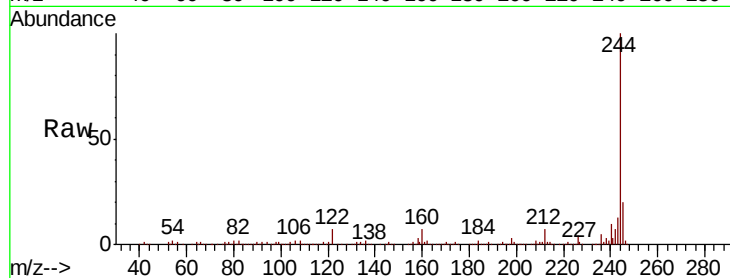

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

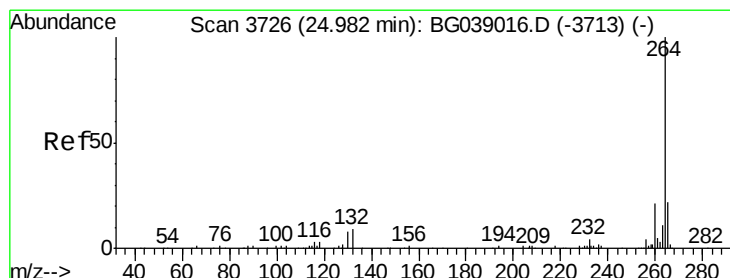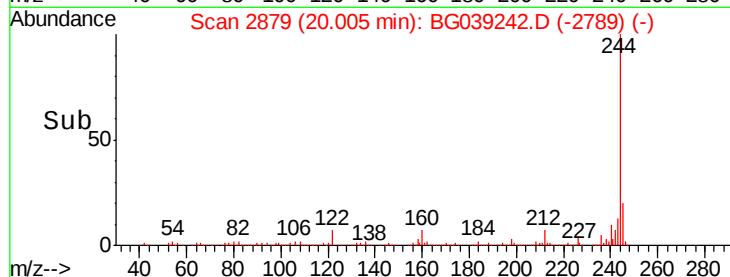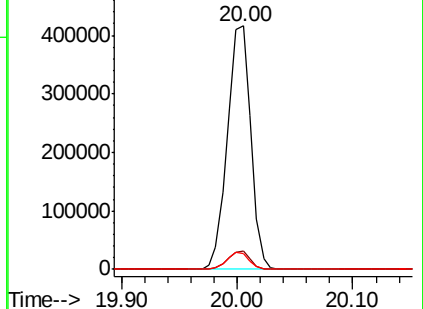

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.02 min

Lab File: BG039242.D

Acq: 21 Jan 2019 20:38


Tgt Ion:264 Resp: 127235

Ion Ratio Lower Upper

264 100

260 21.8 17.0 25.6

265 20.8 17.2 25.8

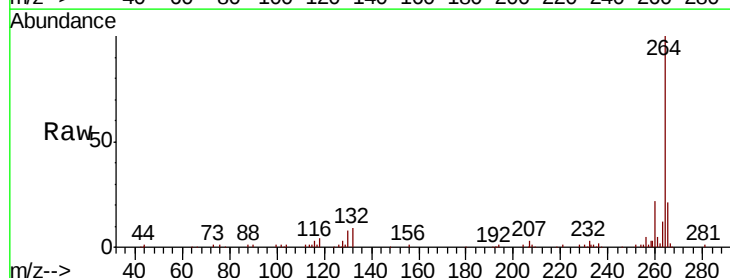

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

