


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012119\
 Data File : BG039228.D
 Acq On : 21 Jan 2019 11:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 04:20:14 2019

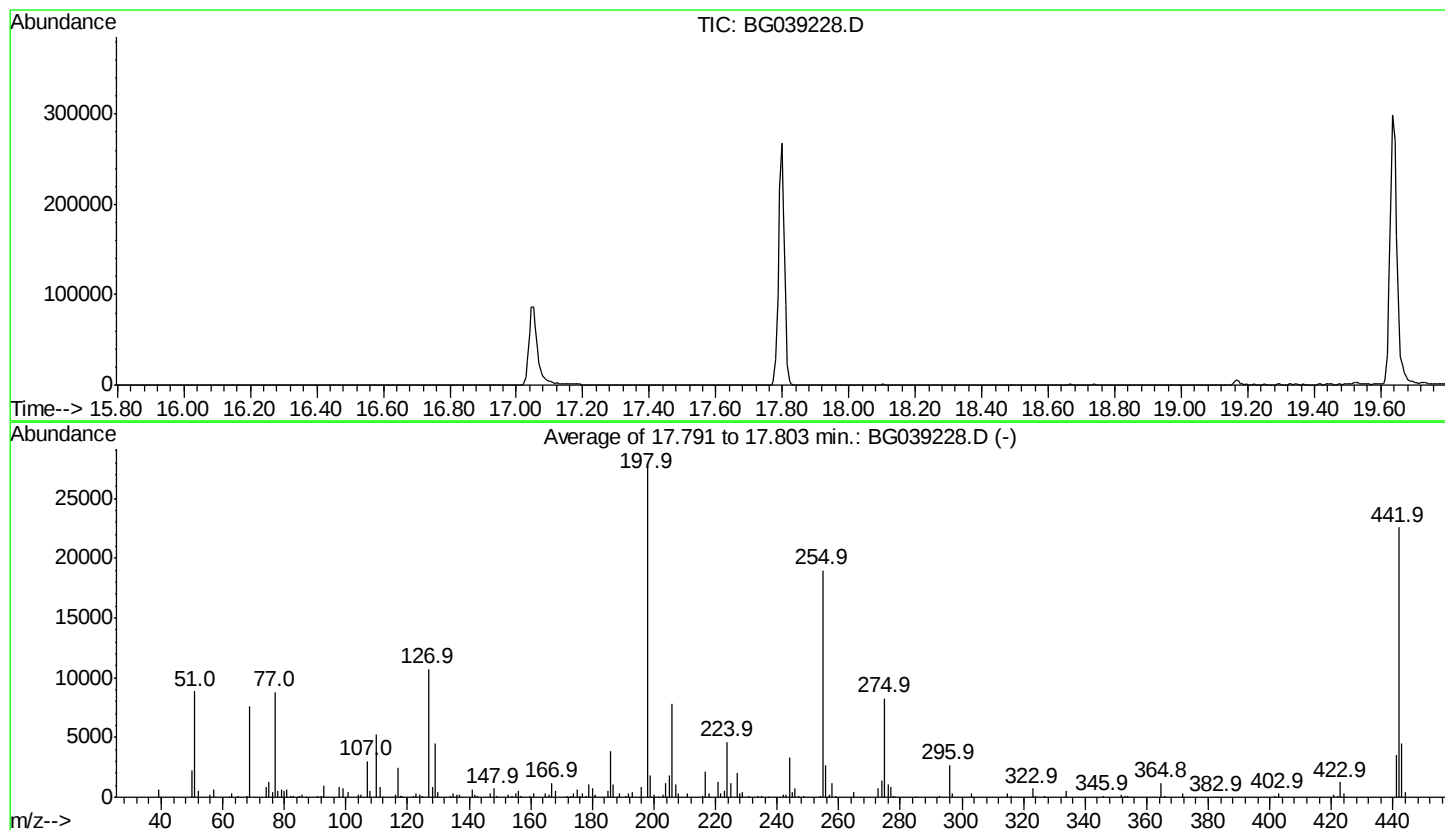

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	8871	PASS
68	69	0.00	2	1.6	121	PASS
69	198	0.00	100	27.6	7648	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.7	10742	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27738	PASS
199	198	5	9	6.7	1857	PASS
275	198	10	60	29.7	8250	PASS
365	198	1	100	4.3	1193	PASS
441	198	0.01	100	12.9	3565	PASS
442	198	50	100	81.3	22545	PASS
443	442	15	24	20.0	4508	PASS