
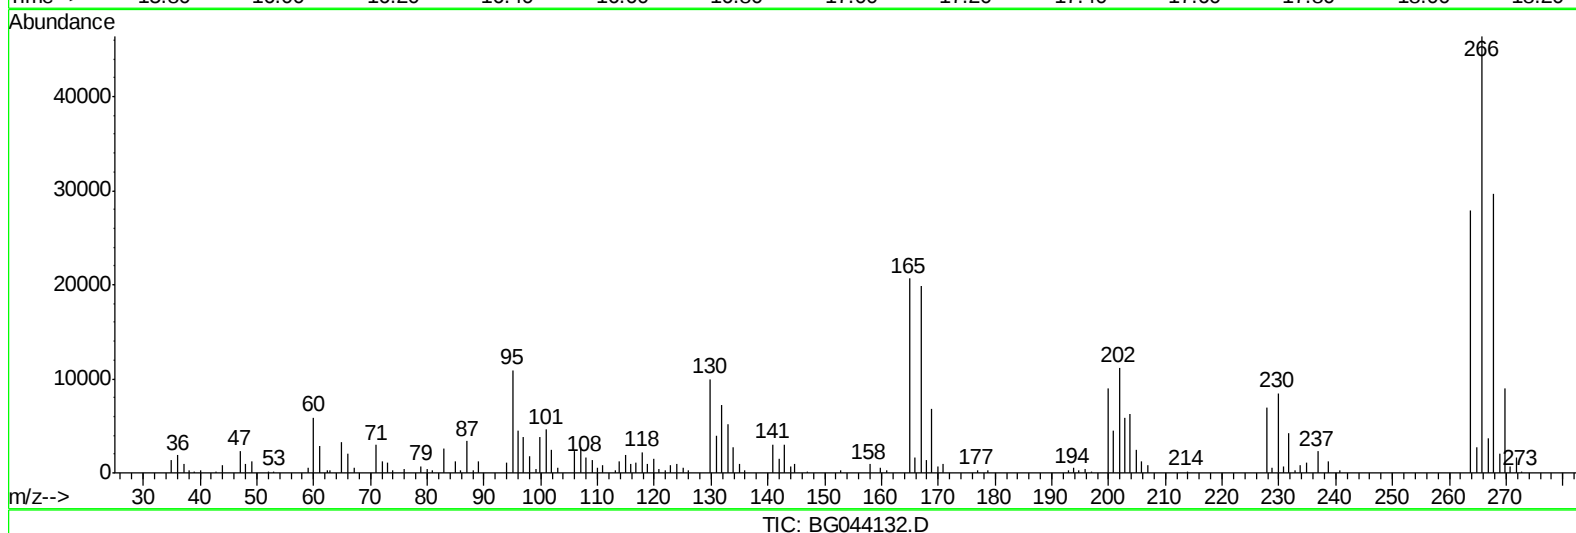


Data File : BG044132.D
Acq On : 21 Jan 2020 14:04
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 07:34:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

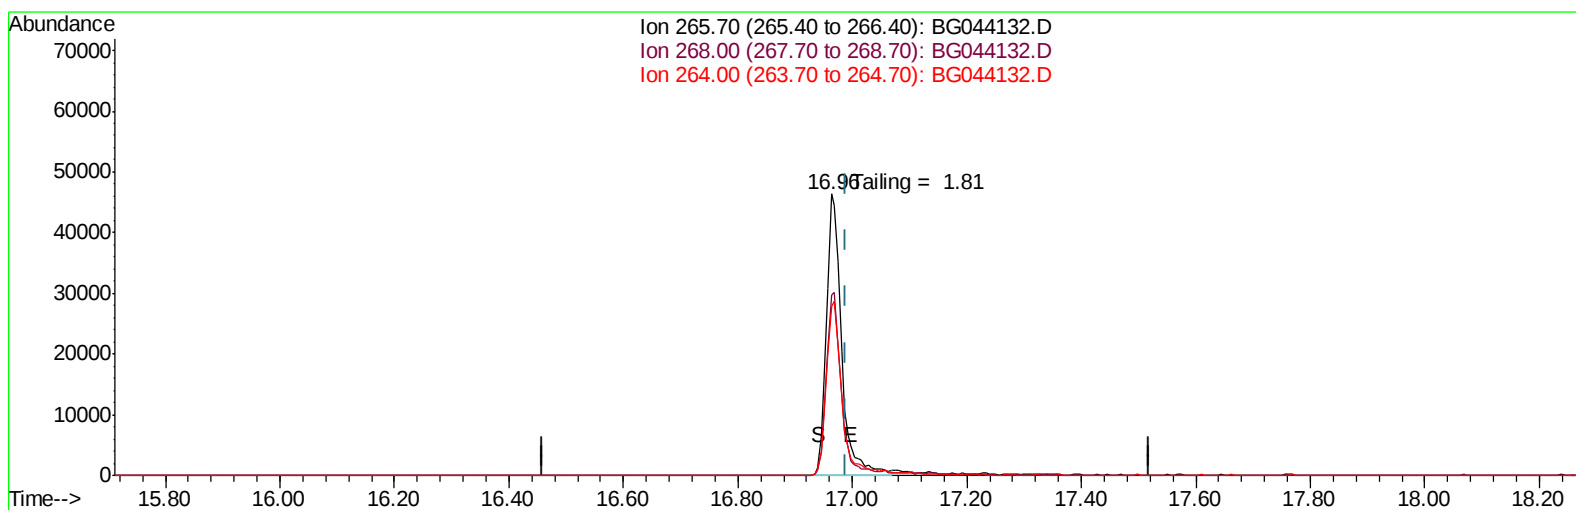

TIC: BG044132.D

(70) Pentachlorophenol (C)



16.963min (-0.026) 163104.12ng

response 84991

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	63.99
264.00	63.50	60.20
0.00	0.00	0.00

Data File : BG044132.D
Acq On : 21 Jan 2020 14:04
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 07:34:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

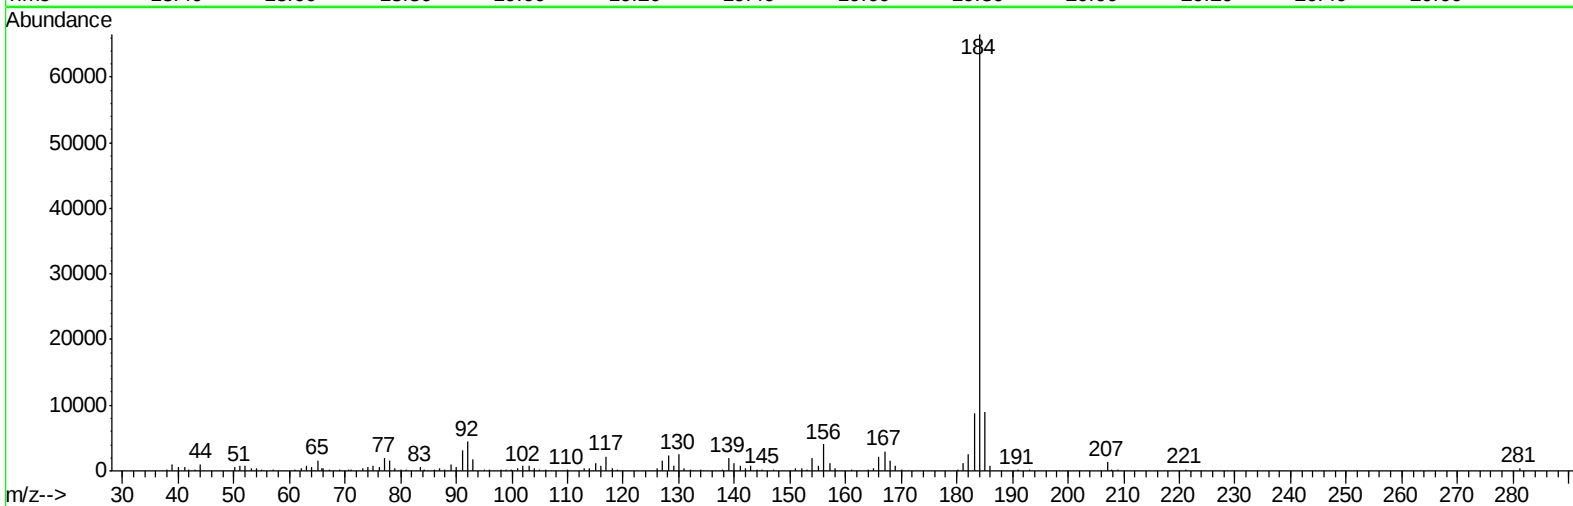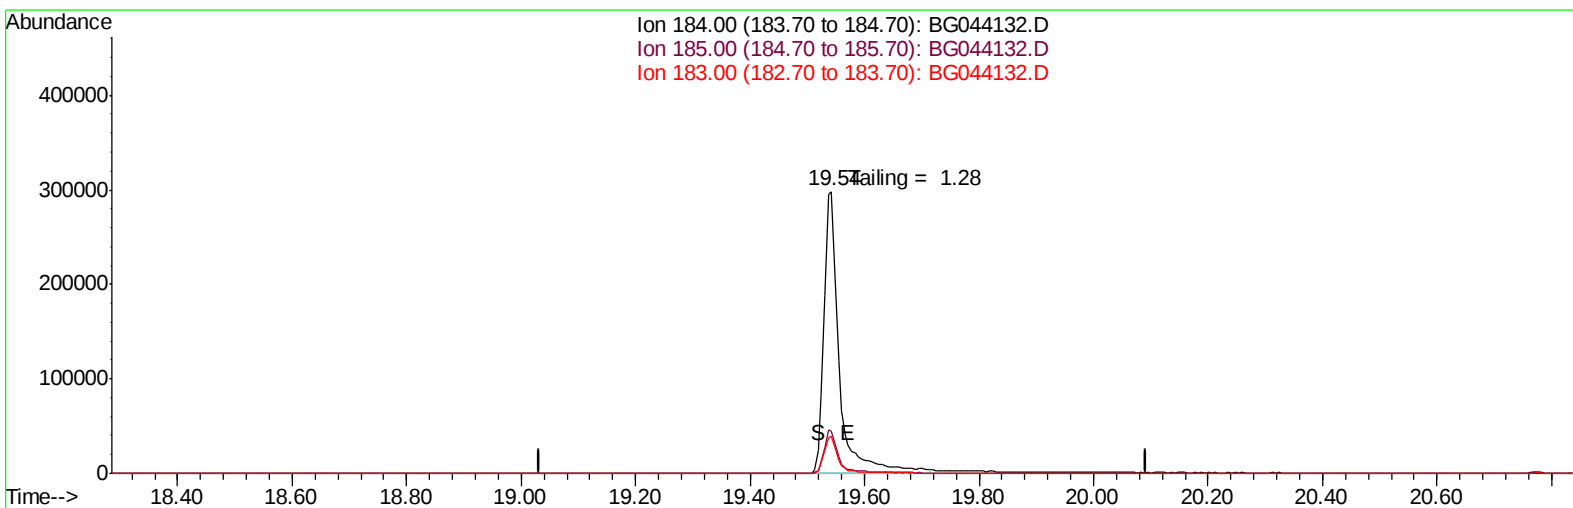

TIC: BG044132.D

(77) Benzidine

19.563min (-19.563) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.70	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00