


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG012120\  
 Data File : BG044132.D  
 Acq On : 21 Jan 2020 14:04  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG123019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Dec 31 13:32:23 2019

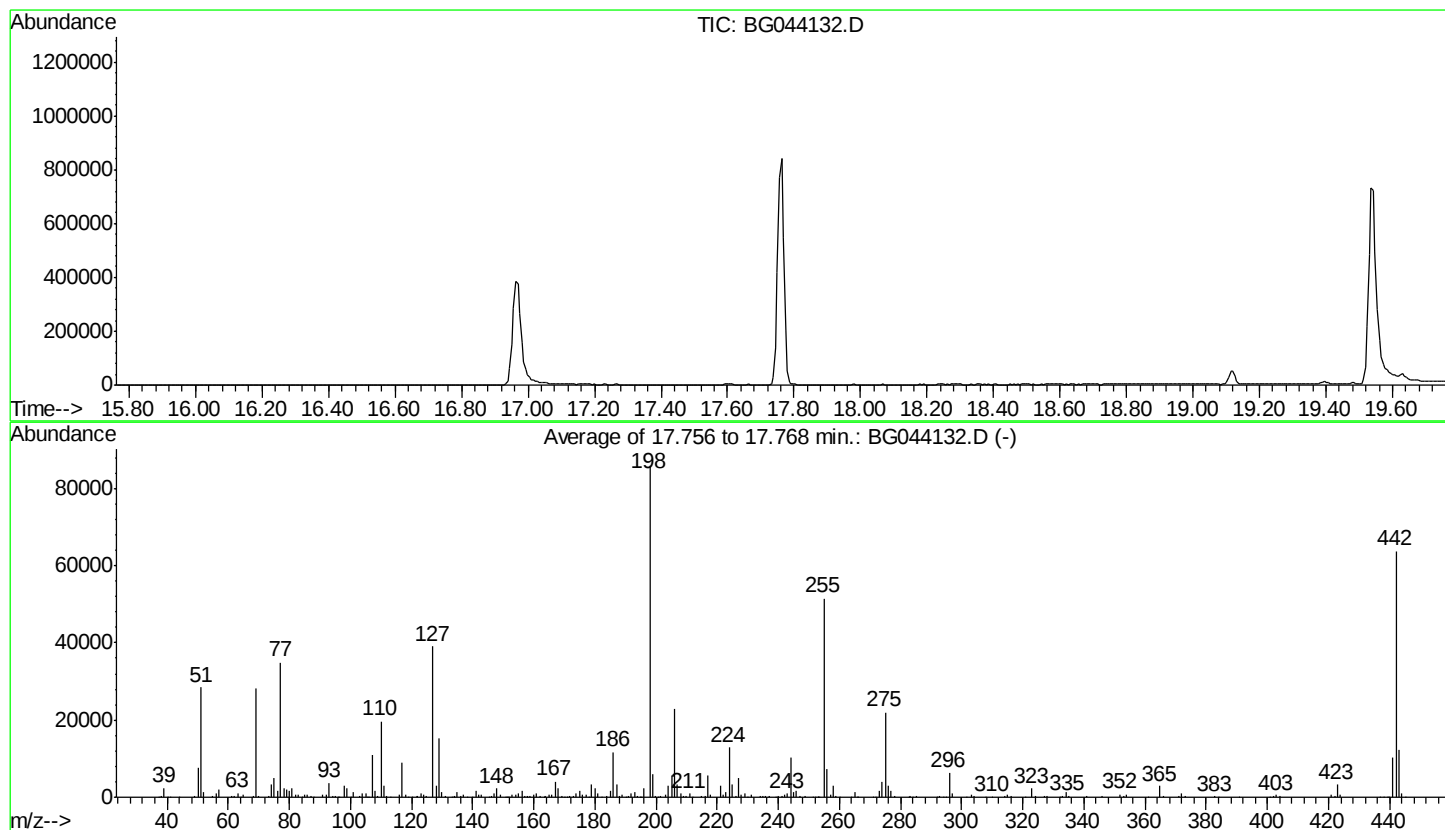

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 33.2      | 28522   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.9       | 254     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.9      | 28226   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 189     | PASS             |
| 127         | 198          | 10           | 80           | 45.4      | 38997   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 85922   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 5924    | PASS             |
| 275         | 198          | 10           | 60           | 25.6      | 21976   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 2972    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.1      | 10398   | PASS             |
| 442         | 198          | 50           | 100          | 74.3      | 63810   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 12253   | PASS             |