
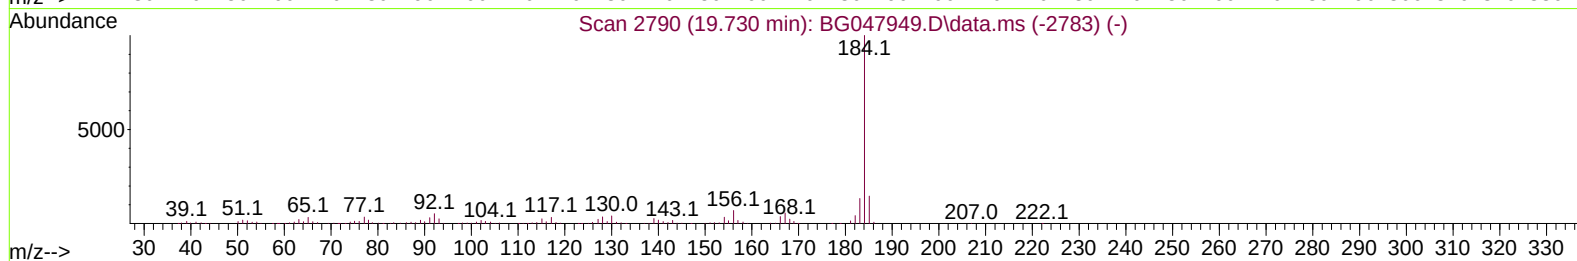
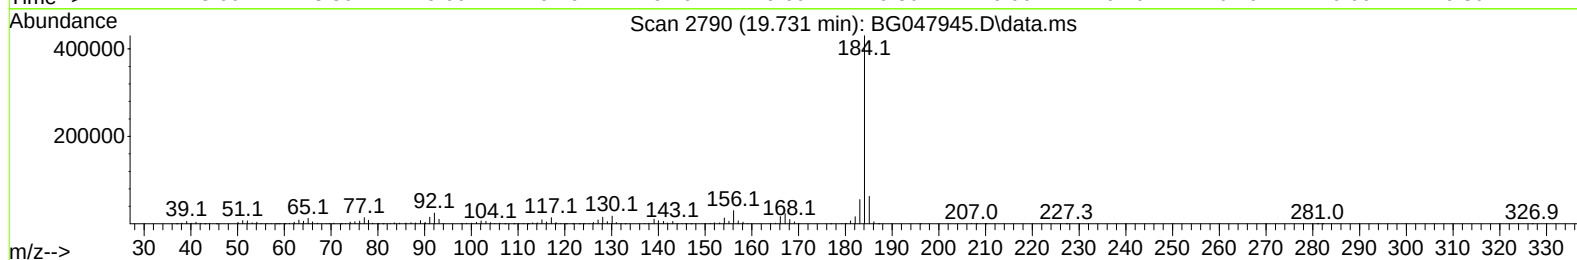


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
 Data File : BG047945.D
 Acq On : 21 Jan 2021 8:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:19:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 21 14:42:53 2021
 Response via : Initial Calibration

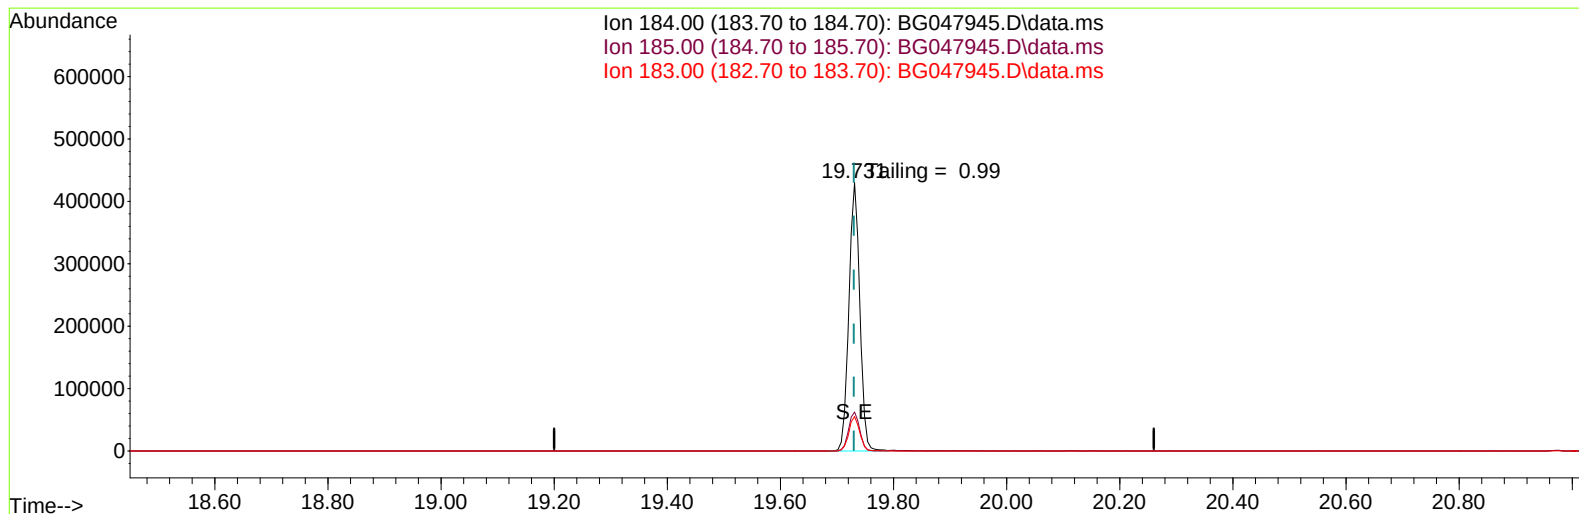




TIC: BG047945.D\data.ms

(77) Benzidine**19.731min (+ 0.001) 28507.91 ng****response 576964**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.56
183.00	13.20	12.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
 Data File : BG047945.D
 Acq On : 21 Jan 2021 8:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:19:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 21 14:42:53 2021
 Response via : Initial Calibration

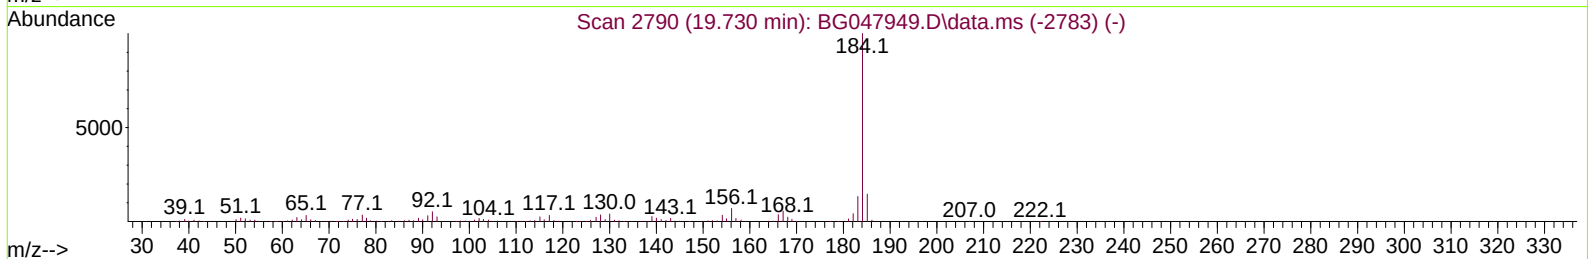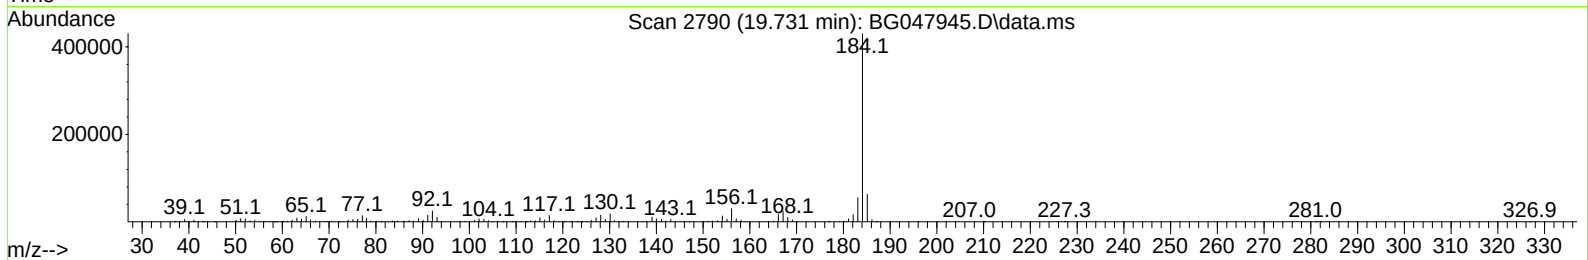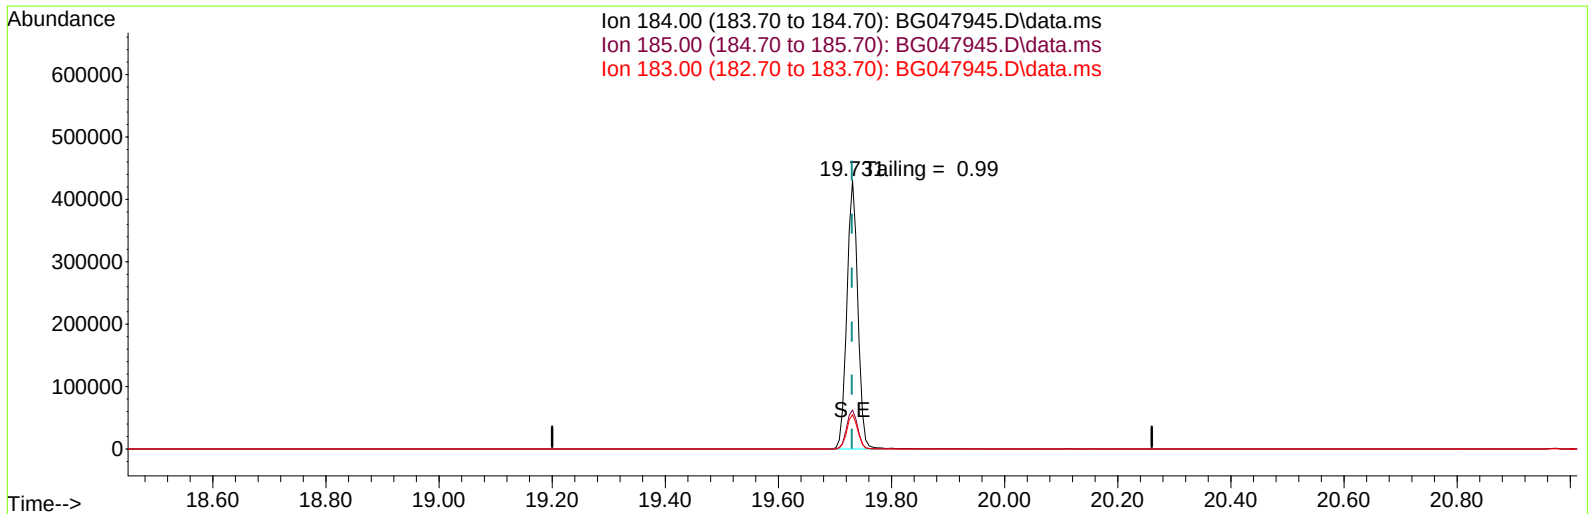

TIC: BG047945.D\data.ms

(77) Benzidine**19.731min (+ 0.001) 28507.91 ng****response 576964**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.56
183.00	13.20	12.85
0.00	0.00	0.00