
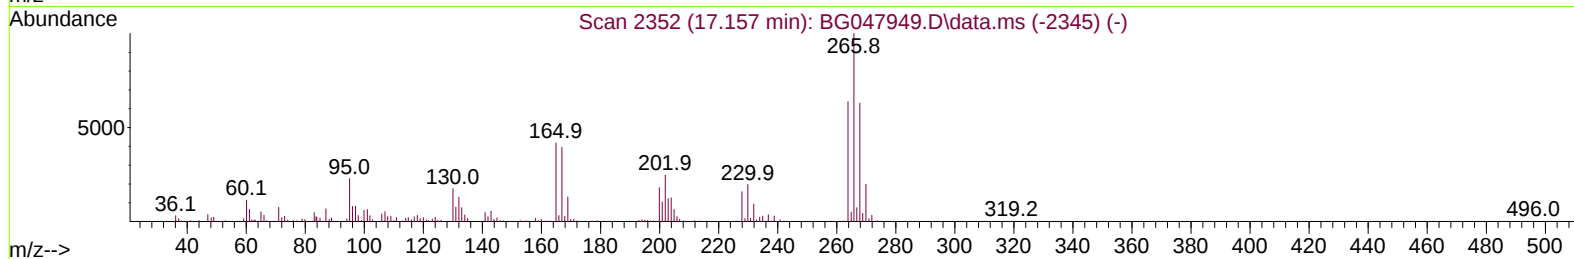
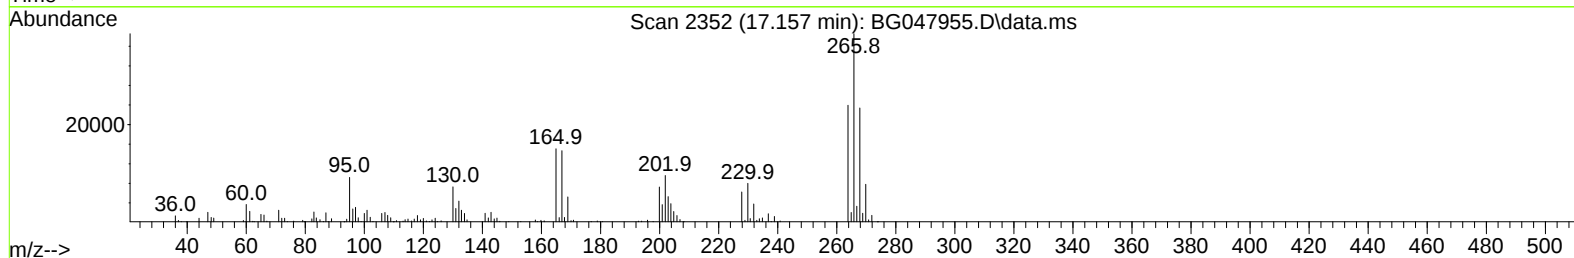


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
Data File : BG047955.D
Acq On : 21 Jan 2021 15:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:25:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 21 14:42:53 2021
Response via : Initial Calibration

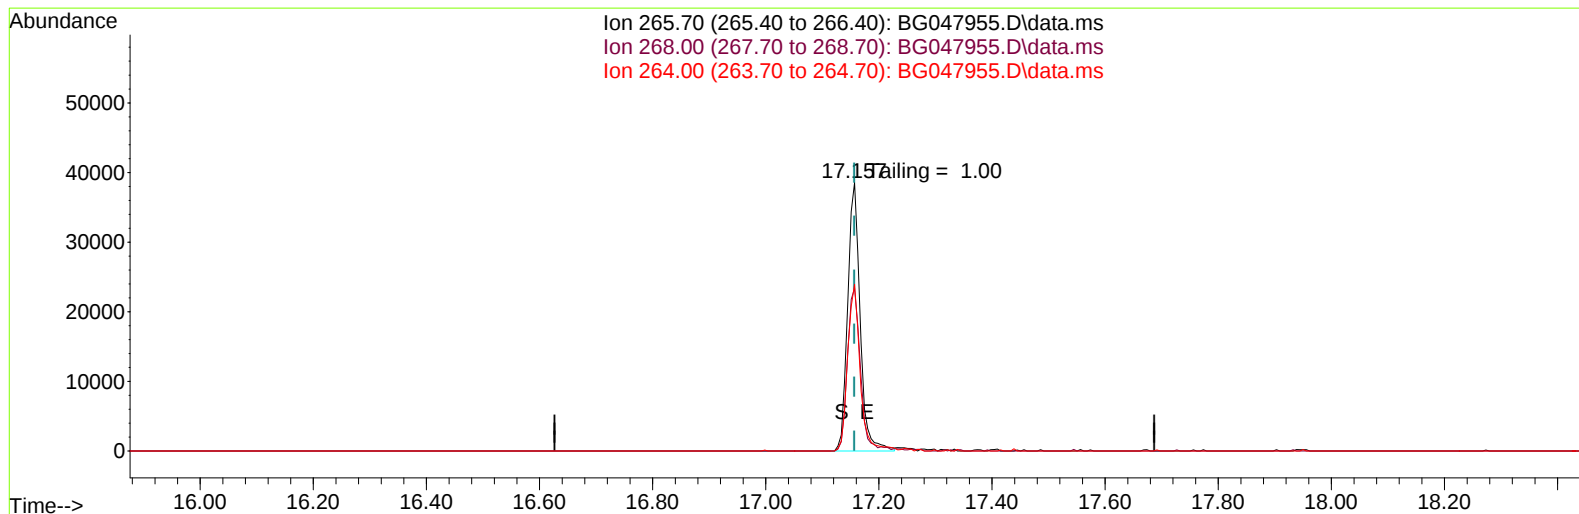

TIC: BG047955.D\data.ms

(70) Pentachlorophenol (C)




17.157min (+ 0.000) 128030.34 ng m

response 60214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.66
264.00	61.60	62.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
Data File : BG047955.D
Acq On : 21 Jan 2021 15:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 01:25:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 21 14:42:53 2021
Response via : Initial Calibration

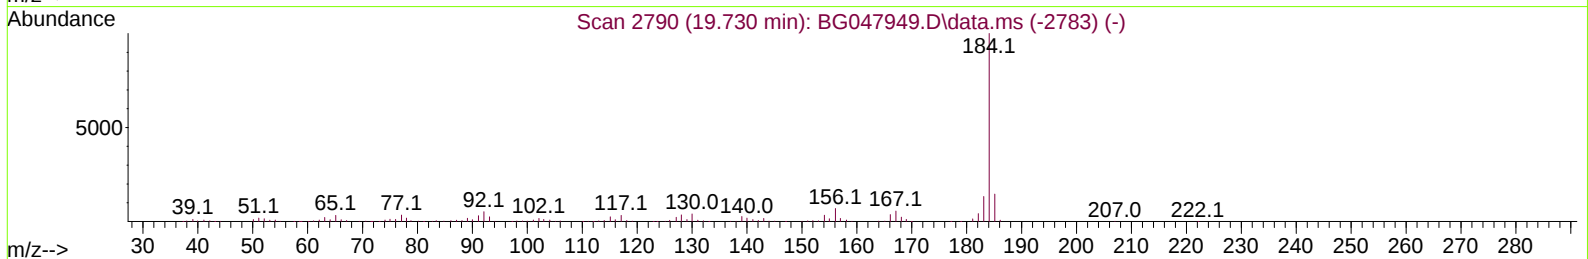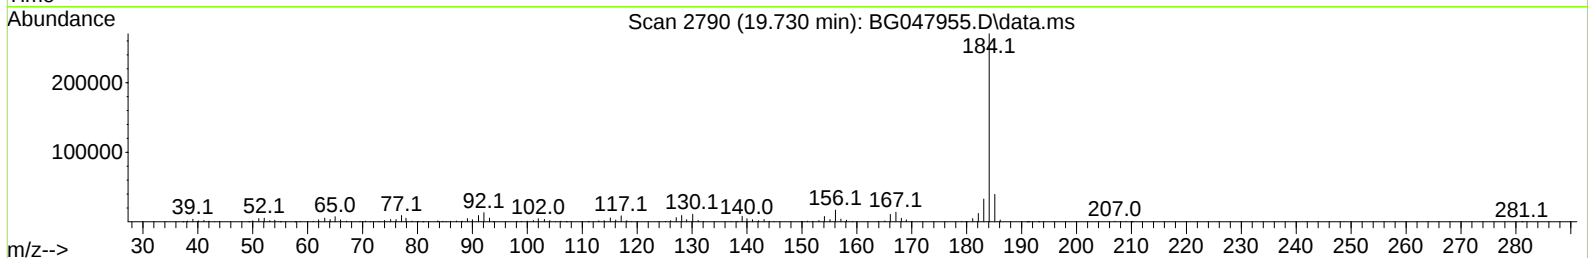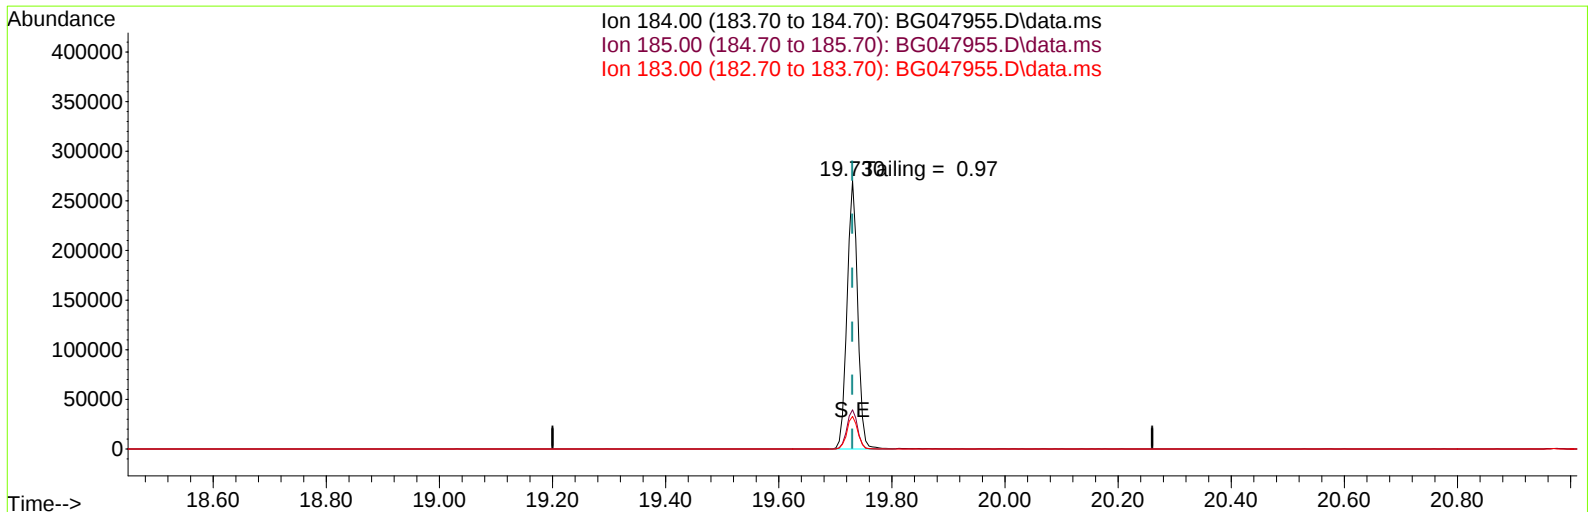

TIC: BG047955.D\data.ms

(77) Benzidine

19.730min (+ 0.000) 5481.32 ng m

response 352580

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	12.17
0.00	0.00	0.00