
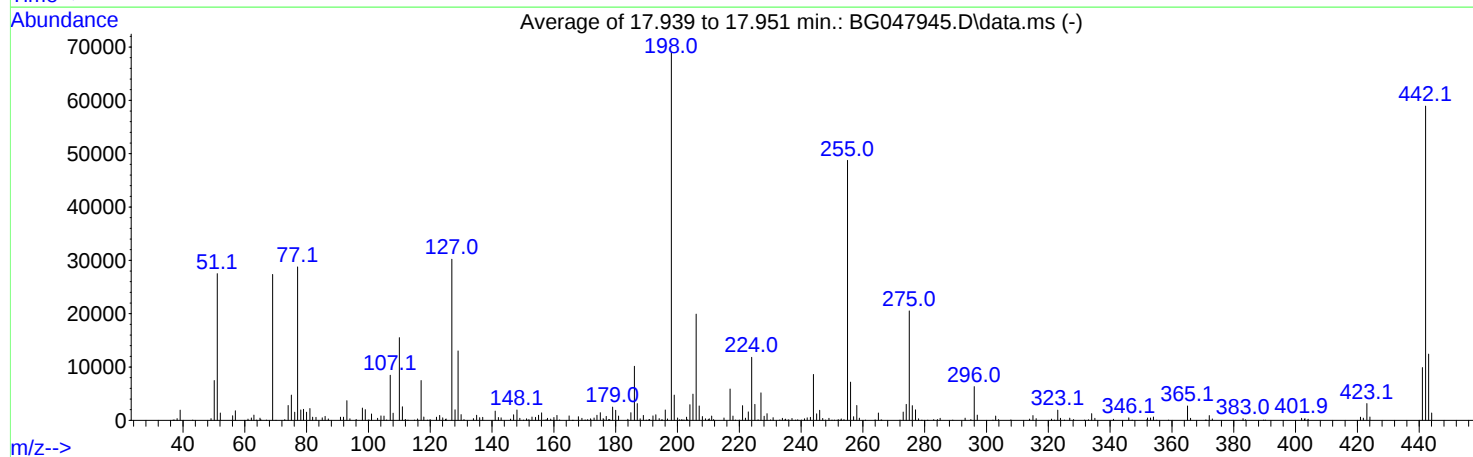


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
 Data File : BG047945.D
 Acq On : 21 Jan 2021 8:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 21 14:42:53 2021

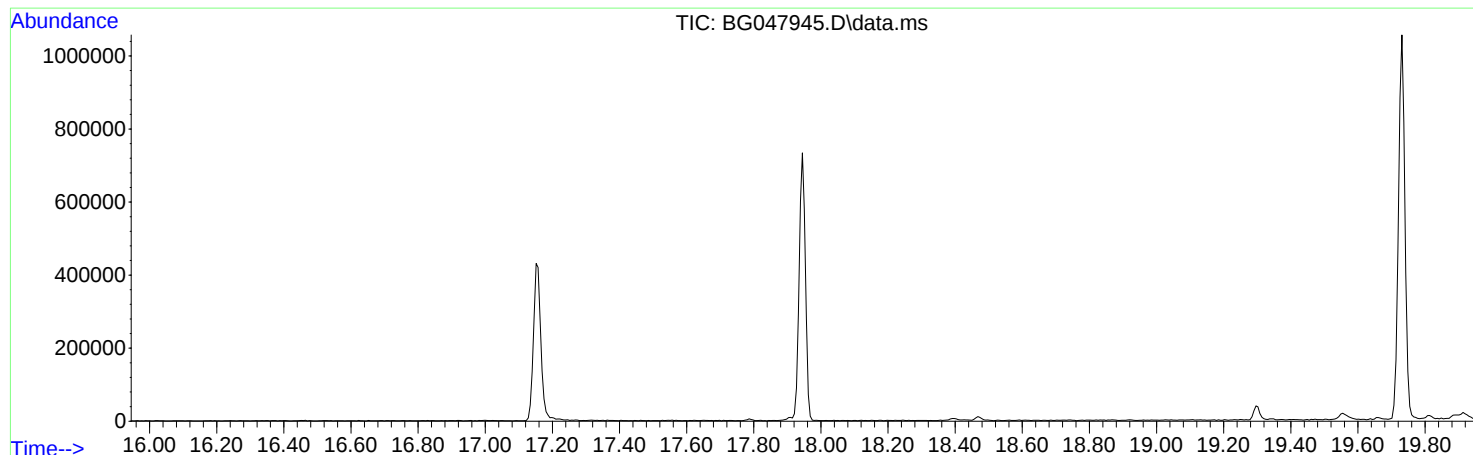

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	27501	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.7	27349	PASS
70	69	0.00	2	0.1	24	PASS
127	198	10	80	43.8	30224	PASS
197	198	0.00	2	0.4	280	PASS
198	198	100	100	100.0	68971	PASS
199	198	5	9	6.9	4751	PASS
275	198	10	60	29.8	20520	PASS
365	198	1	100	3.9	2699	PASS
441	198	0.01	100	14.4	9904	PASS
442	198	50	100	85.4	58917	PASS
443	442	15	24	21.1	12425	PASS