
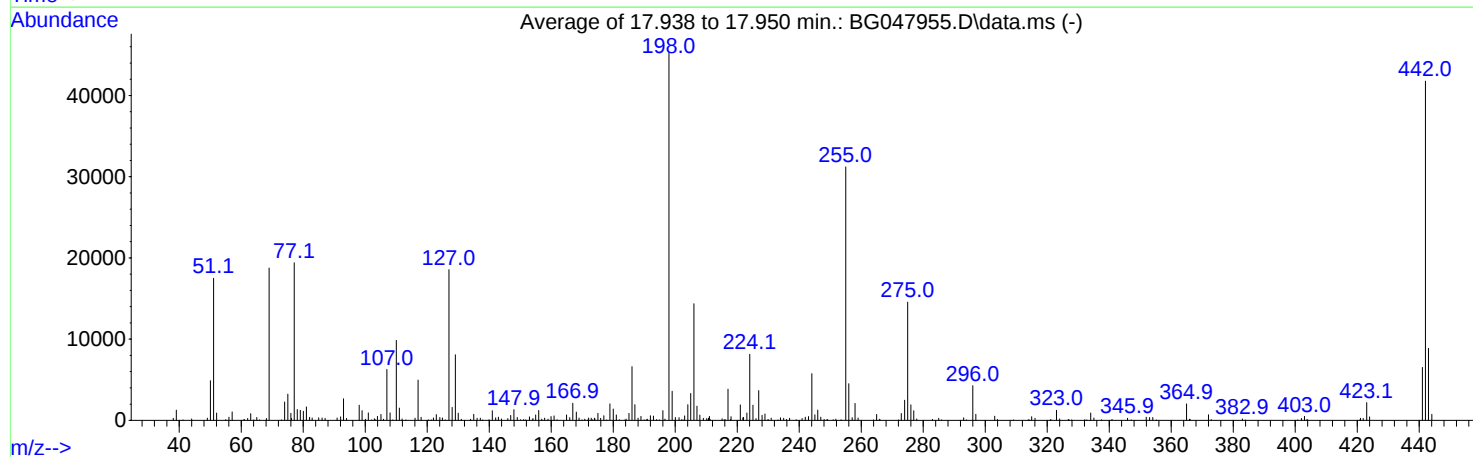


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012121\
 Data File : BG047955.D
 Acq On : 21 Jan 2021 15:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 21 14:42:53 2021

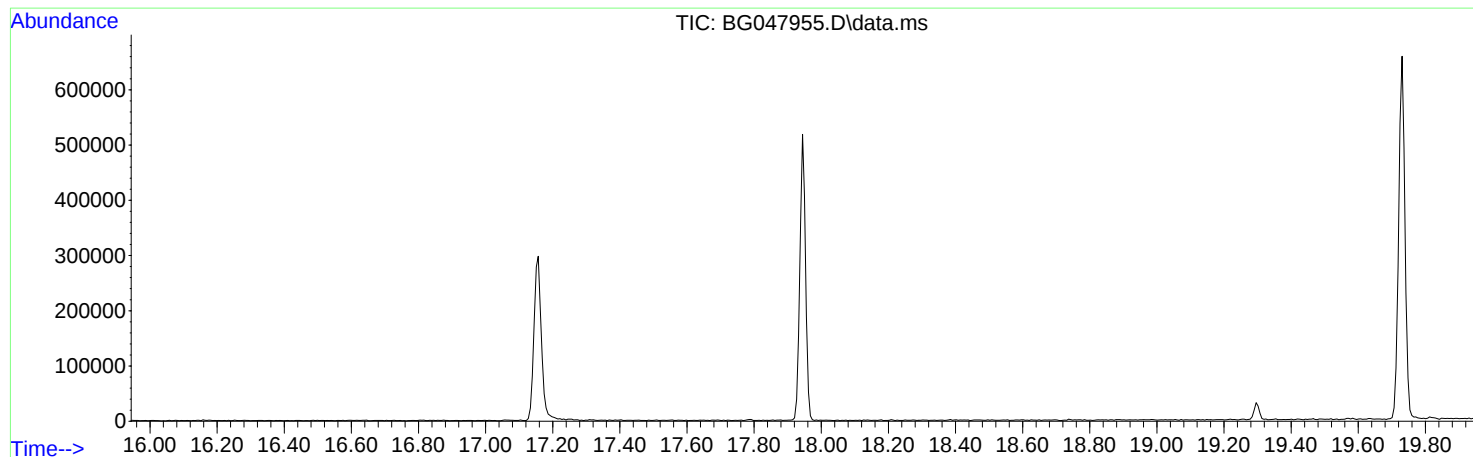

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	17490	PASS
68	69	0.00	2	1.3	246	PASS
69	198	0.00	100	41.4	18750	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	18557	PASS
197	198	0.00	2	0.4	163	PASS
198	198	100	100	100.0	45293	PASS
199	198	5	9	7.9	3592	PASS
275	198	10	60	32.1	14555	PASS
365	198	1	100	4.5	2027	PASS
441	198	0.01	100	14.4	6531	PASS
442	198	50	100	92.2	41776	PASS
443	442	15	24	21.2	8858	PASS