

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012218\
 Data File : BG032219.D
 Acq On : 22 Jan 2018 20:08
 Operator : SJ/JU
 Sample : PB105779BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK79

Quant Time: Jan 23 04:48:45 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG012218.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 22 17:12:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.73	152	37578	20.00	ng/ul	0.00
18) Naphthalene-d8	11.61	136	158391	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.36	164	114212	20.00	ng/ul	0.00
61) Phenanthrene-d10	18.09	188	280982	20.00	ng/ul	0.00
77) Chrysene-d12	22.42	240	351127	20.00	ng/ul	0.00
85) Perylene-d12	26.11	264	365199	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.77	96	3397	5.47	ng/uL	0.00
5) Phenol-d5	7.83	99	73478	28.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	8.01	67	35217	28.91	ng/ul	0.00
9) 2-Chlorophenol-d4	8.24	132	66985	27.80	ng/ul	0.00
13) 4-Methylphenol-d8	9.43	113	72388	30.87	ng/ul	0.00
19) Nitrobenzene-d5	9.93	128	32972	28.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.66	143	41211	29.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.21	165	84708	27.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.73	131	98369	46.45	ng/ul	0.00
43) Dimethylphthalate-d6	14.74	166	286743	30.07	ng/ul	0.00
46) Acenaphthylene-d8	15.06	160	348013	29.77	ng/ul	0.00
51) 4-Nitrophenol-d4	15.51	143	30849	24.28	ng/ul	0.00
57) Fluorene-d10	16.34	176	259335	29.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.44	200	38017	21.93	ng/ul	0.00
70) Anthracene-d10	18.19	188	400732	29.66	ng/ul	0.00
78) Pyrene-d10	20.43	212	495437	30.40	ng/ul	0.00
89) Benzo(a)pyrene-d12	25.86	264	532078	31.52	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.42	70	1950	1.272 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG012218\
Data File : BG032219.D
Acq On : 22 Jan 2018 20:08
Operator : SJ/JU
Sample : PB105779BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK79

Quant Time: Jan 23 04:48:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG012218.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 22 17:12:25 2018
Response via : Initial Calibration

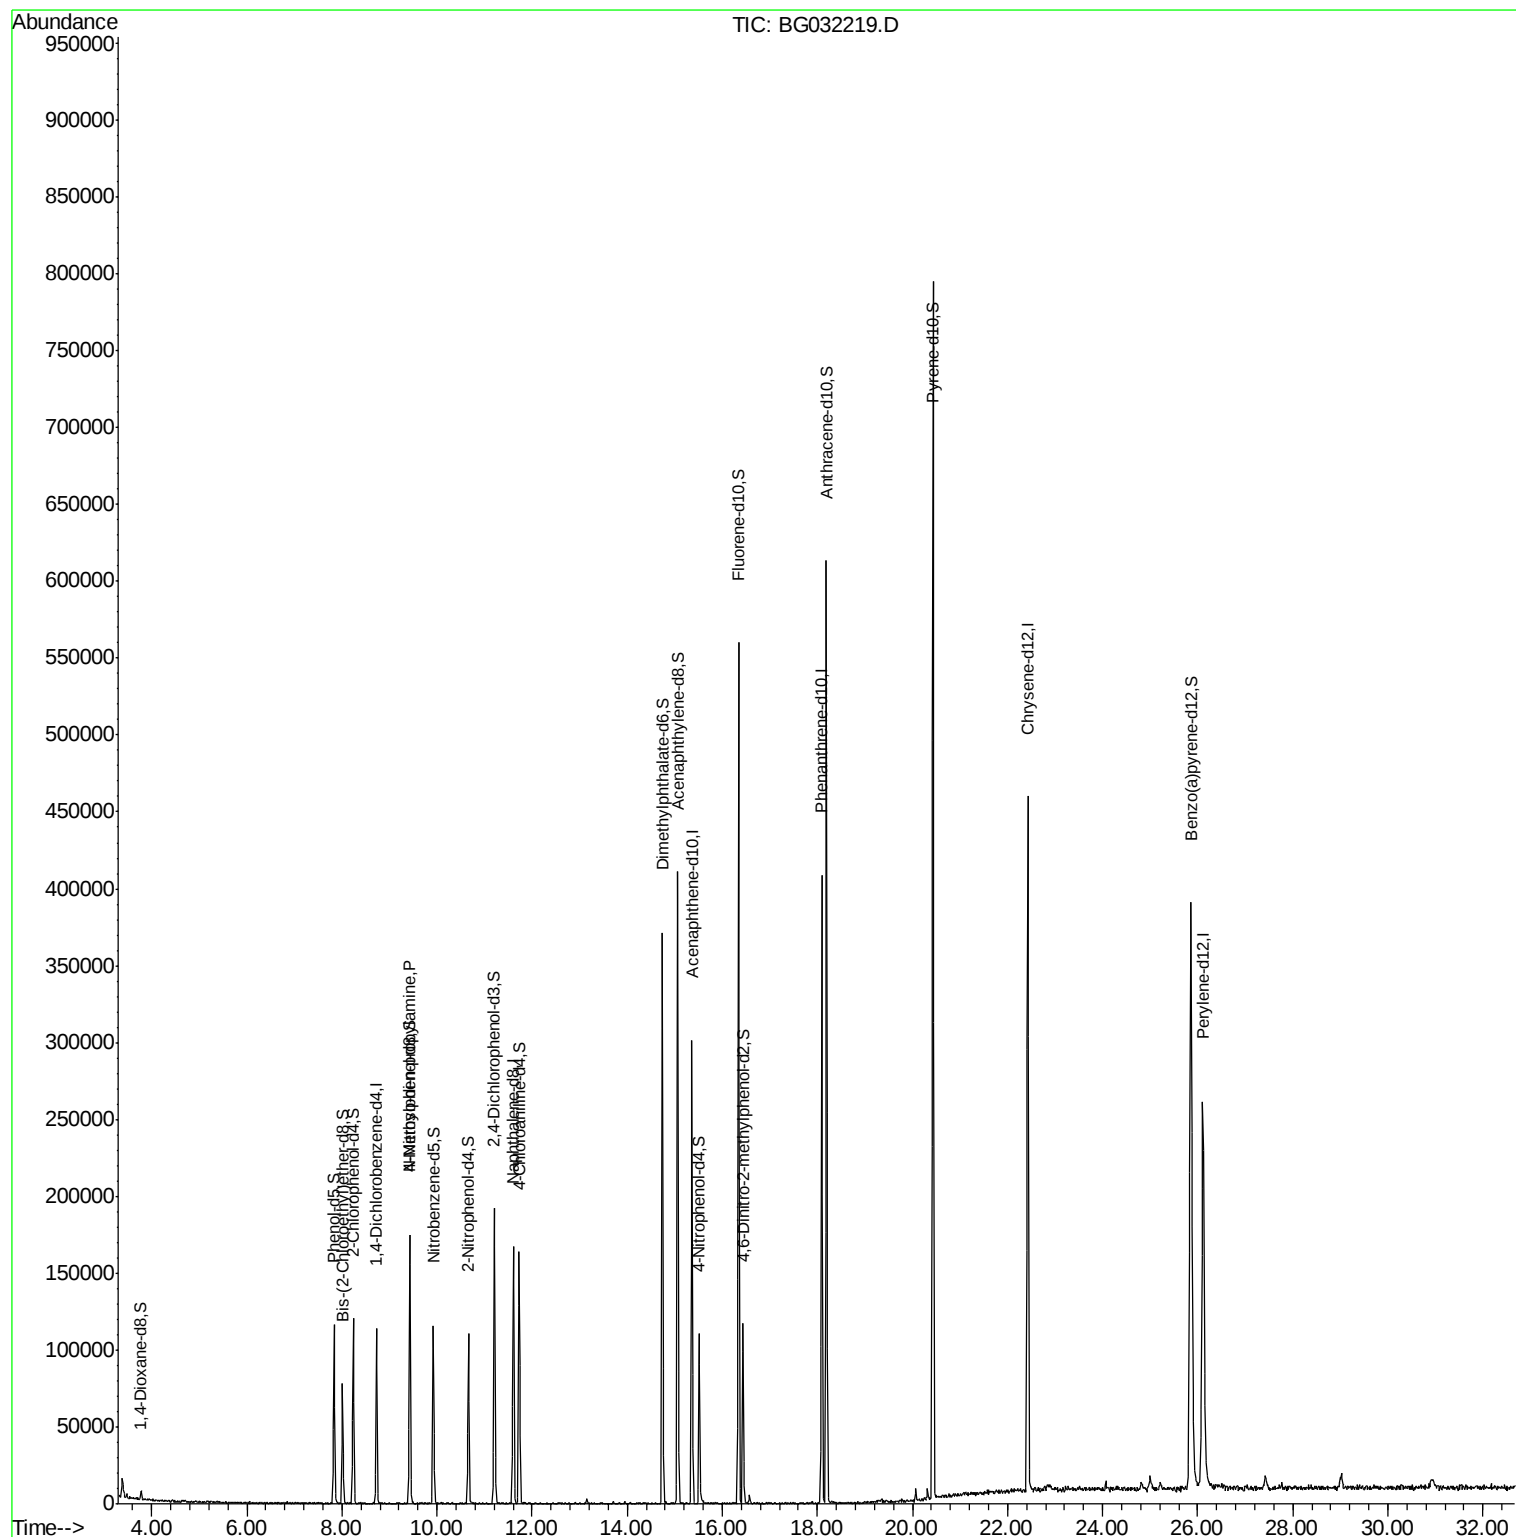

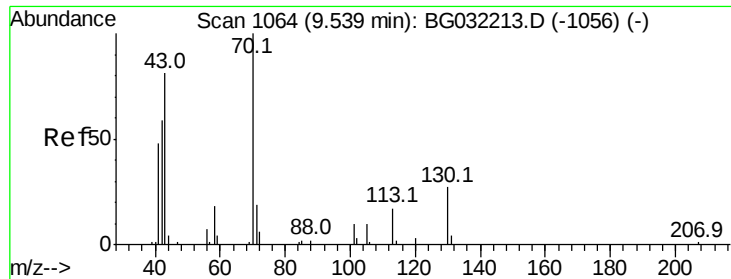

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.272 ng/ul
 RT: 9.42 min Scan# 1044
 Delta R.T. -0.12 min
 Lab File: BG032219.D
 Acq: 22 Jan 2018 20:08

Instrument :
 BNA_G
 ClientSampleId :
 SBLK79

Tot Ion: 70 Resp: 1950
 Ion Ratio Lower Upper
 70 100
 42 327.3 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

