
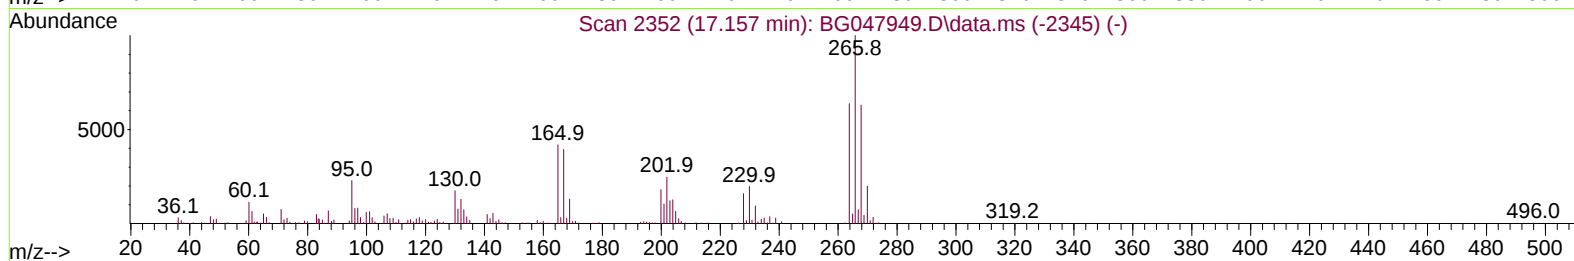
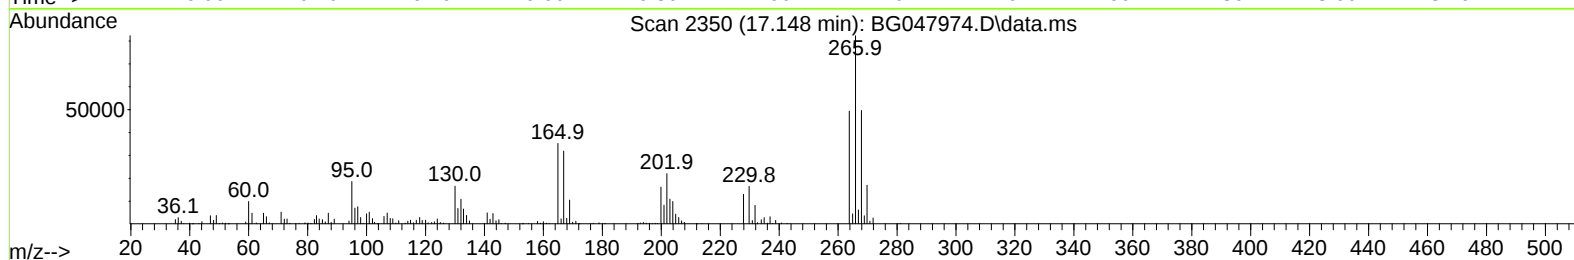


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047974.D
Acq On : 22 Jan 2021 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:33:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 21 14:42:53 2021
Response via : Initial Calibration

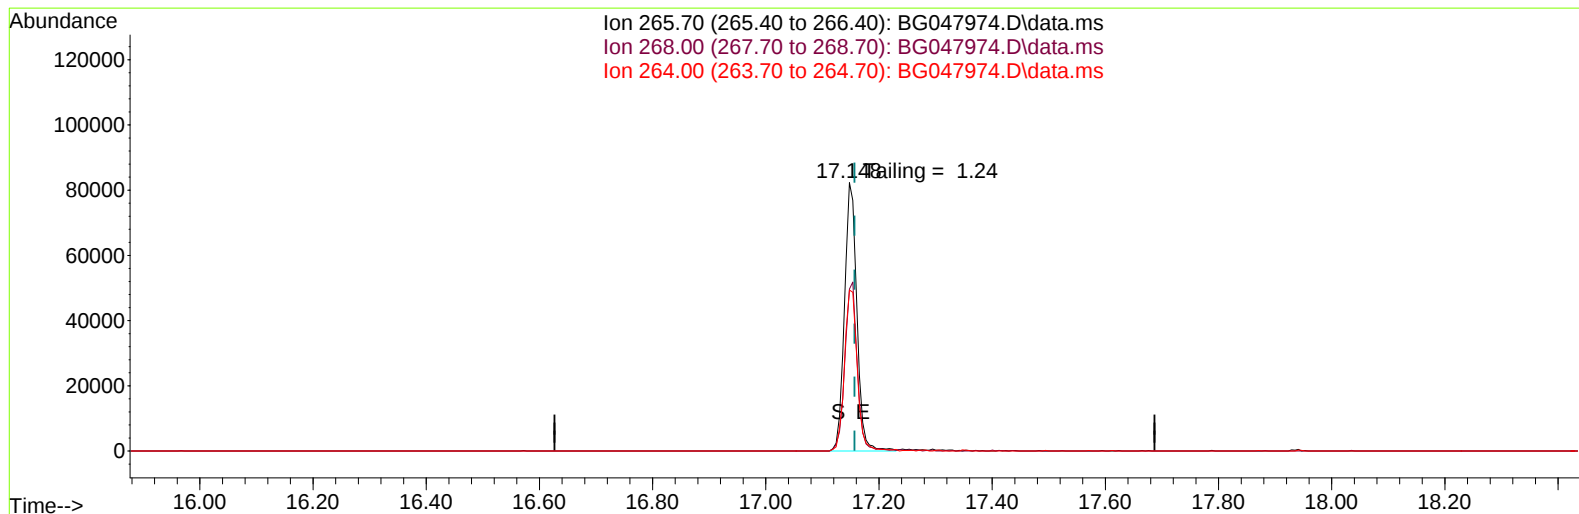

TIC: BG047974.D\data.ms

(70) Pentachlorophenol (C)




17.148min (-0.009) 281193.94 ng

response 125408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.36
264.00	61.60	59.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
 Data File : BG047974.D
 Acq On : 22 Jan 2021 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 23:33:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 21 14:42:53 2021
 Response via : Initial Calibration

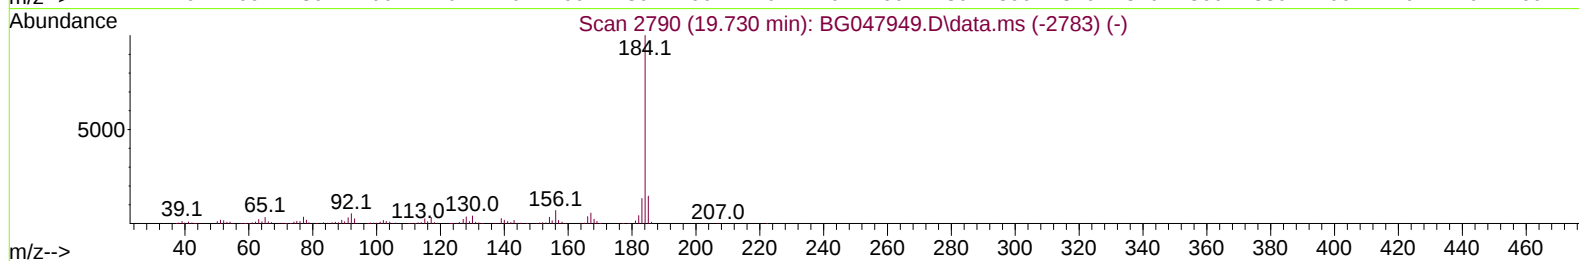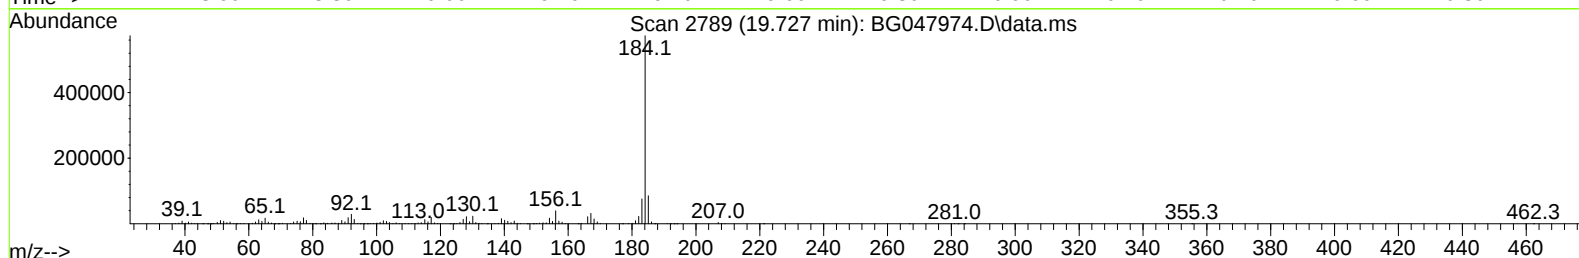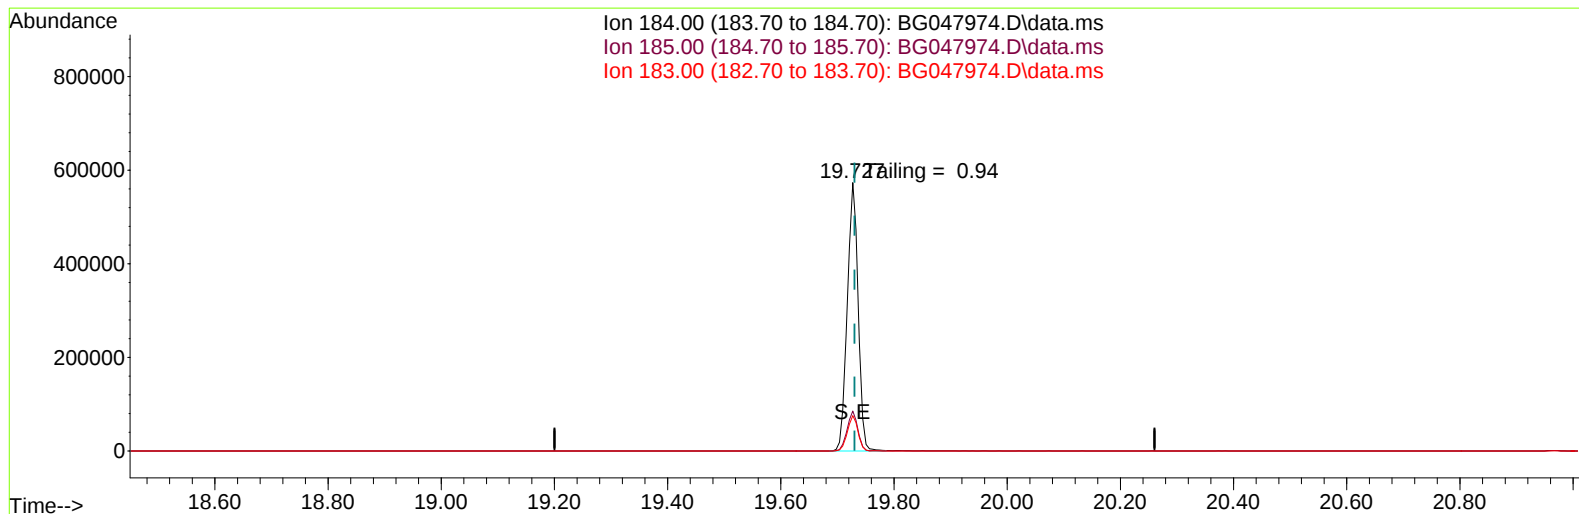

TIC: BG047974.D\data.ms

(77) Benzidine

19.727min (-0.003) 5136.29 ng m

response 766432

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.94
183.00	13.20	13.20
0.00	0.00	0.00