

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
 Data File : BG047985.D
 Acq On : 22 Jan 2021 19:41
 Operator : CG/JU
 Sample : M1207-03 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-SF-03-010-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG047985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.230	318	322	329	rVB2	21361	33746	3.27%	0.443%
2	5.694	394	401	412	rVB	118614	191387	18.53%	2.512%
3	7.280	663	671	679	rBV	140059	243720	23.59%	3.199%
4	8.144	811	818	824	rBV	245960	419563	40.62%	5.507%
5	9.301	1009	1015	1022	rVB	84596	148725	14.40%	1.952%
6	10.958	1286	1297	1306	rBV	309072	576254	55.78%	7.564%
7	11.975	1465	1470	1473	rBV3	7241	10346	1.00%	0.136%
8	12.362	1531	1536	1541	rVB6	6981	10549	1.02%	0.138%
9	13.302	1692	1696	1702	rVV4	13887	19849	1.92%	0.261%
10	13.391	1704	1711	1718	rVB	231998	368927	35.71%	4.842%
11	13.585	1741	1744	1750	rVB6	14729	18763	1.82%	0.246%
12	13.655	1751	1756	1760	rVV3	17144	24708	2.39%	0.324%
13	14.037	1818	1821	1825	rBV5	7556	12556	1.22%	0.165%
14	14.090	1826	1830	1835	rVV6	11076	20978	2.03%	0.275%
15	14.137	1835	1838	1845	rVB7	6518	10887	1.05%	0.143%
16	14.207	1845	1850	1853	rBV3	19278	33375	3.23%	0.438%
17	14.243	1853	1856	1859	rVB3	13809	17071	1.65%	0.224%
18	14.607	1912	1918	1923	rVB9	9406	17683	1.71%	0.232%
19	14.654	1923	1926	1931	rBV4	16831	25655	2.48%	0.337%
20	14.760	1935	1944	1951	rBV2	507498	816392	79.03%	10.716%
21	15.153	2008	2011	2016	rVB6	14407	21691	2.10%	0.285%
22	15.271	2028	2031	2038	rBV8	7328	10860	1.05%	0.143%
23	15.371	2046	2048	2054	rBV5	7350	12661	1.23%	0.166%
24	15.606	2084	2088	2092	rVB4	18155	24548	2.38%	0.322%
25	16.011	2153	2157	2162	rVB2	24107	32719	3.17%	0.429%
26	16.240	2190	2196	2204	rBV	71227	113957	11.03%	1.496%
27	16.463	2230	2234	2235	rBV2	24129	27176	2.63%	0.357%
28	16.487	2236	2238	2244	rVB2	49600	60758	5.88%	0.797%
29	16.610	2256	2259	2264	rBV7	8284	15665	1.52%	0.206%
30	16.746	2277	2282	2284	rBV6	8986	16403	1.59%	0.215%
31	16.863	2298	2302	2307	rVB8	11364	16217	1.57%	0.213%
32	17.257	2365	2369	2372	rBV4	20998	29188	2.83%	0.383%
33	17.315	2374	2379	2384	rVB3	35639	56692	5.49%	0.744%
34	17.503	2405	2411	2416	rBV	619370	970305	93.93%	12.736%
35	17.545	2416	2418	2422	rVB	48410	60896	5.89%	0.799%
36	17.633	2431	2433	2438	rVB2	13349	15992	1.55%	0.210%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
 Data File : BG047985.D
 Acq On : 22 Jan 2021 19:41
 Operator : CG/JU
 Sample : M1207-03 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-SF-03-010-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.909	2477	2480	2485	rVB7	14063	22700	2.20%	0.298%
38	17.997	2491	2495	2501	rBV4	29752	41238	3.99%	0.541%
39	18.379	2557	2560	2565	rBV5	45876	69573	6.73%	0.913%
40	18.602	2597	2598	2604	rVB5	18315	19327	1.87%	0.254%
41	18.684	2609	2612	2615	rBV3	31223	37347	3.62%	0.490%
42	19.284	2711	2714	2717	rBV2	26137	43243	4.19%	0.568%
43	19.548	2754	2759	2764	rVB	144097	208670	20.20%	2.739%
44	19.907	2813	2820	2828	rBV	125444	252157	24.41%	3.310%
45	20.106	2849	2854	2859	rVB	391580	514521	49.81%	6.753%
46	21.787	3134	3140	3145	rVB2	619472	1033016	100.00%	13.559%
47	25.089	3696	3702	3711	rVB	330432	870008	84.22%	11.419%




Sum of corrected areas: 7618662

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047985.D
Acq On : 22 Jan 2021 19:41
Operator : CG/JU
Sample : M1207-03 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-010-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

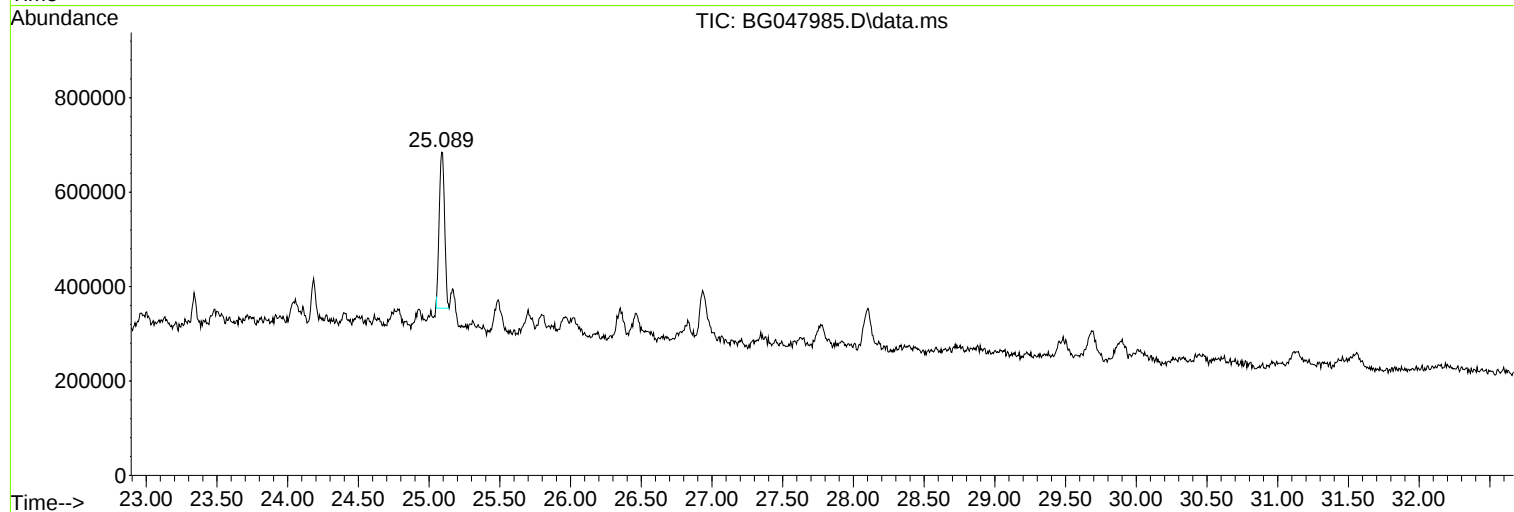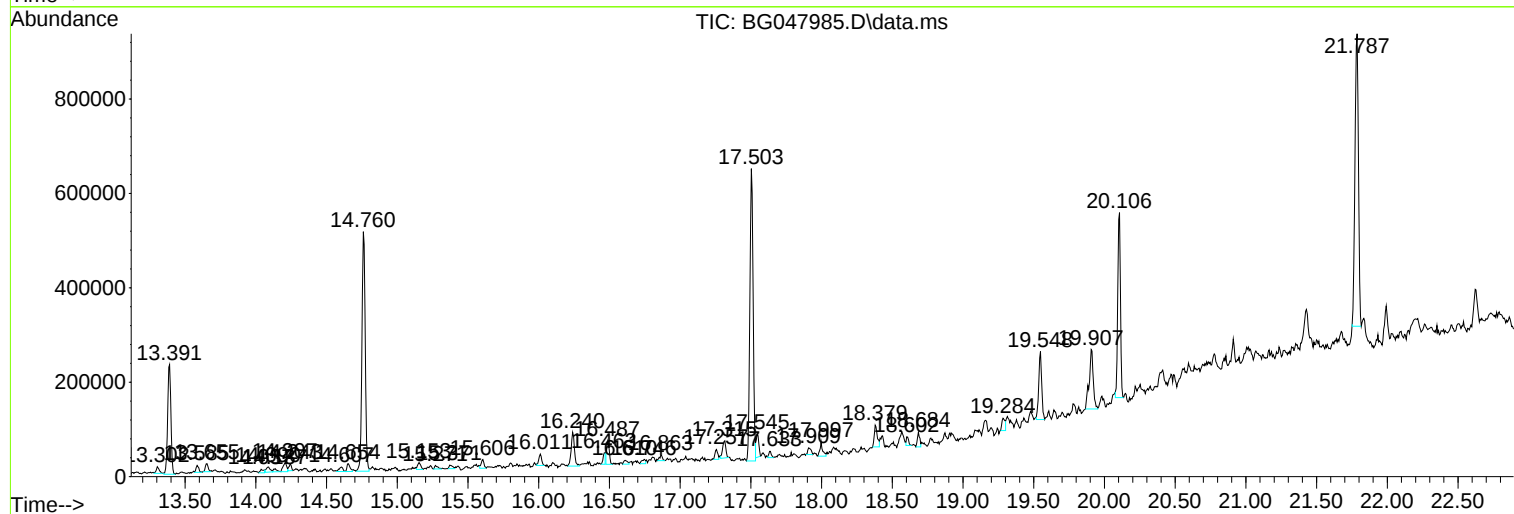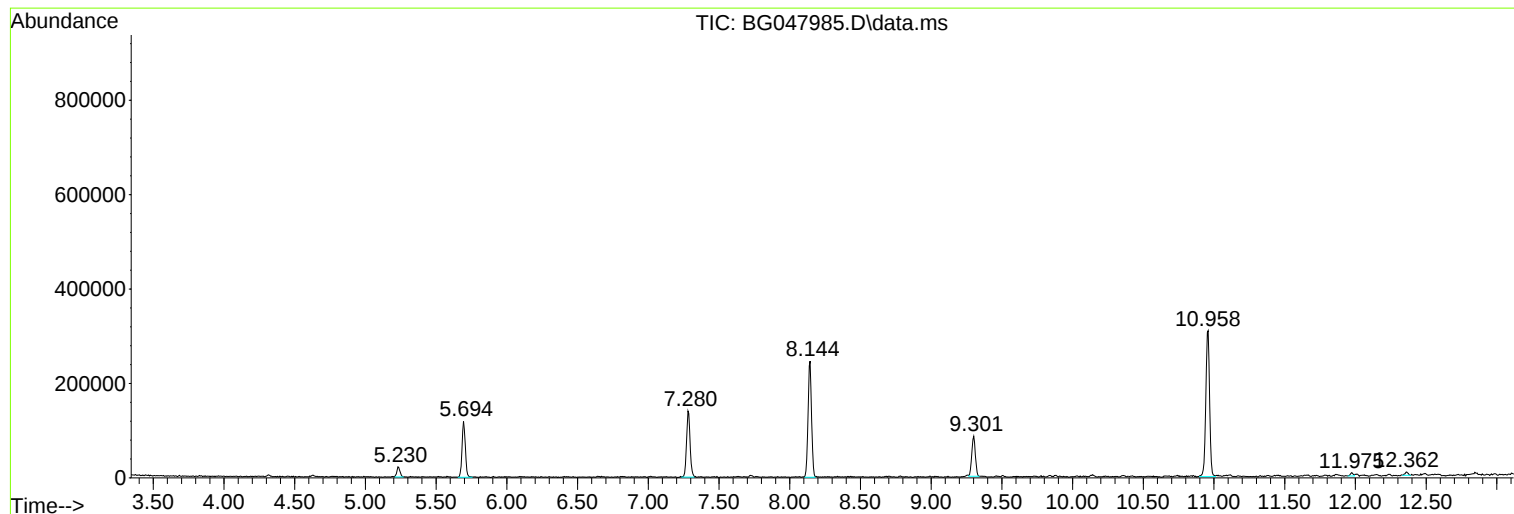

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047985.D
Acq On : 22 Jan 2021 19:41
Operator : CG/JU
Sample : M1207-03 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-010-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047985.D
Acq On : 22 Jan 2021 19:41
Operator : CG/JU
Sample : M1207-03 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-010-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------