

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
 Data File : BG047986.D
 Acq On : 22 Jan 2021 20:21
 Operator : CG/JU
 Sample : M1208-03 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-SF-03-011-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG047986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.231	316	322	328	rVB2	8180	14273	1.24%	0.183%
2	5.695	394	401	410	rBV	124477	201724	17.51%	2.590%
3	7.287	664	672	683	rVB	151275	259833	22.55%	3.336%
4	8.145	809	818	825	rBV	278848	471560	40.93%	6.054%
5	9.302	1009	1015	1022	rVB	90133	155767	13.52%	2.000%
6	10.959	1286	1297	1304	rBV	366878	662843	57.53%	8.510%
7	13.309	1692	1697	1703	rVB7	10022	18067	1.57%	0.232%
8	13.392	1703	1711	1718	rBV	231444	370936	32.20%	4.762%
9	13.585	1741	1744	1753	rVB6	12105	19858	1.72%	0.255%
10	13.715	1761	1766	1769	rVB5	7105	11768	1.02%	0.151%
11	14.091	1825	1830	1835	rVB3	9584	14911	1.29%	0.191%
12	14.144	1835	1839	1844	rVB7	6975	12150	1.05%	0.156%
13	14.208	1844	1850	1851	rBV6	9249	16372	1.42%	0.210%
14	14.655	1923	1926	1930	rVB2	12742	15375	1.33%	0.197%
15	14.766	1935	1945	1952	rBV	590054	933172	80.99%	11.981%
16	15.160	2008	2012	2016	rVB7	15607	21475	1.86%	0.276%
17	15.236	2019	2025	2028	rBV4	10658	15847	1.38%	0.203%
18	15.383	2044	2050	2052	rBV6	9158	14996	1.30%	0.193%
19	15.430	2054	2058	2062	rVB6	10217	13989	1.21%	0.180%
20	15.607	2085	2088	2092	rVB4	11726	17131	1.49%	0.220%
21	15.806	2117	2122	2126	rBV7	11978	23132	2.01%	0.297%
22	16.018	2153	2158	2161	rVB4	12392	21874	1.90%	0.281%
23	16.241	2188	2196	2203	rBV2	93550	158338	13.74%	2.033%
24	16.464	2231	2234	2235	rBV3	18399	18104	1.57%	0.232%
25	16.488	2235	2238	2245	rVB6	32905	50583	4.39%	0.649%
26	17.316	2373	2379	2385	rVB6	23557	41788	3.63%	0.537%
27	17.510	2405	2412	2416	rBV	698007	1052549	91.36%	13.514%
28	17.551	2416	2419	2423	rVB	62017	79888	6.93%	1.026%
29	17.645	2430	2435	2438	rVB	15335	22972	1.99%	0.295%
30	17.998	2492	2495	2500	rBV4	13632	18625	1.62%	0.239%
31	18.386	2556	2561	2565	rBV3	61610	97861	8.49%	1.256%
32	19.291	2711	2715	2718	rBV3	41532	72535	6.30%	0.931%
33	19.549	2755	2759	2766	rBV	125614	172974	15.01%	2.221%
34	19.913	2818	2821	2828	rVB	124229	178345	15.48%	2.290%
35	20.107	2850	2854	2858	rVB2	363712	451531	39.19%	5.797%
36	21.788	3134	3140	3146	rBV2	674759	1152136	100.00%	14.792%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047986.D
Acq On : 22 Jan 2021 20:21
Operator : CG/JU
Sample : M1208-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-011-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37 25.101 3697 3704 3711 rVB2 350132 913408 79.28% 11.727%




Sum of corrected areas: 7788690

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047986.D
Acq On : 22 Jan 2021 20:21
Operator : CG/JU
Sample : M1208-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-011-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

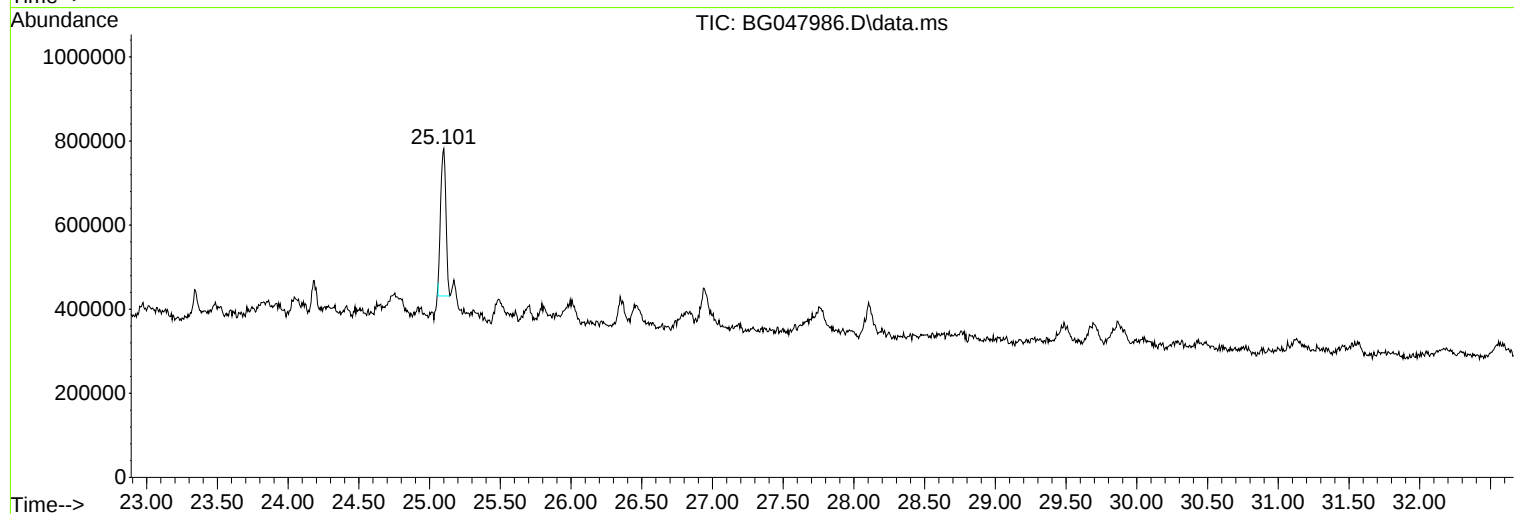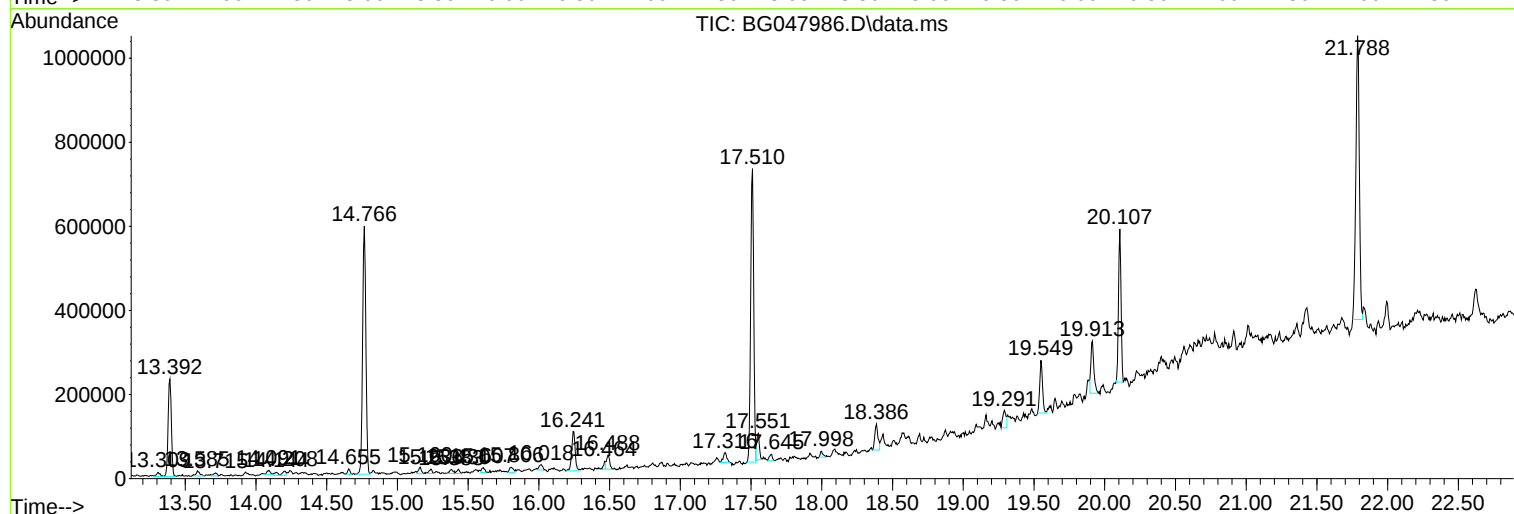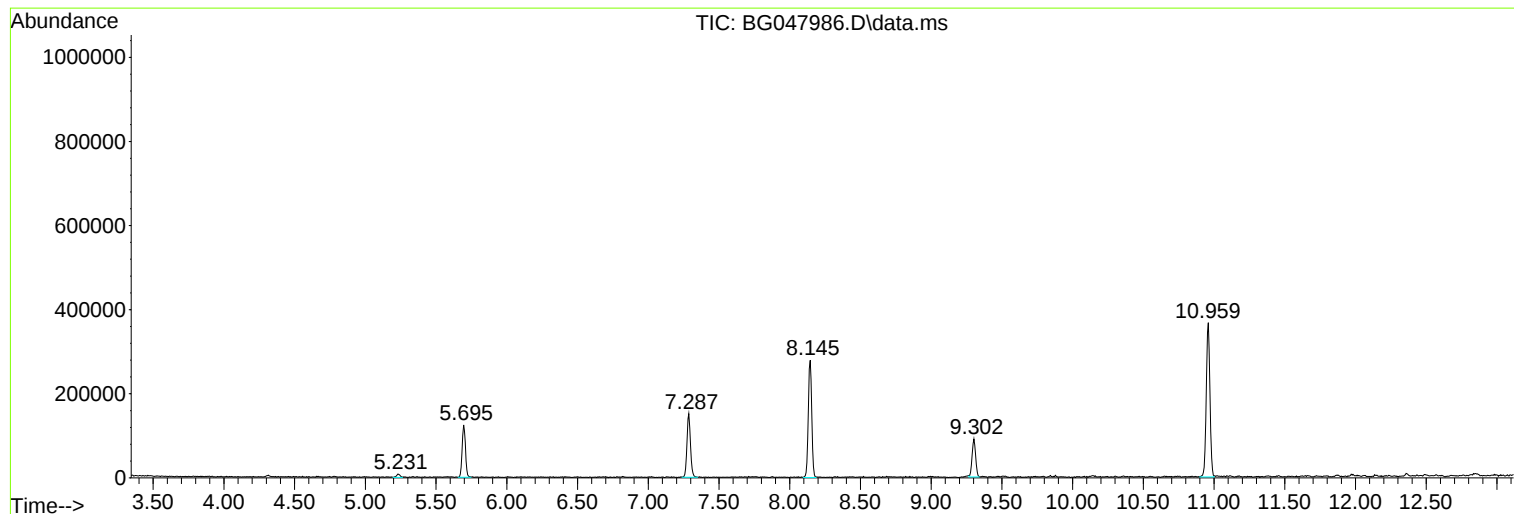

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047986.D
Acq On : 22 Jan 2021 20:21
Operator : CG/JU
Sample : M1208-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-011-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
Data File : BG047986.D
Acq On : 22 Jan 2021 20:21
Operator : CG/JU
Sample : M1208-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-03-011-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
