
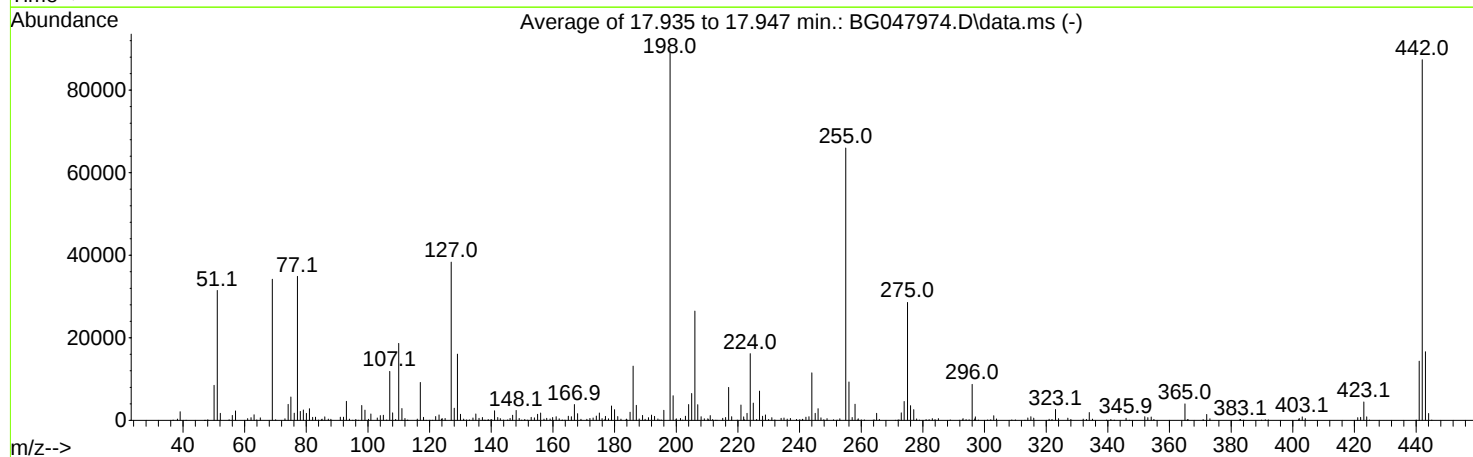


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012221\
 Data File : BG047974.D
 Acq On : 22 Jan 2021 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 21 14:42:53 2021

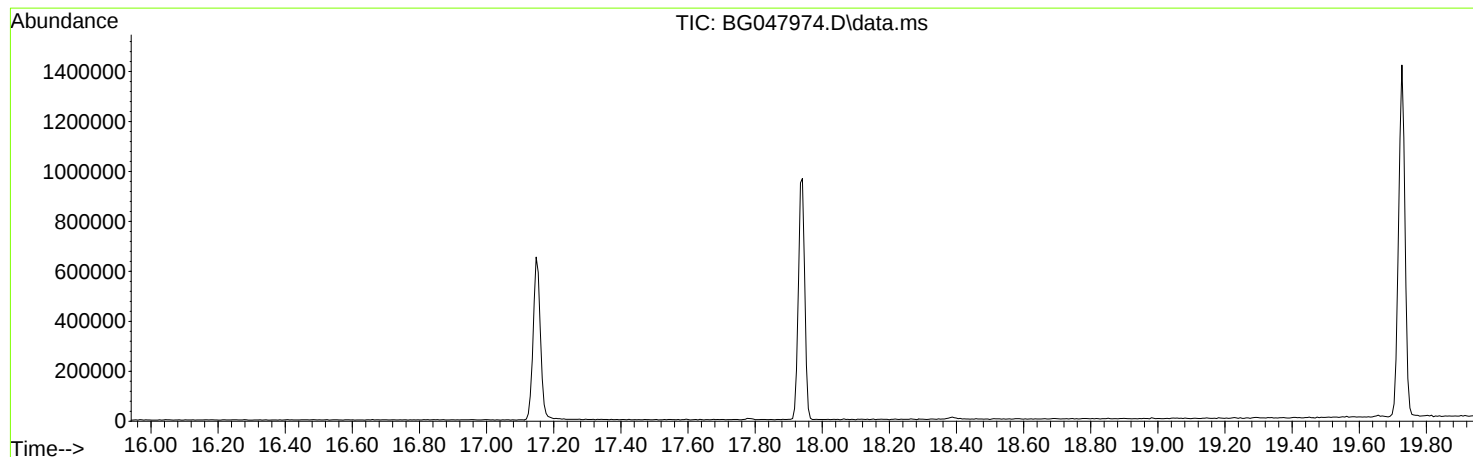

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	31467	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.4	34200	PASS
70	69	0.00	2	0.5	162	PASS
127	198	10	80	43.0	38347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89123	PASS
199	198	5	9	6.7	5957	PASS
275	198	10	60	32.1	28576	PASS
365	198	1	100	4.5	3995	PASS
441	198	0.01	100	16.1	14345	PASS
442	198	50	100	98.0	87379	PASS
443	442	15	24	19.0	16635	PASS