
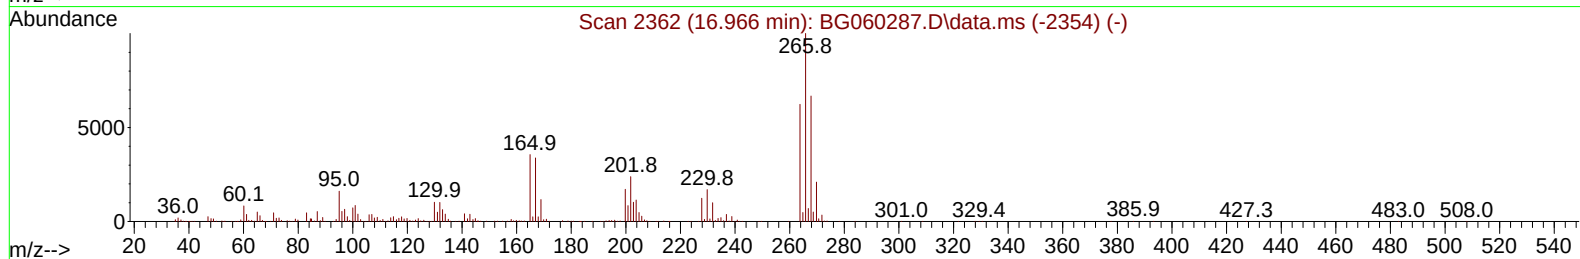
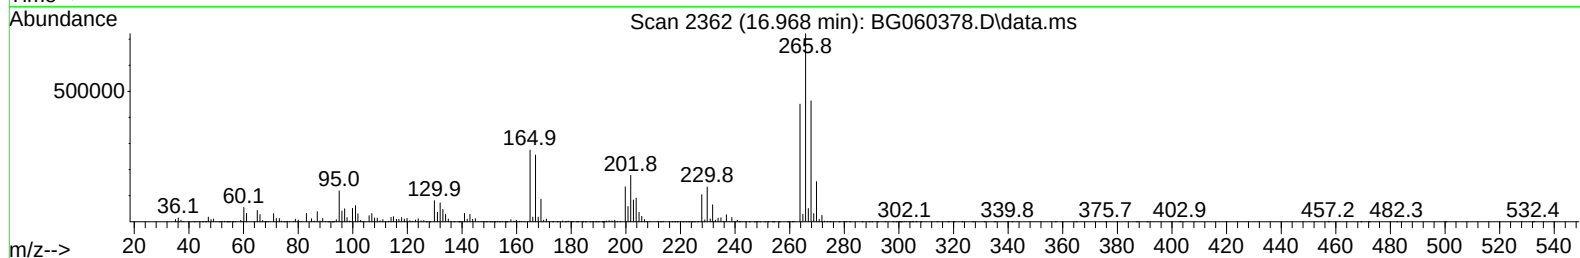


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060378.D
Acq On : 22 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 11:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

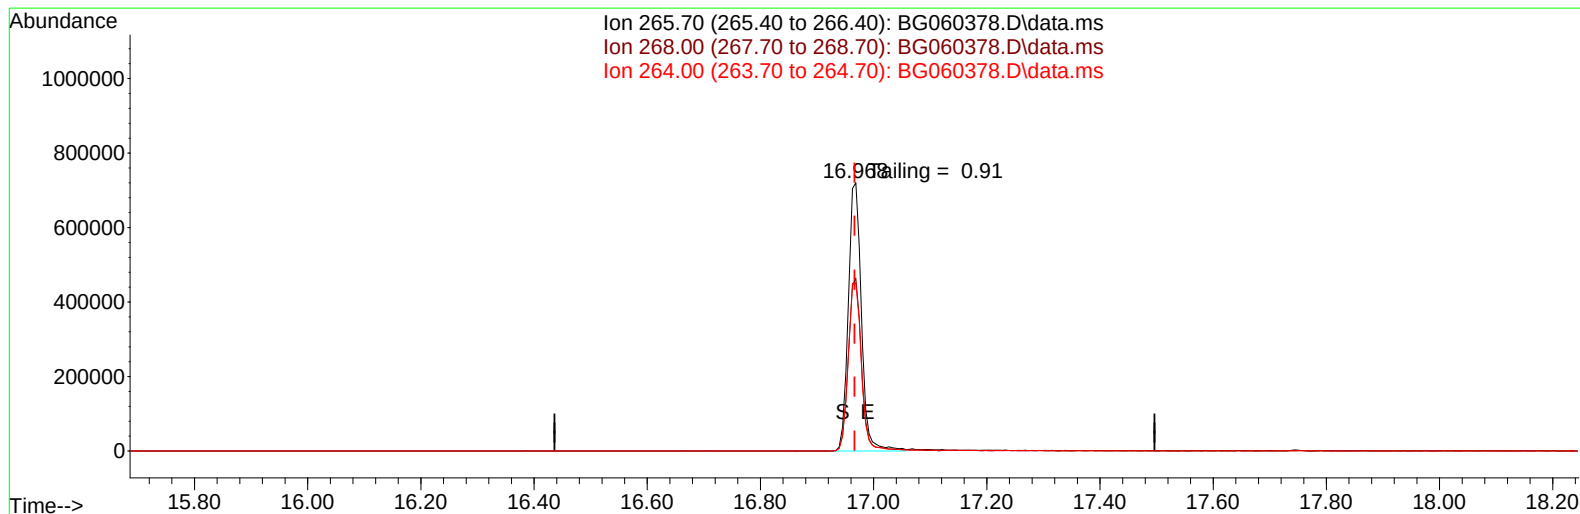




TIC: BG060378.D\data.ms

(70) Pentachlorophenol (C)**16.968min (+ 0.002) 753839.74 ng****response 1162710**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.39
264.00	62.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060378.D
Acq On : 22 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 11:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

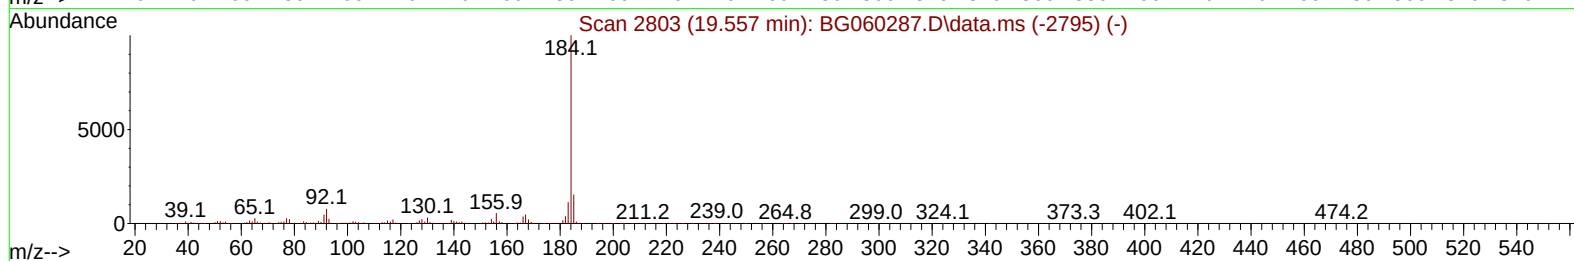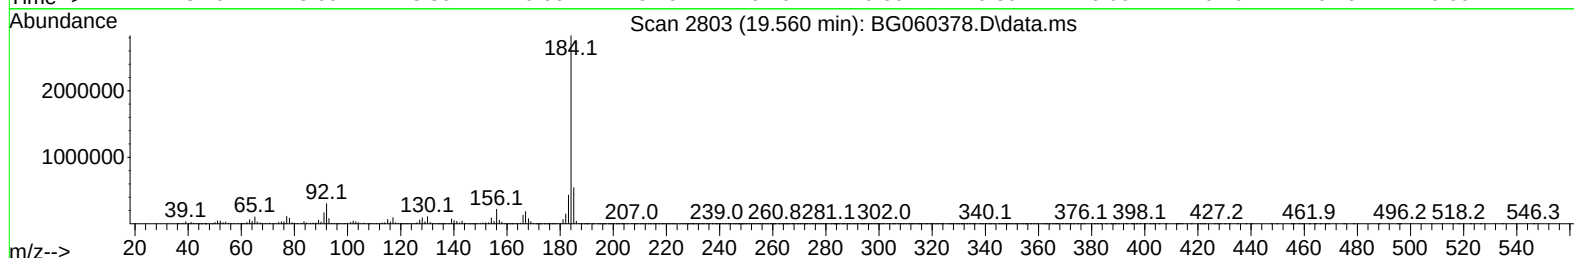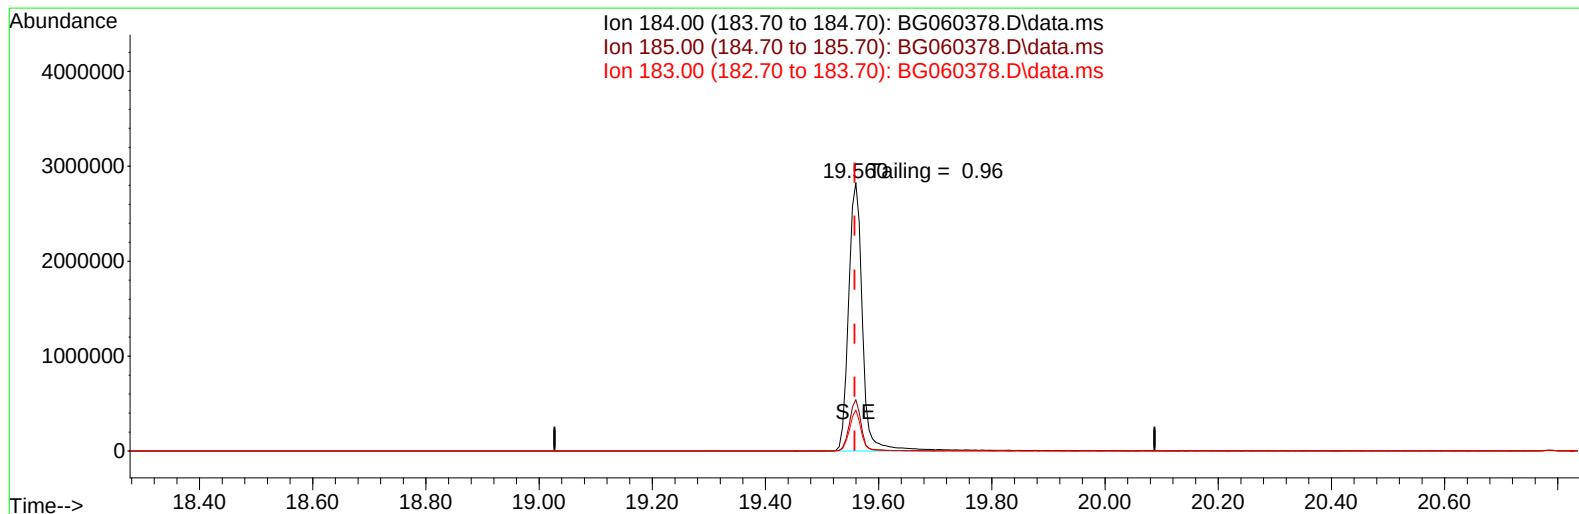

TIC: BG060378.D\data.ms

(77) Benzidine

19.560min (+ 0.002) 187901.14 ng m

response 4792492

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	19.14#
183.00	11.20	15.27#
0.00	0.00	0.00