

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
 Data File : BG060394.D
 Acq On : 22 Jan 2024 21:09
 Operator : MA/JU
 Sample : P1200-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CHRT-24376

Quant Time: Jan 23 00:40:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 09 04:07:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	456251	20.000	ng	0.00
21) Naphthalene-d8	10.732	136	1925093	20.000	ng	0.00
39) Acenaphthene-d10	14.569	164	1312320	20.000	ng	0.00
64) Phenanthrene-d10	17.330	188	2518238	20.000	ng	# 0.02
76) Chrysene-d12	21.584	240	2512415	20.000	ng	0.00
86) Perylene-d12	24.757	264	3028455	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.503	112	1253623	45.193	ng	0.00
7) Phenol-d6	7.095	99	1600998	38.977	ng	0.00
23) Nitrobenzene-d5	9.093	82	1061411	26.035	ng	0.00
42) 2,4,6-Tribromophenol	16.061	330	691530	35.816	ng	0.00
45) 2-Fluorobiphenyl	13.188	172	2255941	23.900	ng	0.00
79) Terphenyl-d14	19.945	244	2789820	19.223	ng	0.01


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060394.D
Acq On : 22 Jan 2024 21:09
Operator : MA/JU
Sample : P1200-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CHRT-24376

Quant Time: Jan 23 00:40:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration




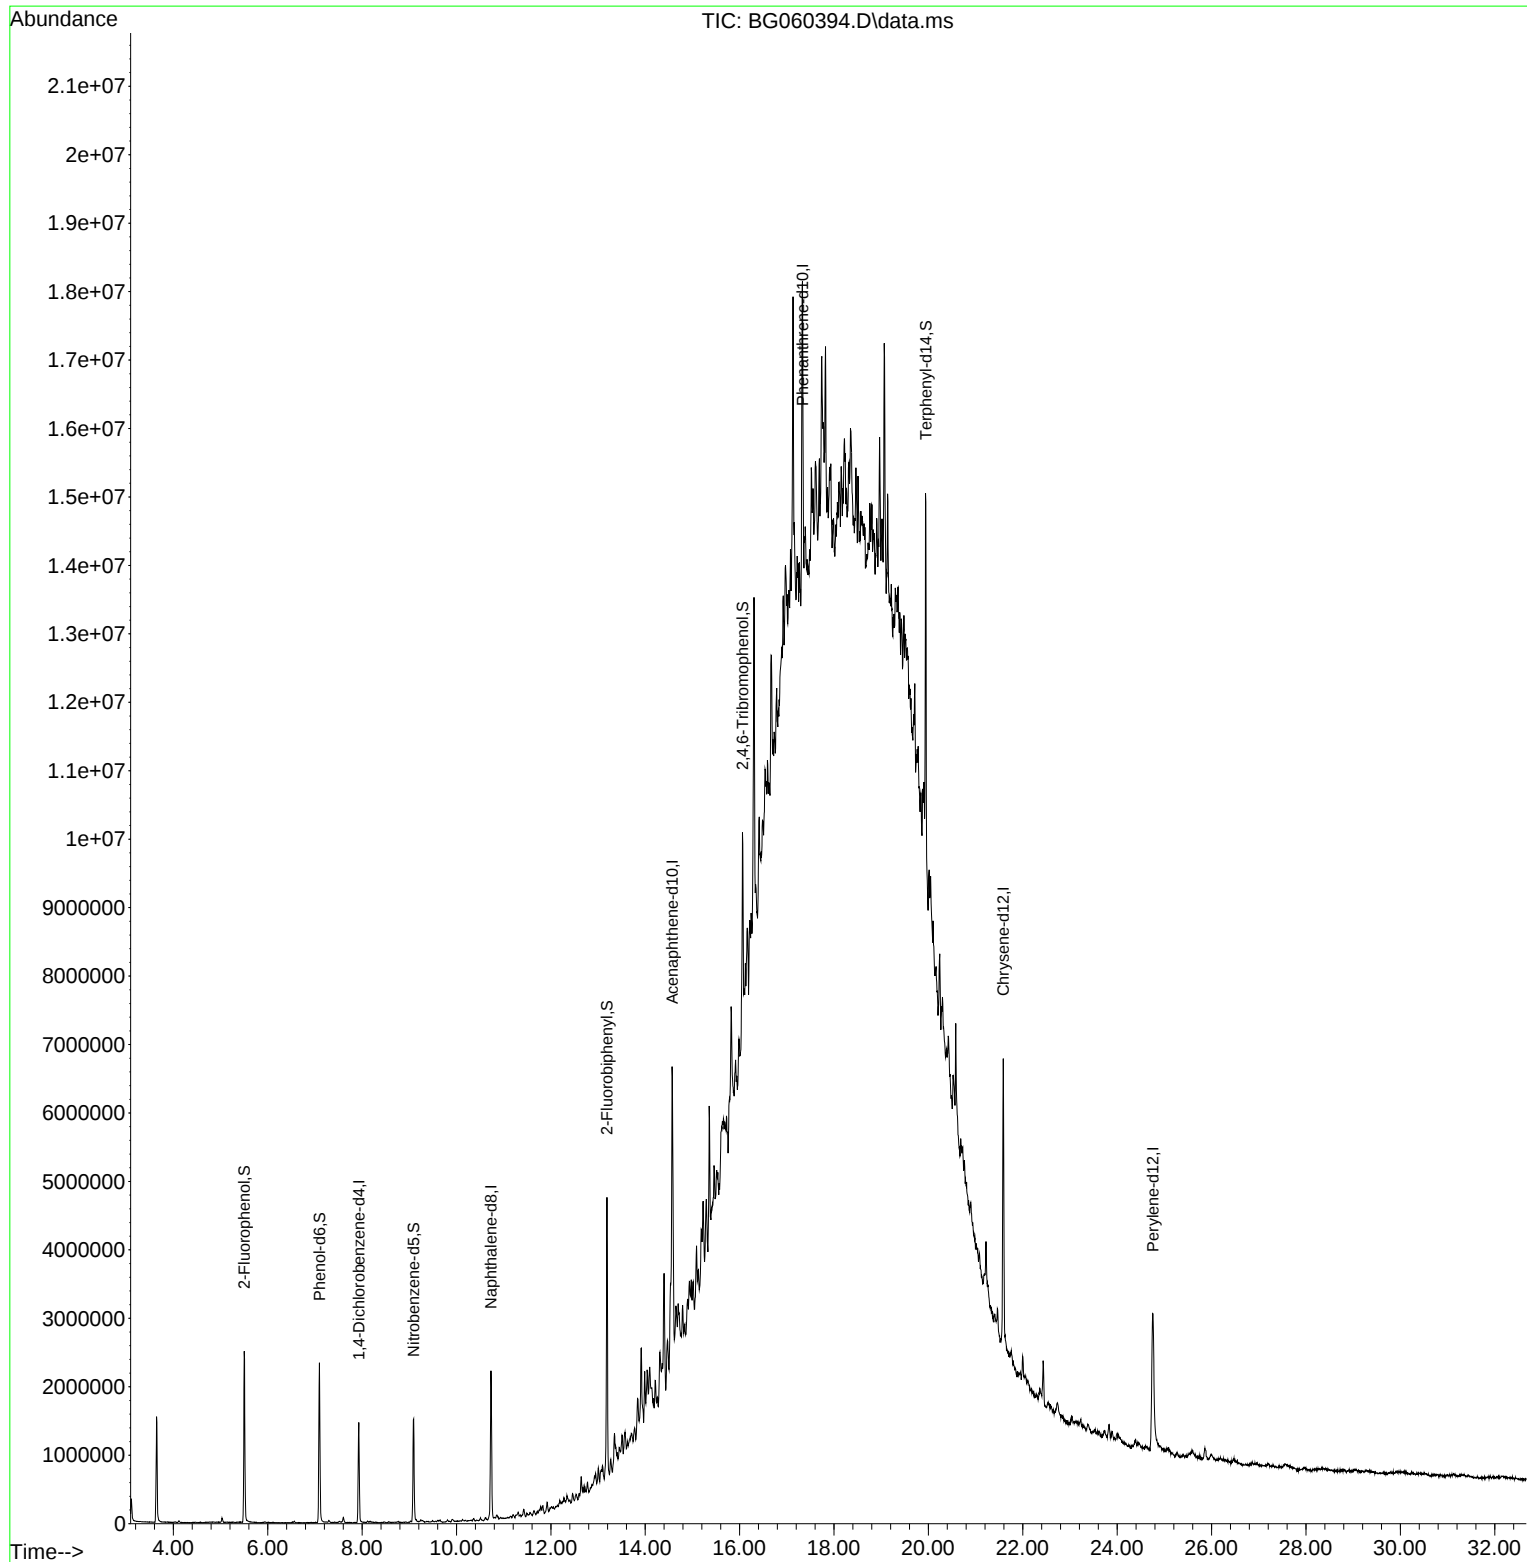




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.929 min Scan# 81
Delta R.T. -0.001 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09




Instrument :
BNA_G
ClientSampleId :
CHRT-24376


Tgt Ion:152 Resp: 456251
Ion Ratio Lower Upper
152 100
150 149.4 114.5 171.7
115 53.2 43.0 64.6

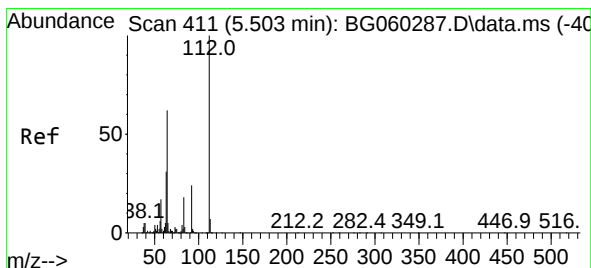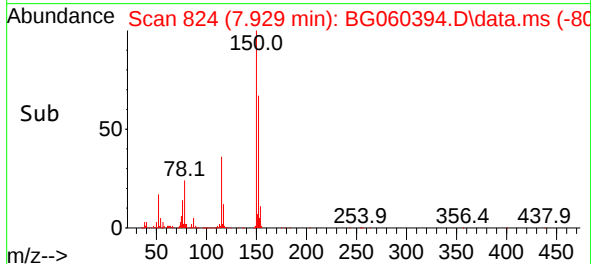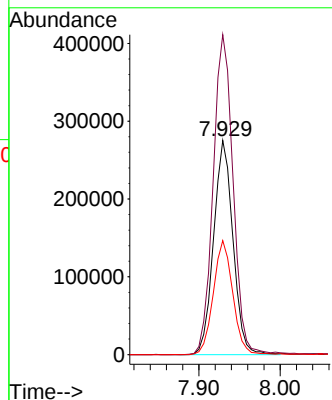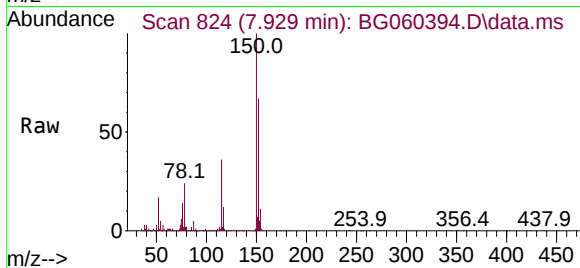

#5
2-Fluorophenol
Concen: 45.193 ng
RT: 5.503 min Scan# 411
Delta R.T. -0.000 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09

Tgt Ion:112 Resp: 1253623
Ion Ratio Lower Upper
112 100
64 62.1 49.8 74.6
63 30.8 24.4 36.6


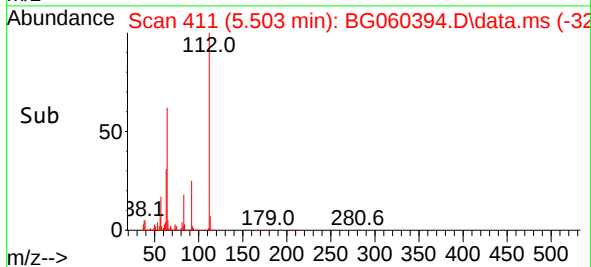
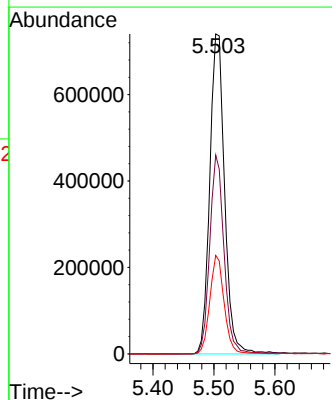
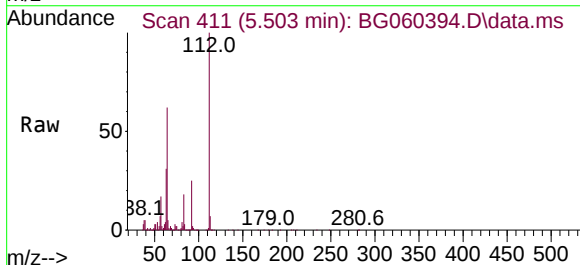




#7
Phenol-d6
Concen: 38.977 ng
RT: 7.095 min Scan# 682
Delta R.T. -0.000 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09




Instrument :
BNA_G
ClientSampleId :
CHRT-24376


Tgt Ion: 99 Resp: 1600998
Ion Ratio Lower Upper
99 100
42 13.0 10.9 16.3
71 28.1 21.5 32.3

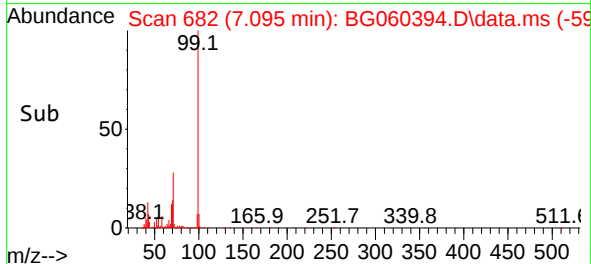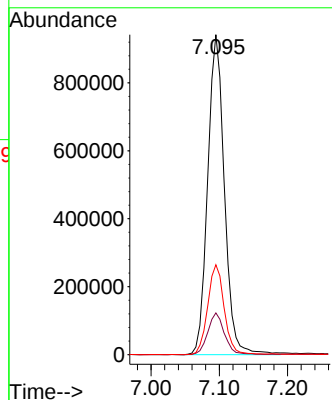

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.732 min Scan# 1301
Delta R.T. -0.000 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09

Tgt Ion:136 Resp: 1925093
Ion Ratio Lower Upper
136 100
137 10.9 8.2 12.4
54 8.4 6.2 9.2
68 7.6 6.3 9.5

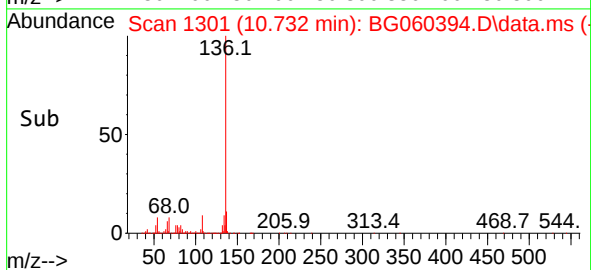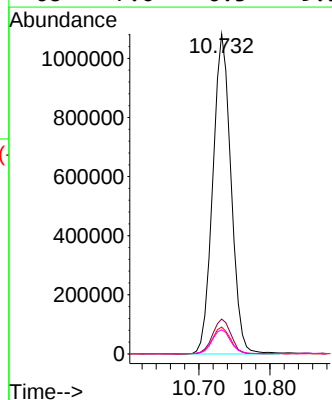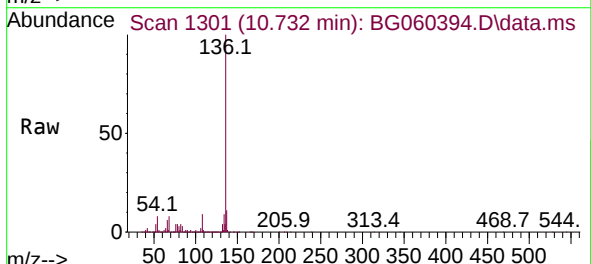



#23

Nitrobenzene-d5

Concen: 26.035 ng

RT: 9.093 min Scan# 1022

Delta R.T. -0.000 min

Lab File: BG060394.D

Acq: 22 Jan 2024 21:09

Instrument :





BNA_G

ClientSampleId :

CHRT-24376

Tgt Ion: 82 Resp: 1061411

Ion	Ratio	Lower	Upper
82	100		
128	38.3	29.6	44.4
54	42.3	33.6	50.4

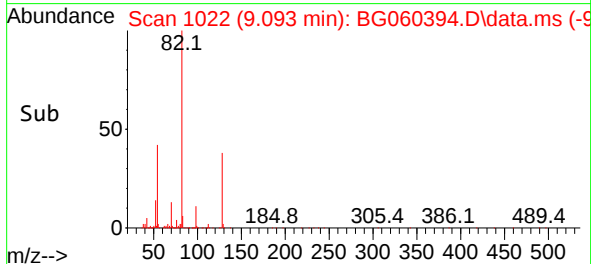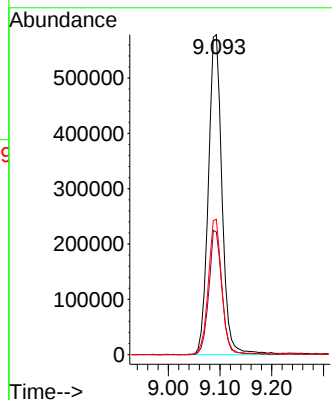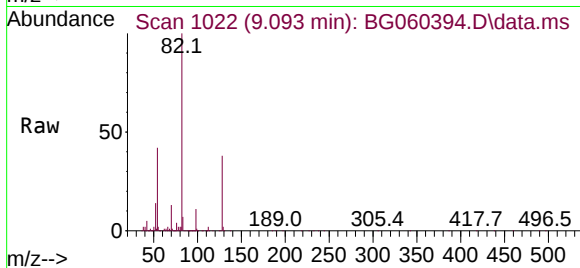

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.569 min Scan# 1954




Delta R.T. -0.000 min


Lab File: BG060394.D

Acq: 22 Jan 2024 21:09

Tgt Ion:164 Resp: 1312320

Ion	Ratio	Lower	Upper
164	100		
162	100.3	84.4	126.6
160	42.6	34.6	52.0


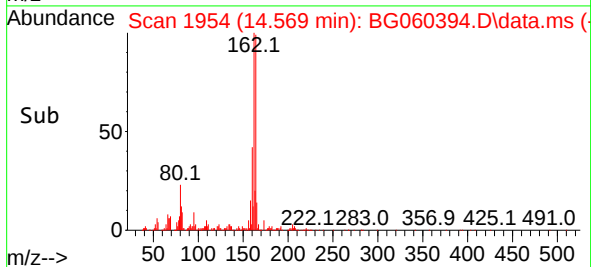
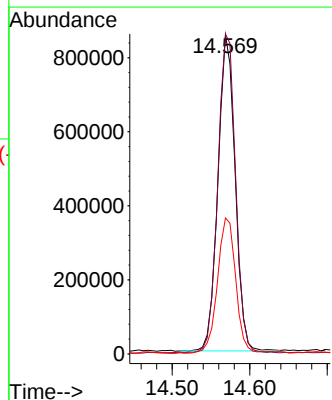
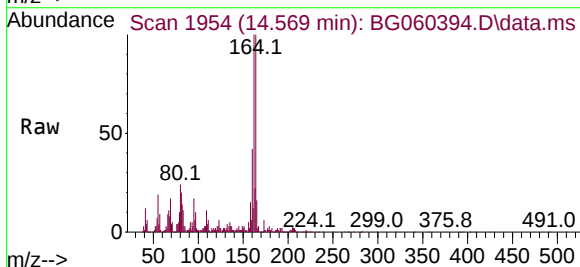




#42
2,4,6-Tribromophenol
Concen: 35.816 ng
RT: 16.061 min Scan# 21
Delta R.T. 0.006 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09




Instrument :
BNA_G
ClientSampleId :
CHRT-24376


Tgt Ion:330 Resp: 691530
Ion Ratio Lower Upper
330 100
332 96.5 76.7 115.1
141 24.7 18.6 28.0

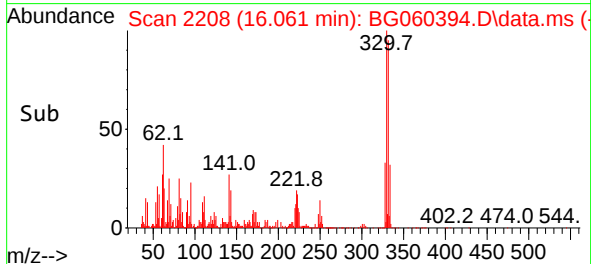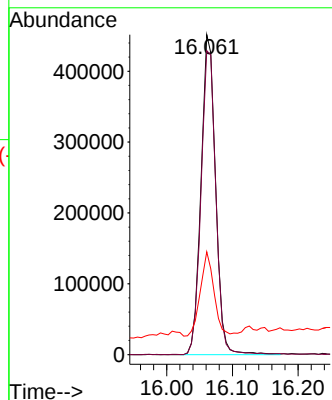

#45
2-Fluorobiphenyl
Concen: 23.900 ng
RT: 13.188 min Scan# 1719
Delta R.T. -0.000 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09

Tgt Ion:172 Resp: 2255941
Ion Ratio Lower Upper
172 100
171 36.8 34.6 51.8
170 25.5 24.4 36.6

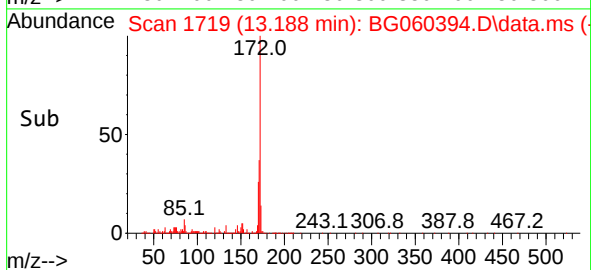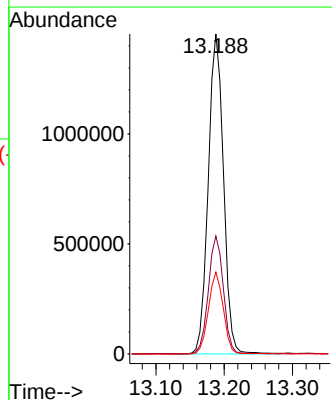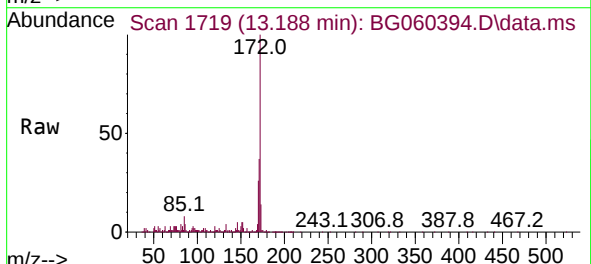




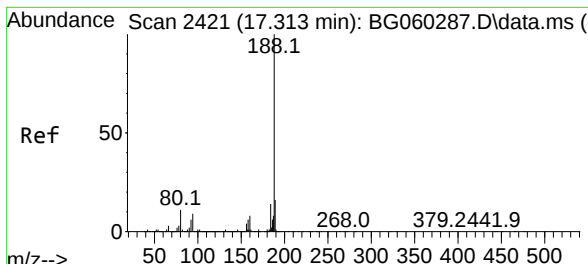


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.330 min Scan# 24
Delta R.T. 0.017 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09

Instrument :
BNA_G
ClientSampleId :
CHRT-24376

Tgt Ion:188 Resp: 2518238




Ion	Ratio	Lower	Upper
188	100		
94	13.8	7.1	10.7#
80	14.8	8.5	12.7#

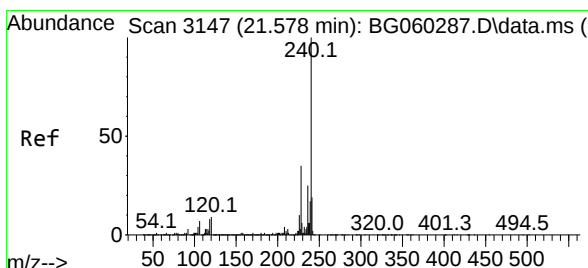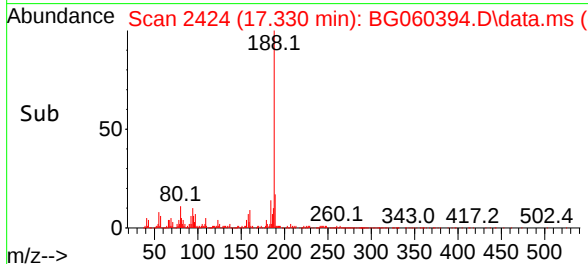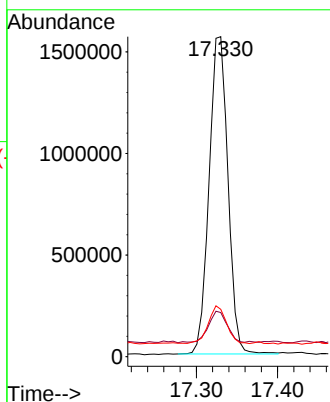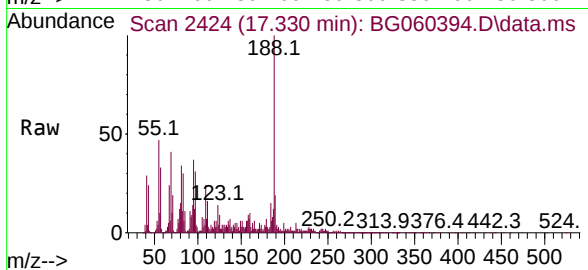


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.584 min Scan# 3148
Delta R.T. 0.006 min
Lab File: BG060394.D
Acq: 22 Jan 2024 21:09

Tgt Ion:240 Resp: 2512415

Ion	Ratio	Lower	Upper
240	100		
120	10.8	7.3	10.9
236	28.2	20.3	30.5

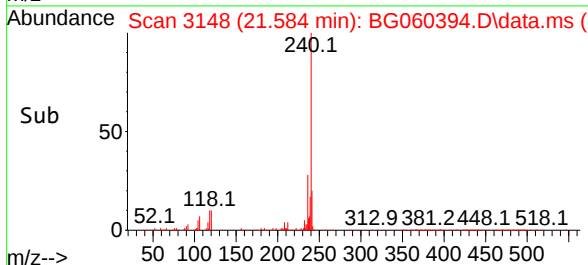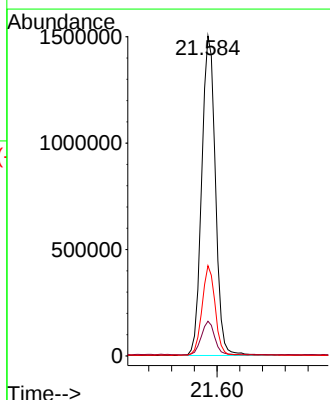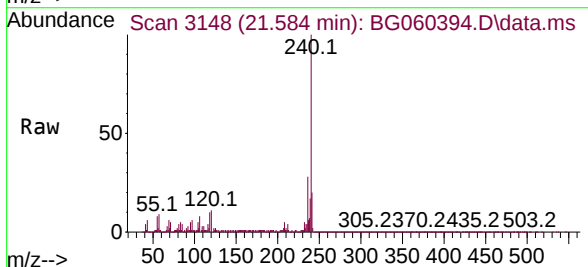

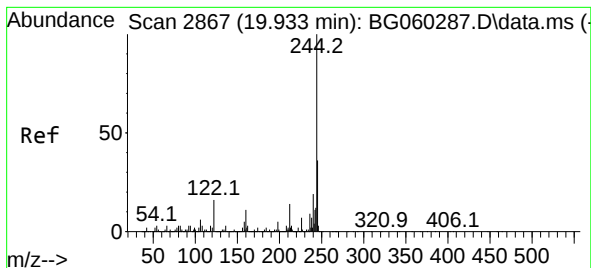

#79

Terphenyl-d14

Concen: 19.223 ng

RT: 19.945 min Scan# 2867

Delta R.T. 0.012 min

Lab File: BG060394.D

Acq: 22 Jan 2024 21:09

Instrument :

BNA_G

ClientSampleId :

CHRT-24376





Tgt Ion:244 Resp: 2789820

Ion Ratio Lower Upper

244 100

212 8.3 10.9 16.3#

122 10.7 12.6 18.8#

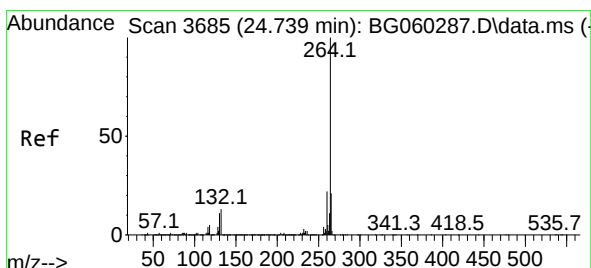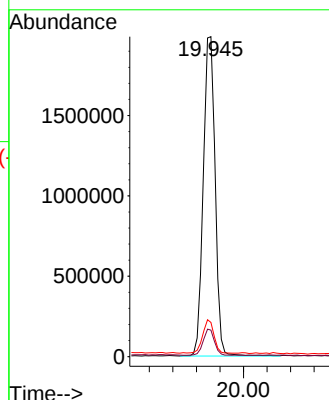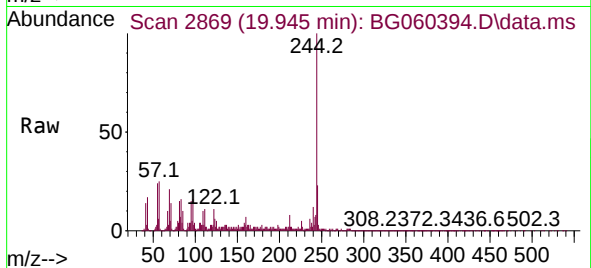

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.757 min Scan# 3688

Delta R.T. 0.017 min

Lab File: BG060394.D

Acq: 22 Jan 2024 21:09

Tgt Ion:264 Resp: 3028455

Ion Ratio Lower Upper

264 100

260 23.8 17.8 26.6

265 22.4 16.8 25.2

