


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060378.D
Acq On : 22 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

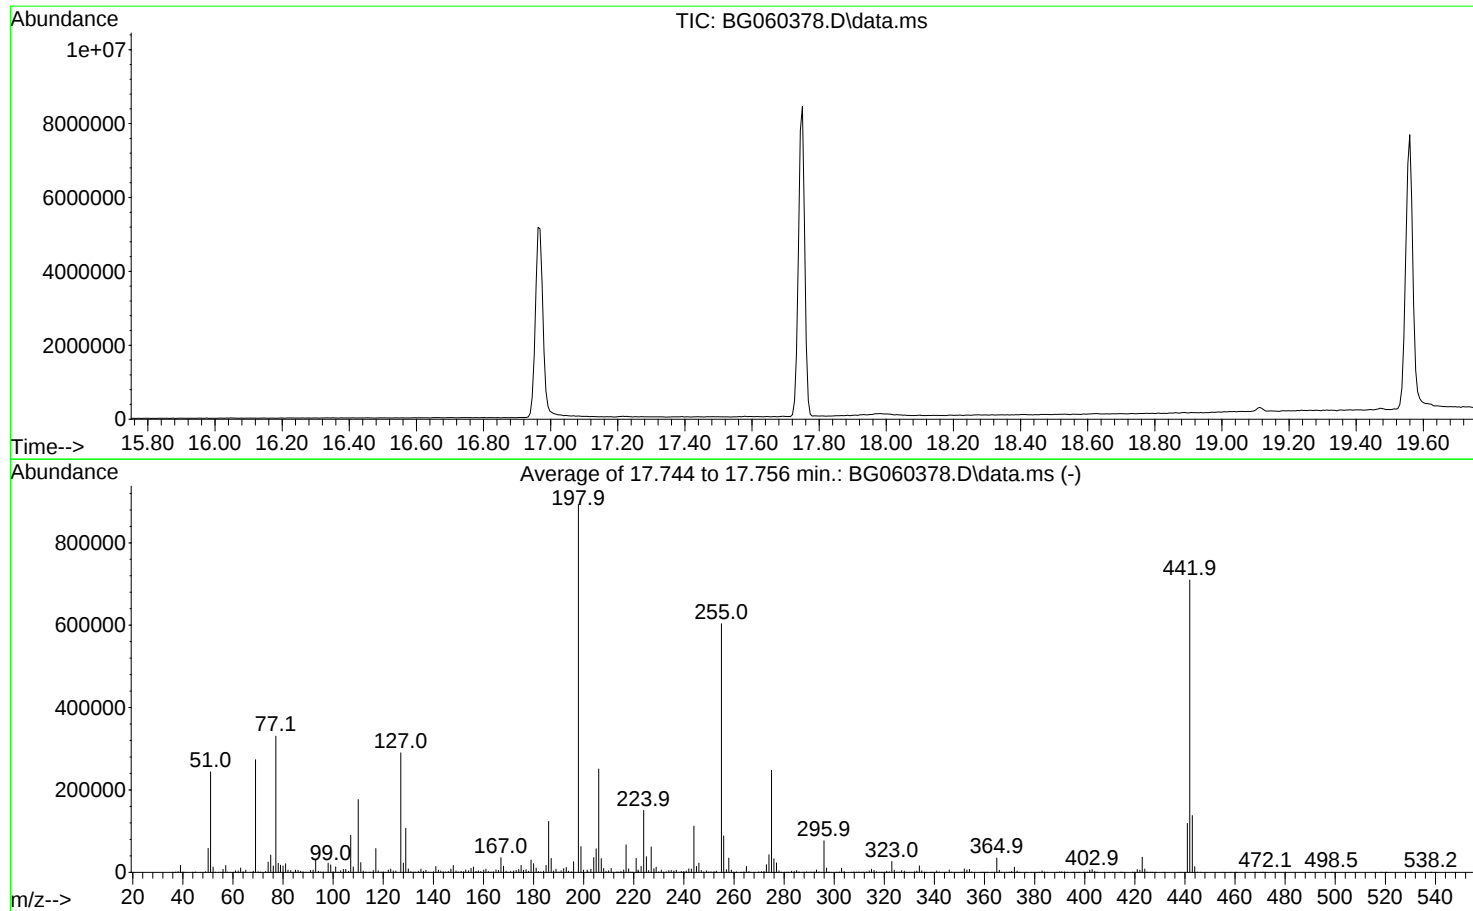




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	243790	PASS
68	69	0.00	2	0.9	2441	PASS
69	198	0.00	100	30.6	273358	PASS
70	69	0.00	2	0.5	1391	PASS
127	198	10	80	32.5	289984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	893269	PASS
199	198	5	9	7.0	62419	PASS
275	198	10	60	27.7	247659	PASS
365	198	1	100	3.9	34520	PASS
441	198	0.01	100	13.3	118811	PASS
442	442	50	100	100.0	709867	PASS
443	442	15	24	19.4	137898	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060378.D
Acq On : 22 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 22 11:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

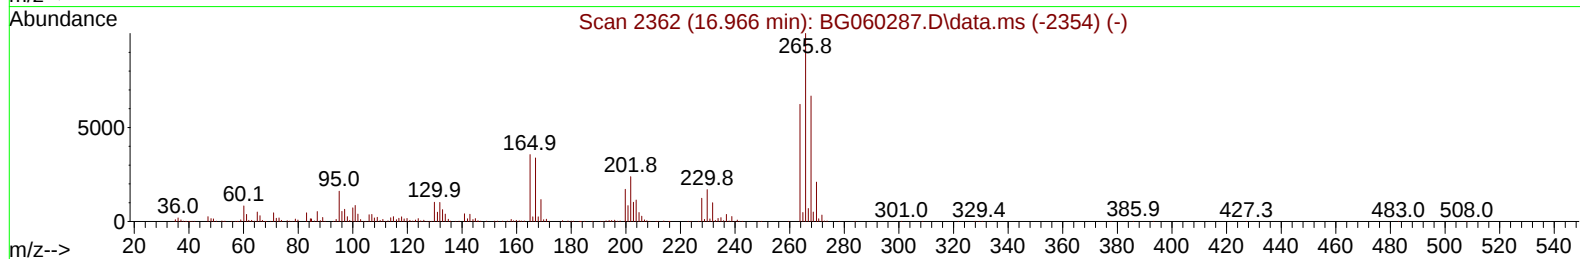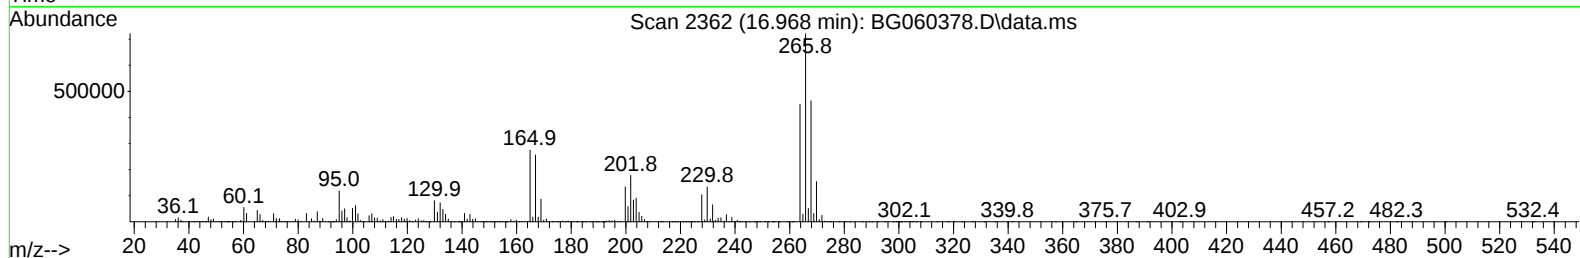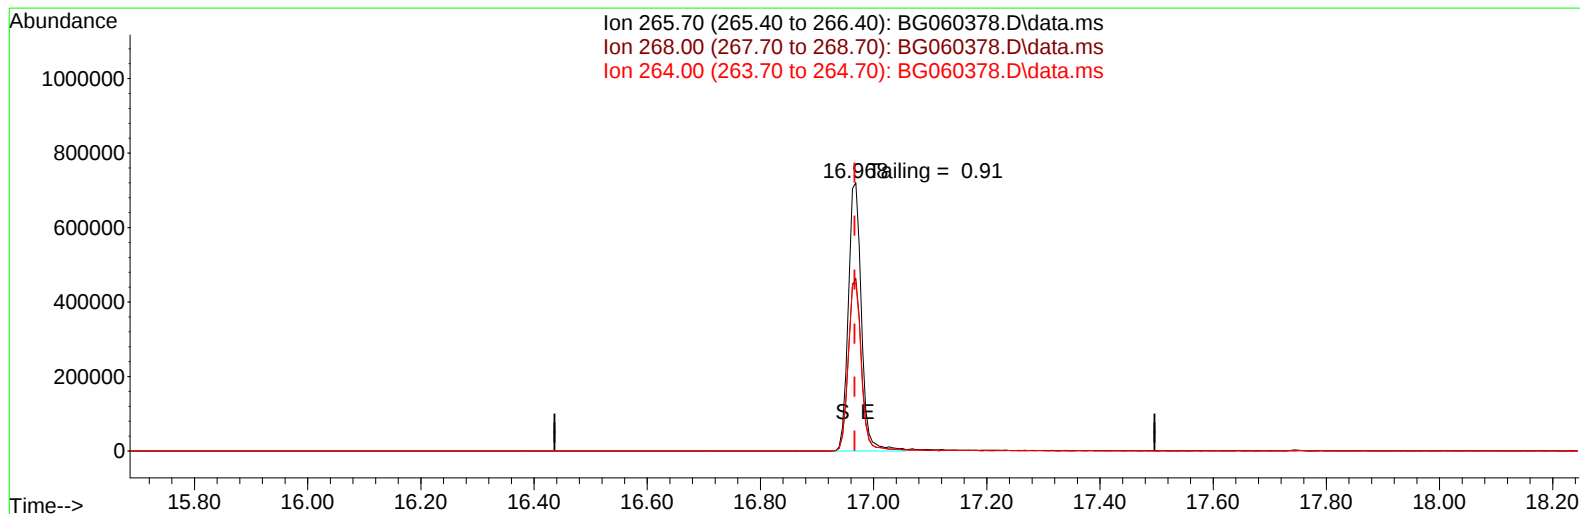

TIC: BG060378.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.002) 753839.74 ng




response 1162710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.39
264.00	62.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012224\
Data File : BG060378.D
Acq On : 22 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 22 11:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

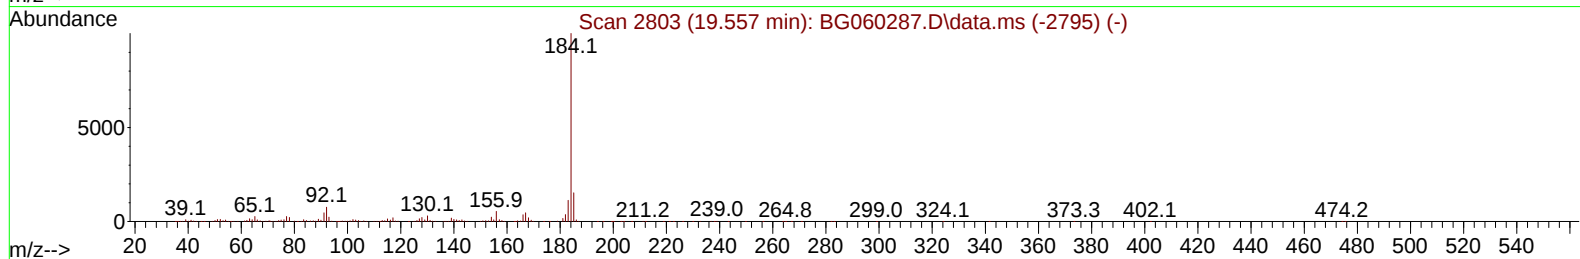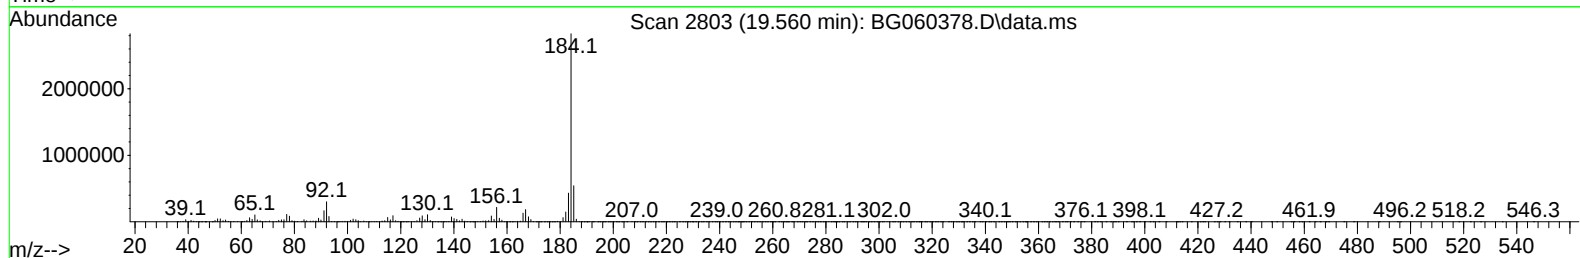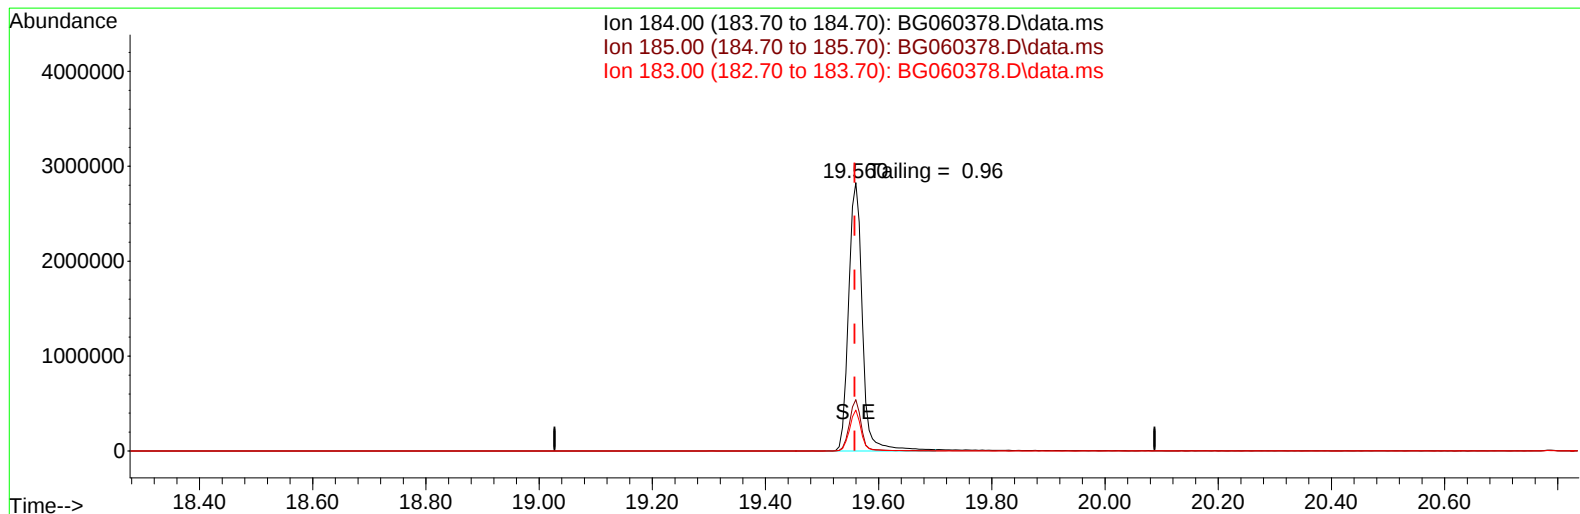

TIC: BG060378.D\data.ms

(77) Benzidine

19.560min (+ 0.002) 187901.14 ng m

response 4792492

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	19.14#
183.00	11.20	15.27#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/22/2024	BNA_G	<u>BG060378.D</u>
Compound Name	Response	Retention Time
DDT	2647436	20.788
DDD	81835	20.341
DDE	6184	19.836
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
88019	2735455	3.22

Instrument :
BNA_G
ClientSampleId :
DFTPP