


Data Path : Z:\HPCHEM1\BNA G\Data\BG012318\
 Data File : BG032224.D
 Acq On : 23 Jan 2018 10:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

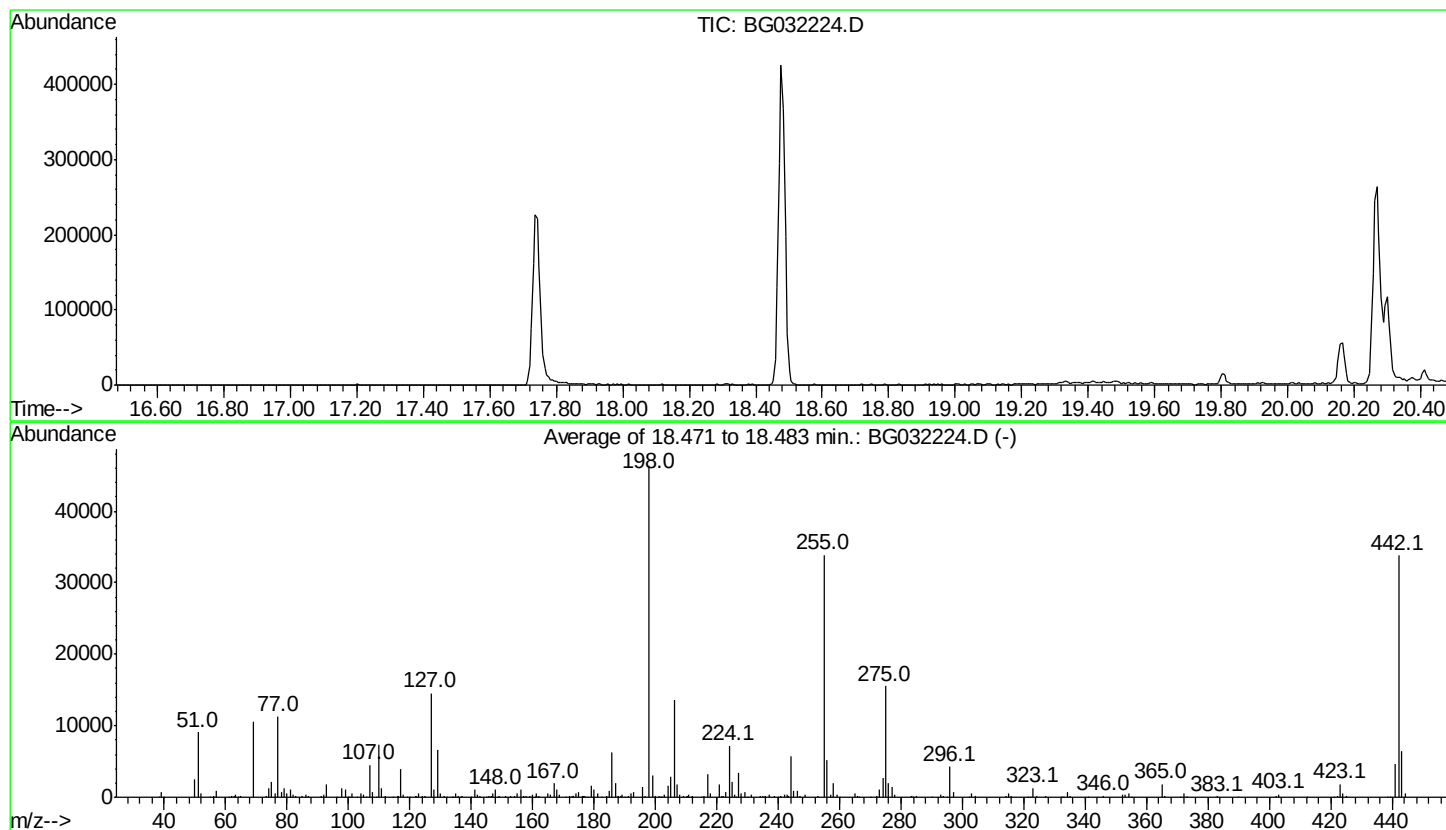

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	9118	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.7	10534	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.3	14524	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46378	PASS
199	198	5	9	6.7	3113	PASS
275	198	10	60	33.4	15497	PASS
365	198	1	100	3.9	1822	PASS
441	442	0.01	24	14.0	4718	PASS
442	198	50	100	72.9	33818	PASS
443	442	15	24	19.2	6501	PASS