


Data Path : Z:\HPCHEM1\BNA G\DATA\BG012318\
 Data File : BG032243.D
 Acq On : 24 Jan 2018 00:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

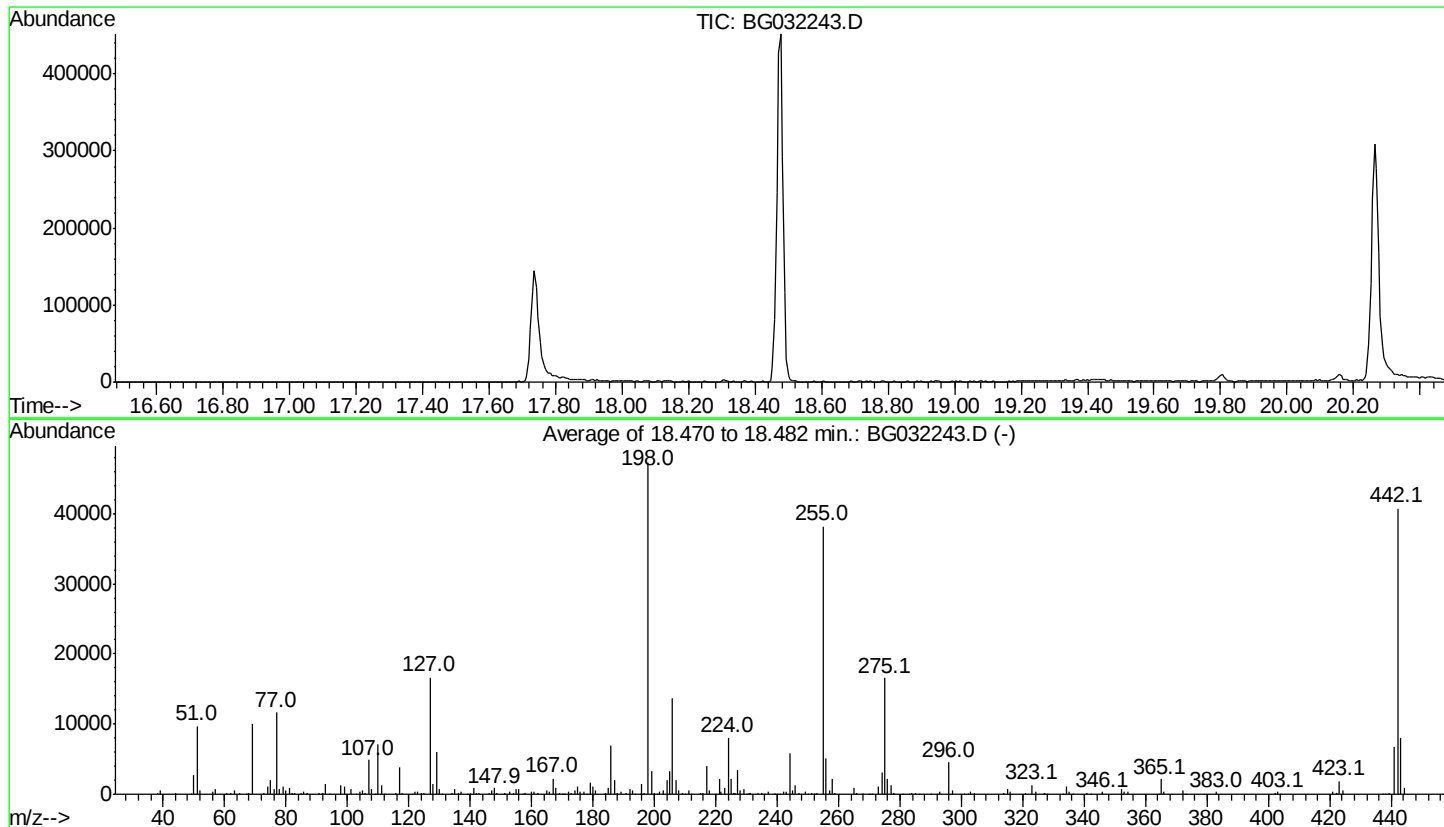

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	9694	PASS
68	69	0.00	2	1.4	141	PASS
69	198	0.00	100	21.4	10110	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.3	16697	PASS
197	198	0.00	2	0.5	233	PASS
198	198	100	100	100.0	47277	PASS
199	198	5	9	7.1	3346	PASS
275	198	10	60	35.0	16564	PASS
365	198	1	100	4.5	2129	PASS
441	442	0.01	24	16.8	6836	PASS
442	198	50	100	86.2	40741	PASS
443	442	15	24	19.6	7988	PASS