
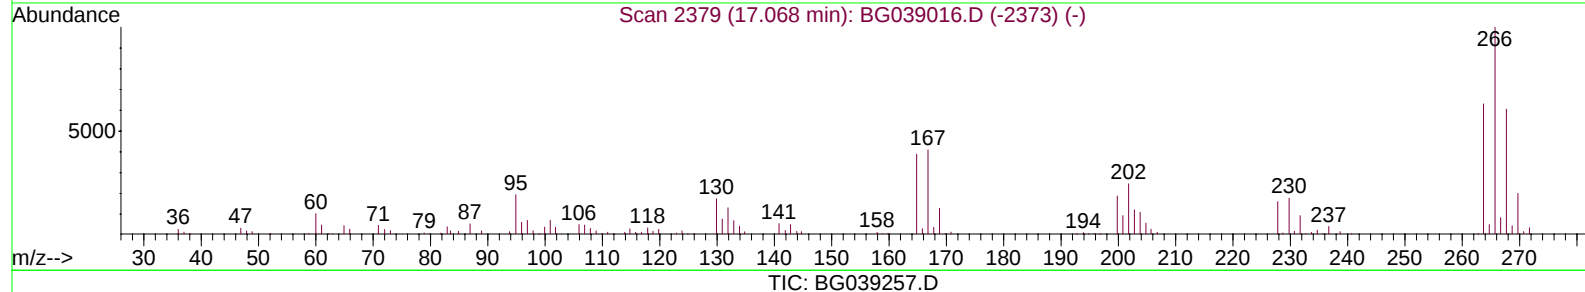
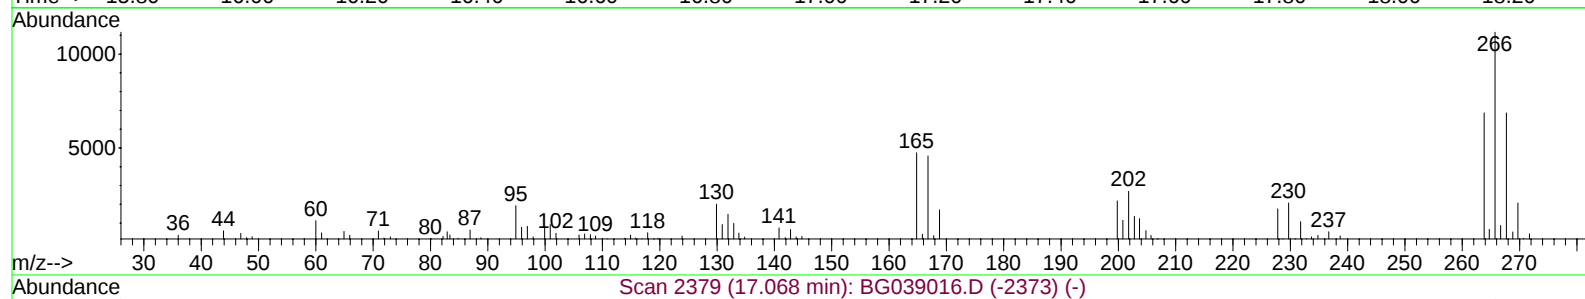


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012319\
Data File : BG039257.D
Acq On : 23 Jan 2019 10:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 18:03:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

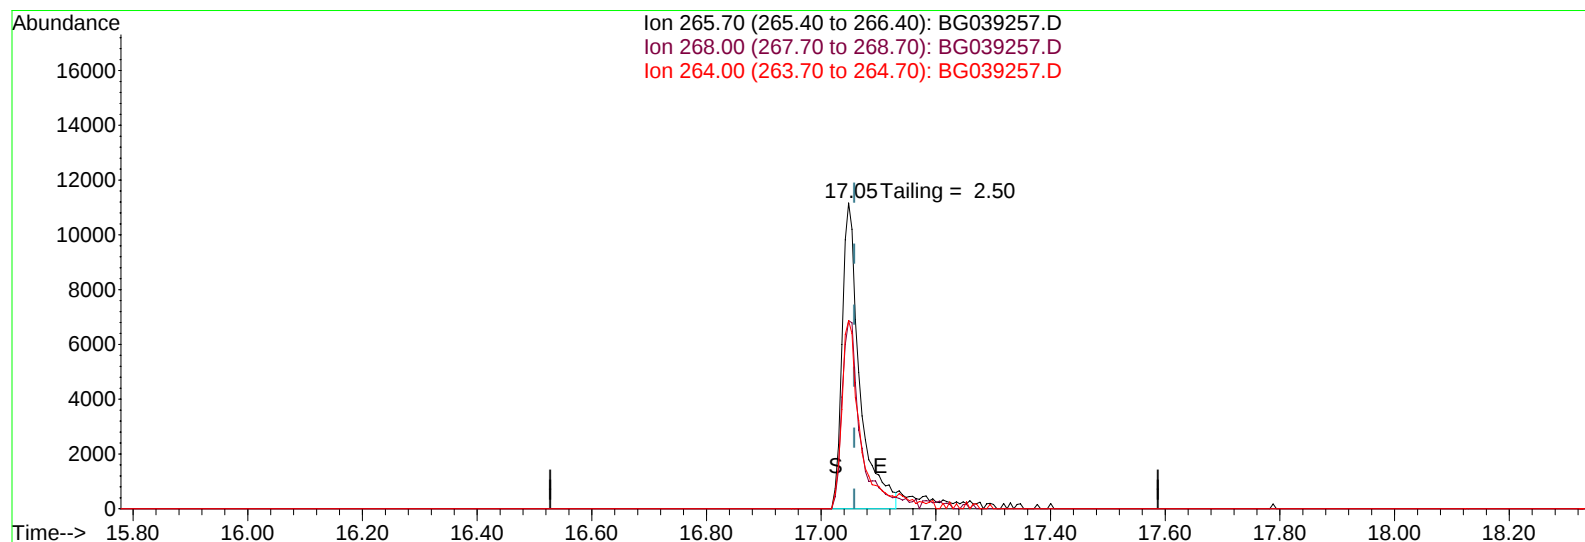

(70) Pentachlorophenol (C)




17.048min (-0.010) 18606.40ng

response 25027

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.53
264.00	68.20	67.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012319\
 Data File : BG039257.D
 Acq On : 23 Jan 2019 10:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 18:03:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

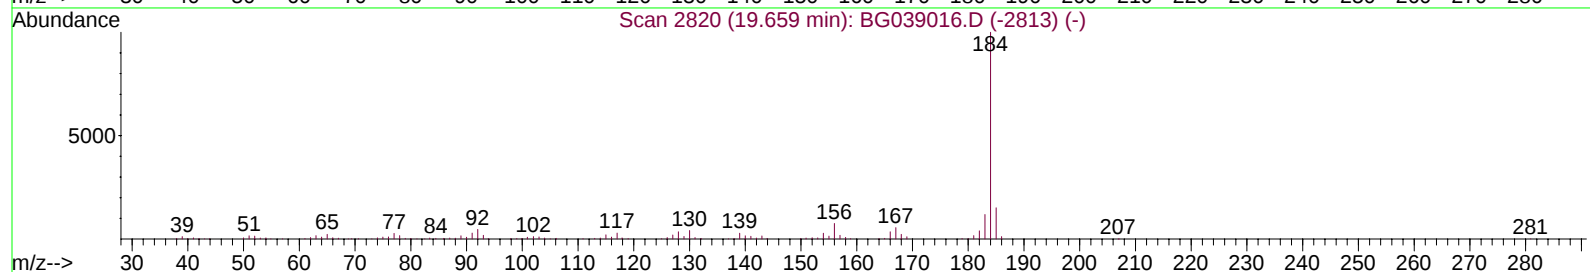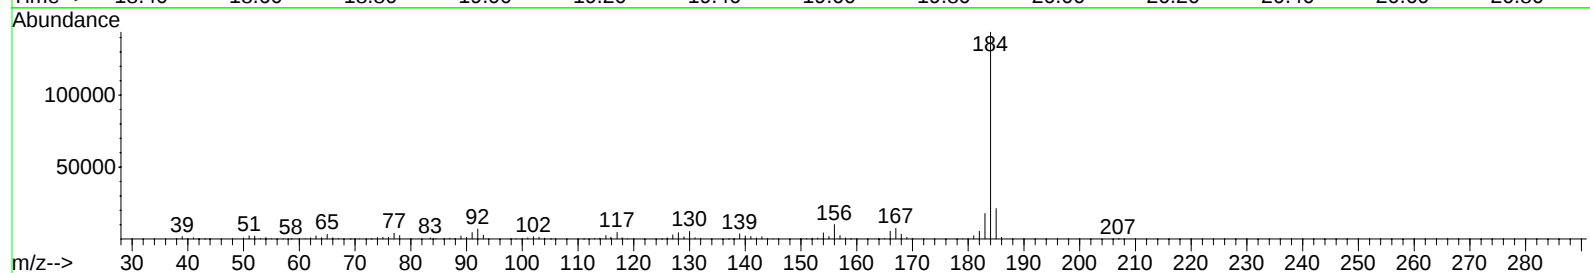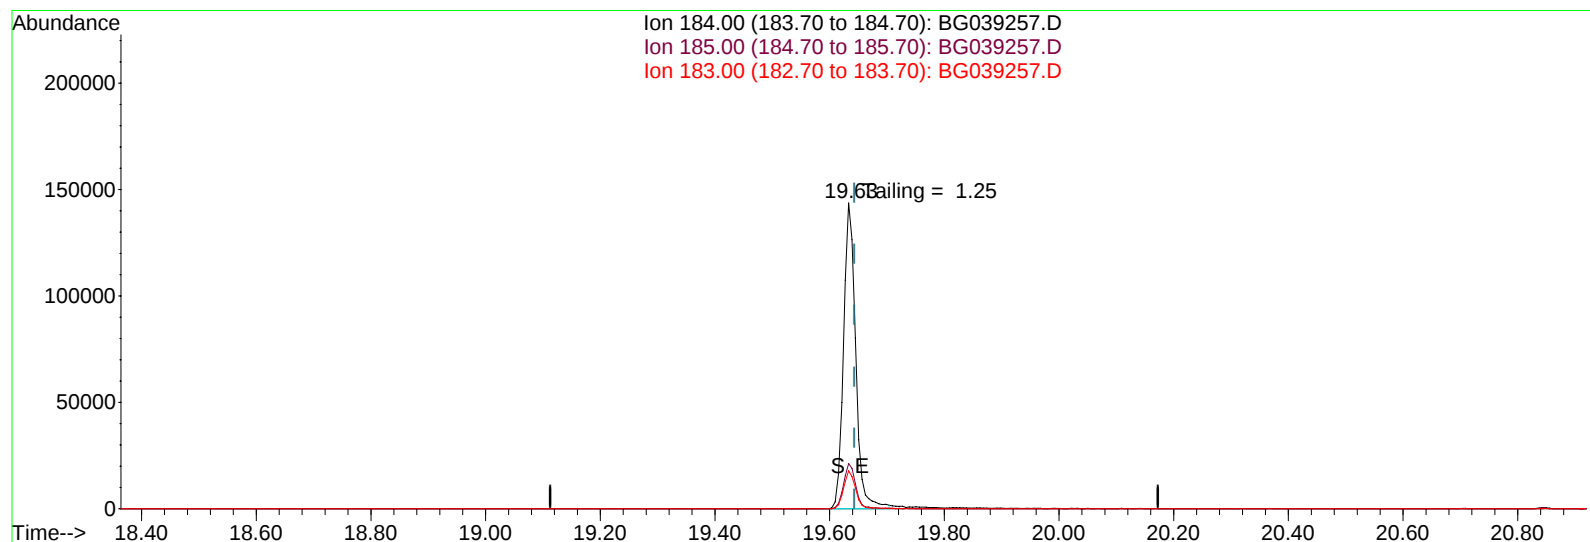

TIC: BG039257.D

(77) Benzidine

19.633min (-0.010) 0.00ng

response 214086

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.78
183.00	11.90	12.41
0.00	0.00	0.00