

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012319\
 Data File : BG039273.D
 Acq On : 23 Jan 2019 21:26
 Operator : JU/SJ
 Sample : PB116574TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB116574TB

Quant Time: Jan 24 00:50:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	17282	20.00	ng	-0.01
21) Naphthalene-d8	10.82	136	54661	20.00	ng	-0.01
39) Acenaphthene-d10	14.65	164	42208	20.00	ng	0.00
64) Phenanthrene-d10	17.39	188	111150	20.00	ng	-0.01
76) Chrysene-d12	21.66	240	111395	20.00	ng	-0.02
87) Perylene-d12	24.93	264	112972	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	129223	141.84	ng	0.00
7) Phenol-d6	7.17	99	178759	136.34	ng	0.00
23) Nitrobenzene-d5	9.19	82	90773	90.87	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	53626	75.79	ng	-0.01
45) 2-Fluorobiphenyl	13.27	172	227441	73.75	ng	0.00
79) Terphenyl-d14	20.00	244	479625	79.65	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012319\
Data File : BG039273.D
Acq On : 23 Jan 2019 21:26
Operator : JU/SJ
Sample : PB116574TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB116574TB

Quant Time: Jan 24 00:50:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

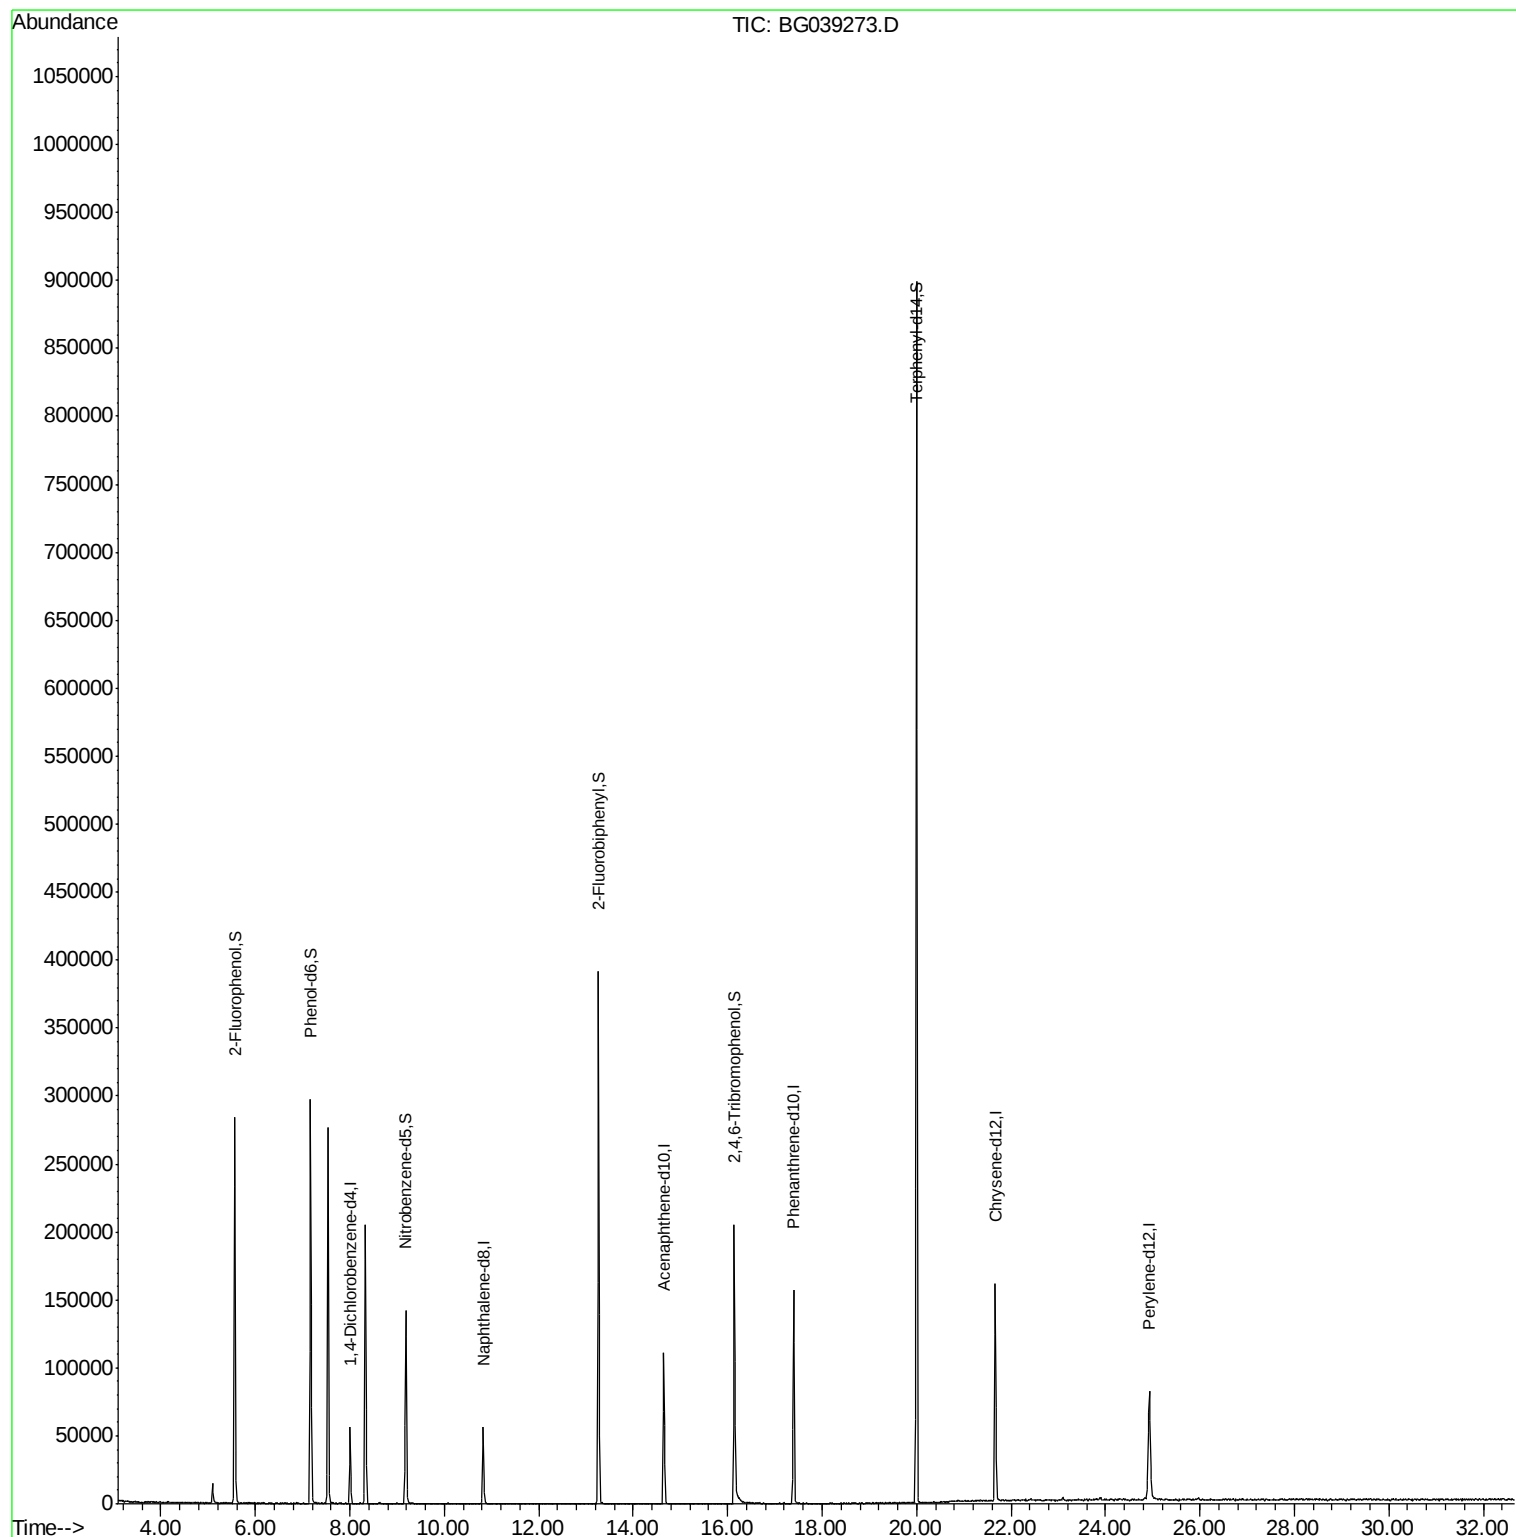




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 837
Delta R.T. -0.01 min
Lab File: BG039273.D
Acq: 23 Jan 2019 21:26

Instrument :
BNA_G
ClientSampleId :
PB116574TB

Tot Ion:152 Resp: 17282
Ion Ratio Lower Upper
152 100
150 157.3 124.7 187.1
115 52.0 46.5 69.7

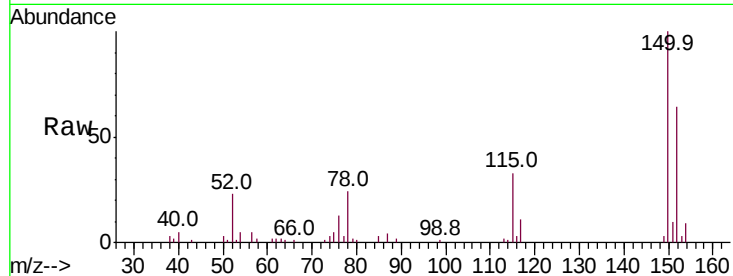


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

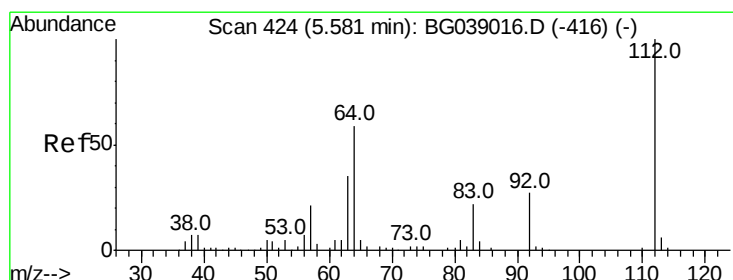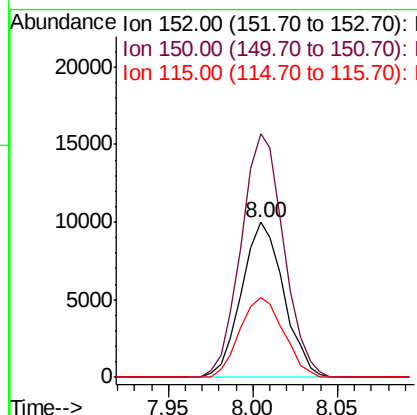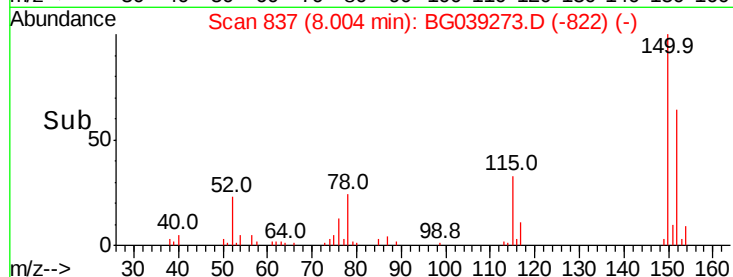



#5

2-Fluorophenol
Concen: 141.843 ng
RT: 5.56 min Scan# 421
Delta R.T. -0.00 min
Lab File: BG039273.D
Acq: 23 Jan 2019 21:26

Tgt Ion:112 Resp: 129223
Ion Ratio Lower Upper
112 100
64 64.4 47.0 70.6
63 34.3 28.0 42.0

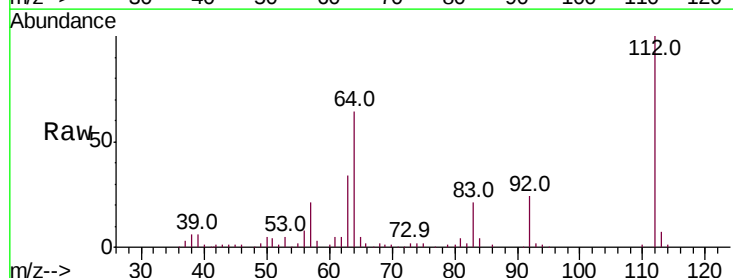

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

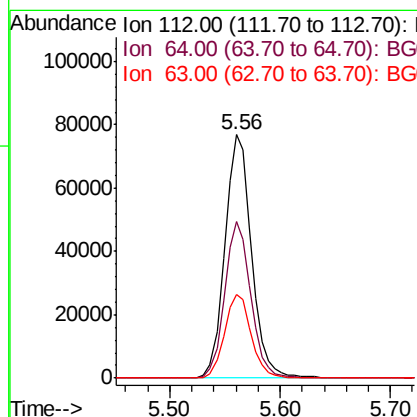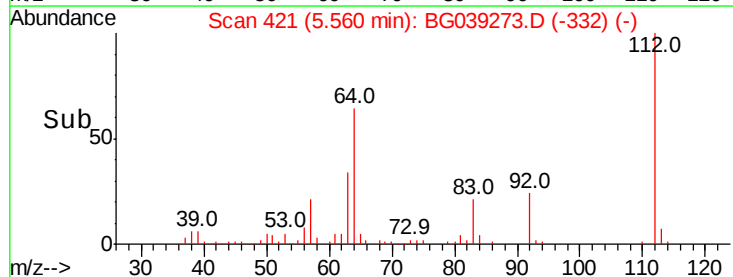



#7

Phenol-d6

Concen: 136.344 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.00 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26

Instrument :

BNA_G

ClientSampleId :

PB116574TB


Tot Ion: 99 Resp: 178759

Ion Ratio Lower Upper




99 100

42 19.4 15.8 23.6

71 36.1 30.2 45.4

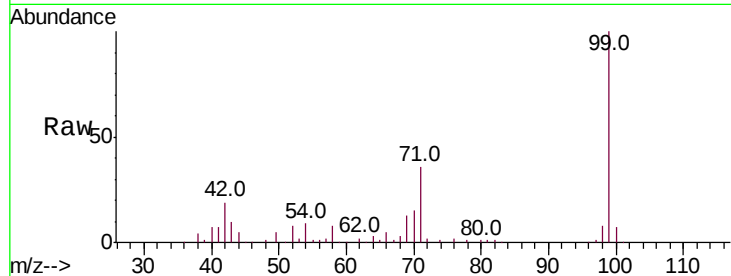

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

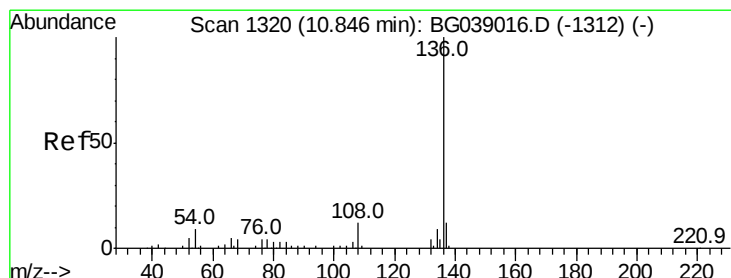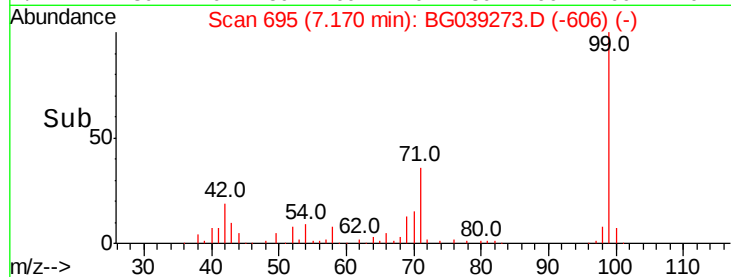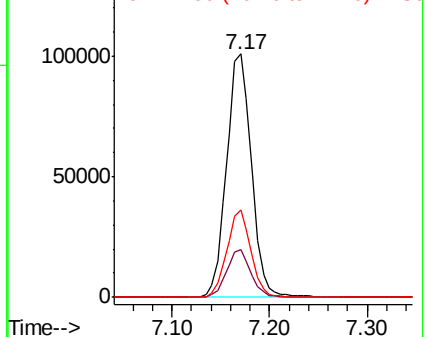

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26

Tgt Ion:136 Resp: 54661


Ion Ratio Lower Upper

136 100



137 11.2 9.4 14.2


54 8.5 7.2 10.8

68 4.7 3.5 5.3

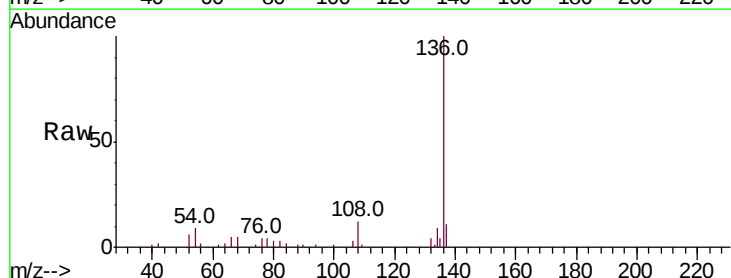

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



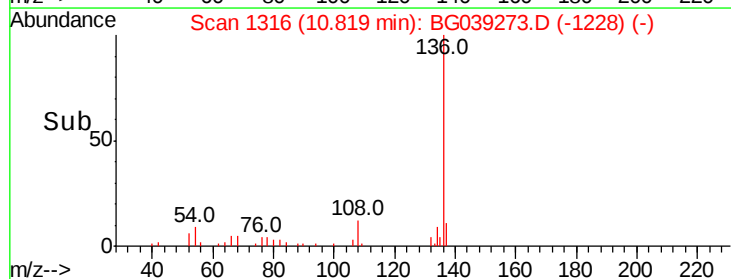
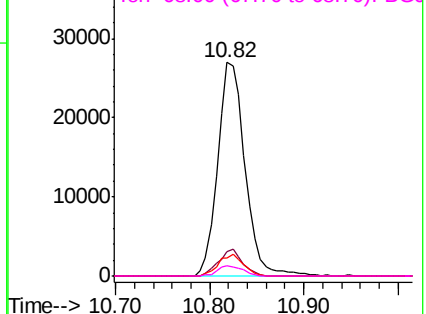


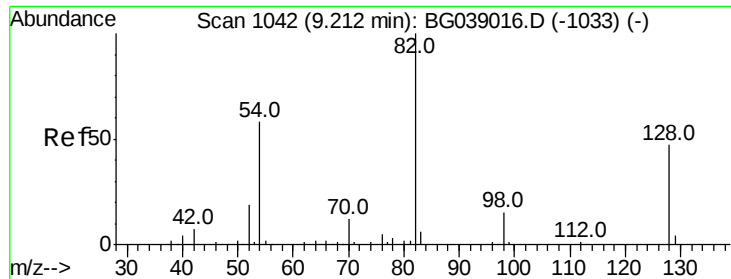

#23
 Nitrobenzene-d5
 Concen: 90.870 ng
 RT: 9.19 min Scan# 1038
 Delta R.T. -0.00 min
 Lab File: BG039273.D
 Acq: 23 Jan 2019 21:26




Instrument :
 BNA_G
 ClientSampleId :
 PB116574TB


Tot Ion: 82 Resp: 90773
 Ion Ratio Lower Upper
 82 100
 128 44.2 37.3 55.9
 54 56.5 46.4 69.6

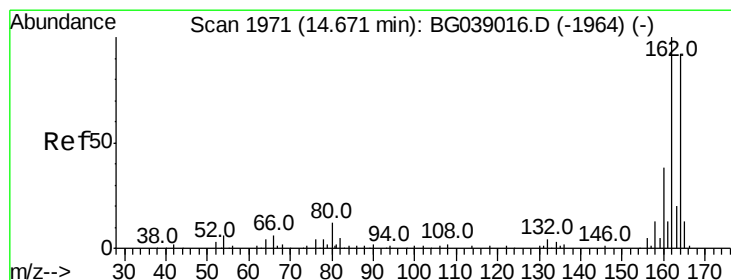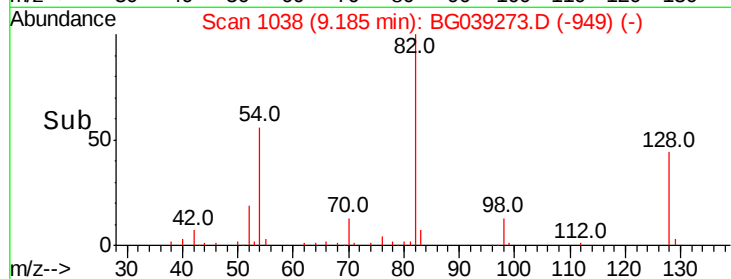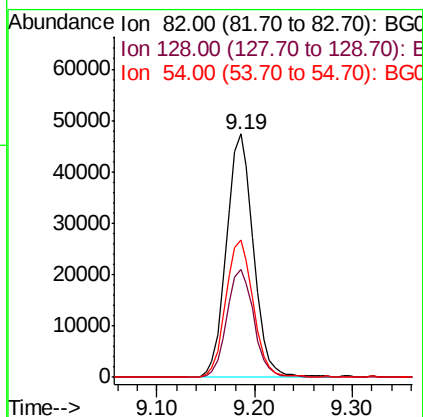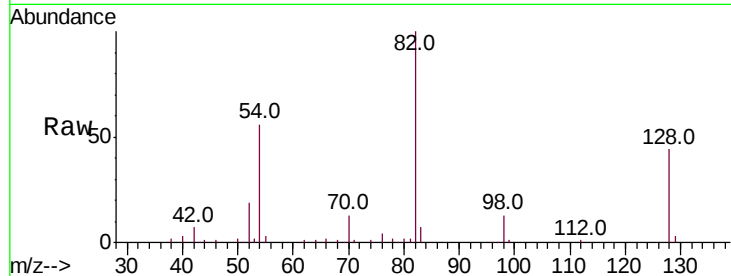

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.65 min Scan# 1968
 Delta R.T. -0.00 min
 Lab File: BG039273.D
 Acq: 23 Jan 2019 21:26

Tgt Ion: 164 Resp: 42208
 Ion Ratio Lower Upper
 164 100
 162 104.1 87.2 130.8
 160 43.2 33.3 49.9

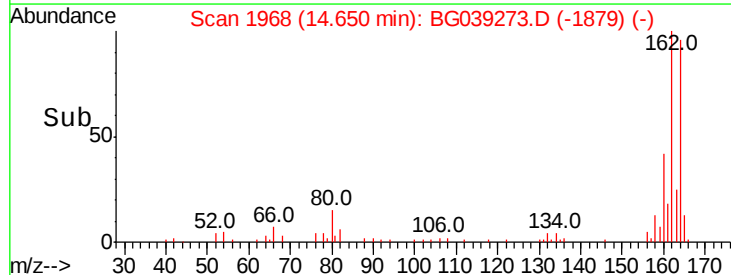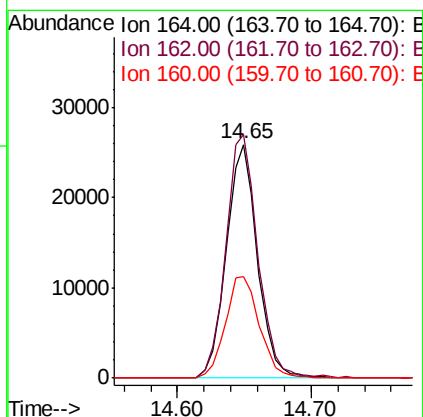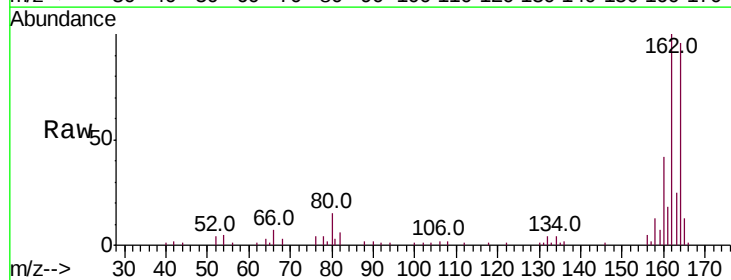

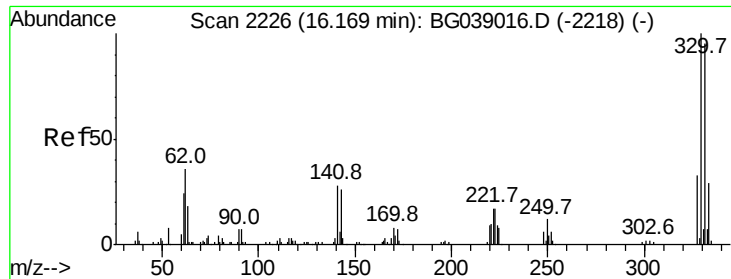

#42

2,4,6-Tribromophenol

Concen: 75.794 ng

RT: 16.14 min Scan# 2222

Delta R.T. -0.01 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26

Instrument :

BNA_G

ClientSampleId :

PB116574TB


Tot Ion:330 Resp: 53626

Ion Ratio Lower Upper

330 100

332 98.4 75.7 113.5




141 32.0 24.9 37.3

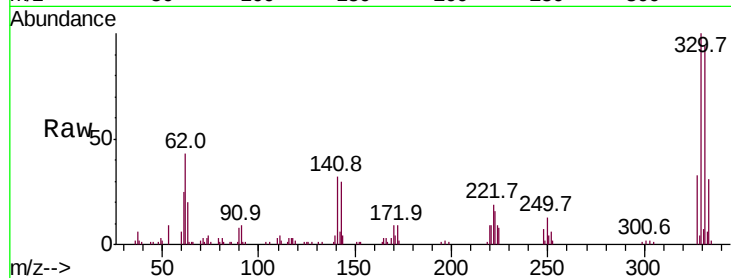

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

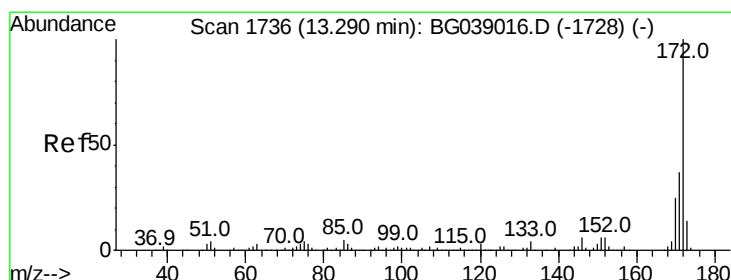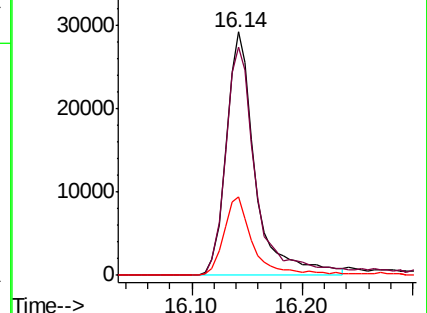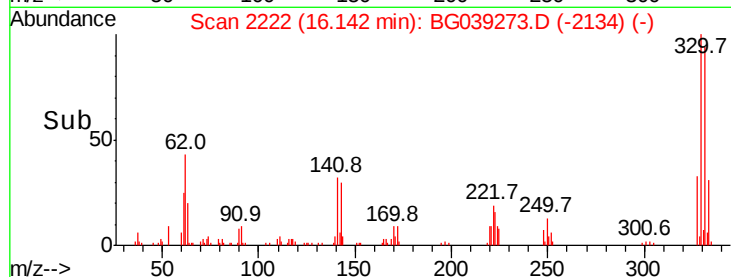

#45

2-Fluorobiphenyl

Concen: 73.746 ng

RT: 13.27 min Scan# 1733

Delta R.T. -0.00 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26


Tgt Ion:172 Resp: 227441

Ion Ratio Lower Upper

172 100

171 36.8 29.4 44.0



170 23.9 20.1 30.1

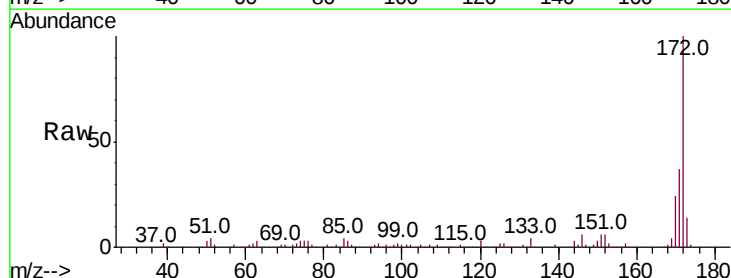


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

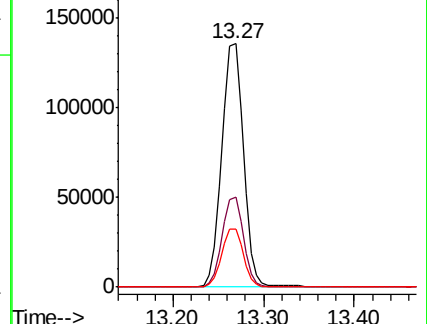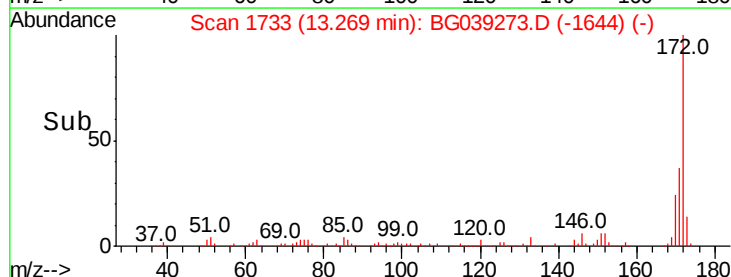

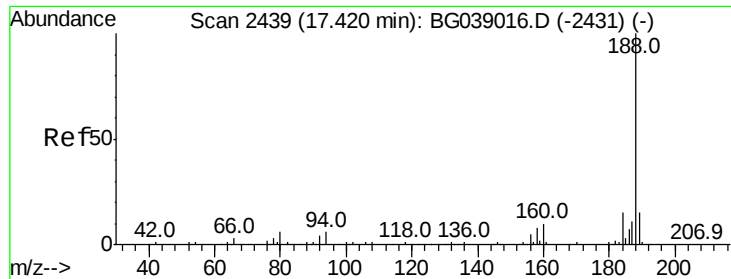

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.39 min Scan# 2435

Delta R.T. -0.01 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26

Instrument :

BNA_G

ClientSampleId :

PB116574TB


Tot Ion:188 Resp: 111150

Ion Ratio Lower Upper

188 100

94 6.2 5.0 7.4




80 7.5 4.7 7.1#

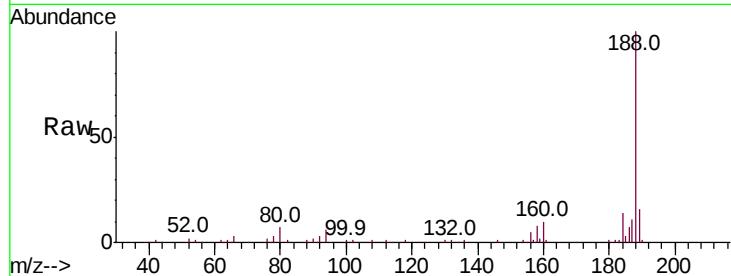

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

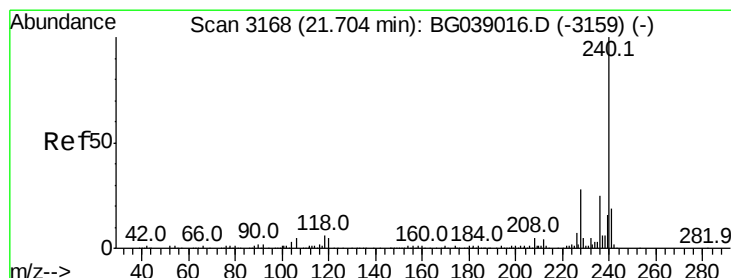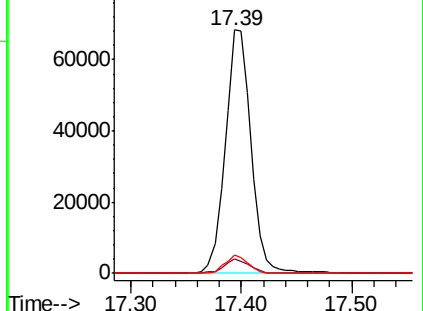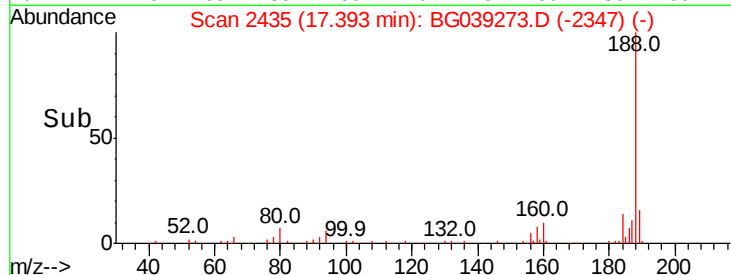

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.66 min Scan# 3162

Delta R.T. -0.02 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26


Tgt Ion:240 Resp: 111395

Ion Ratio Lower Upper

240 100

120 6.4 4.3 6.5



236 25.0 20.1 30.1

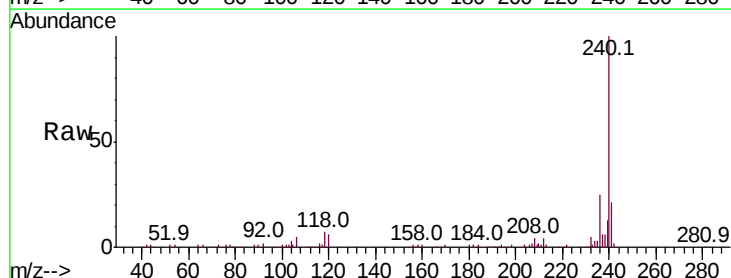


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

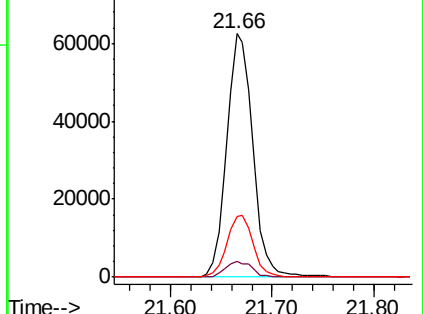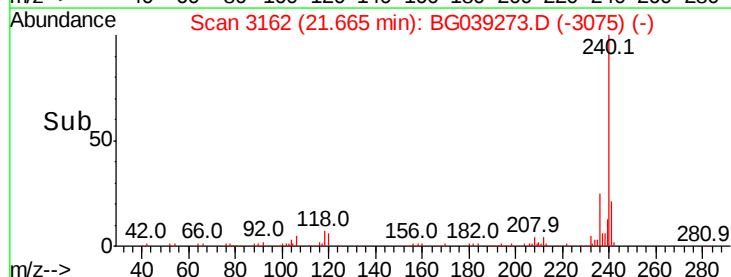

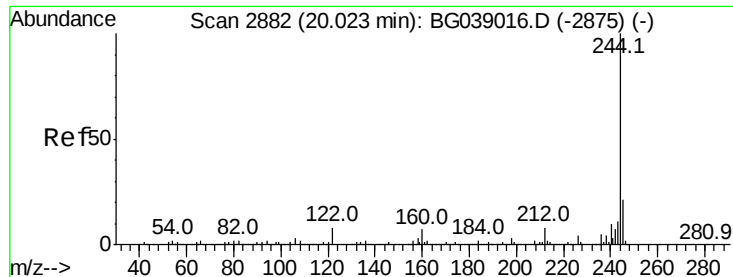

#79

Terphenyl-d14

Concen: 79.649 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26

Instrument :

BNA_G

ClientSampleId :

PB116574TB


Tot Ion:244 Resp: 479625

Ion Ratio Lower Upper

244 100

212 7.2 6.1 9.1




122 6.4 6.1 9.1

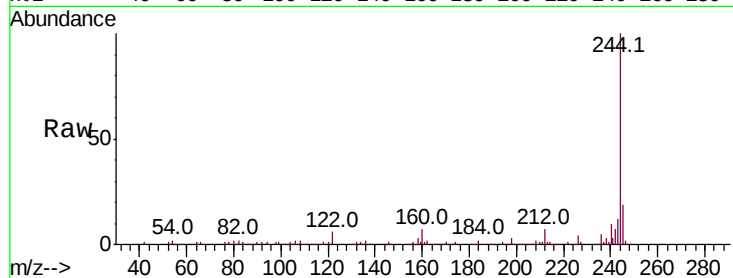

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

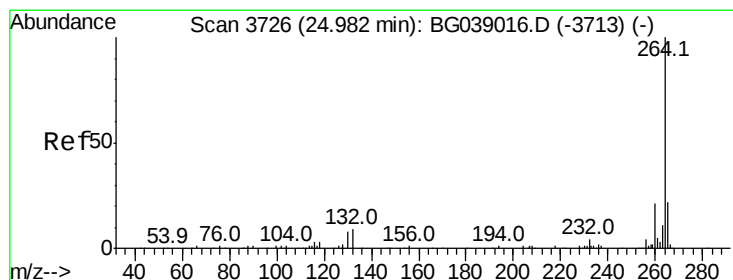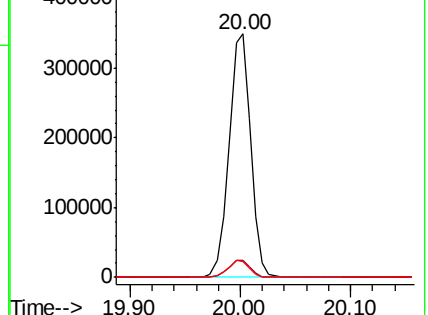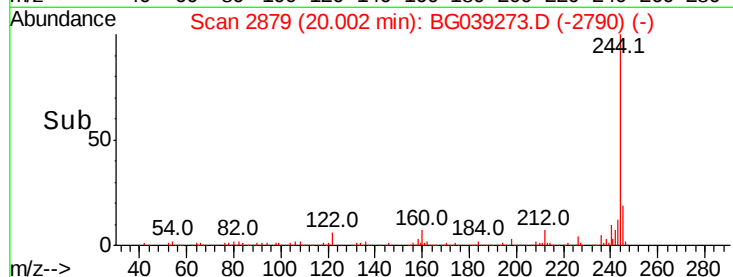

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.02 min

Lab File: BG039273.D

Acq: 23 Jan 2019 21:26


Tgt Ion:264 Resp: 112972

Ion Ratio Lower Upper

264 100

260 21.0 17.0 25.6

265 20.9 17.2 25.8

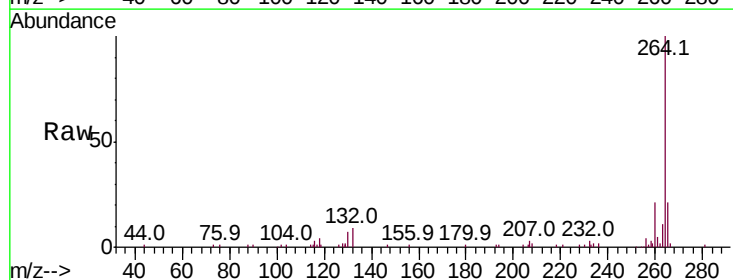

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

