
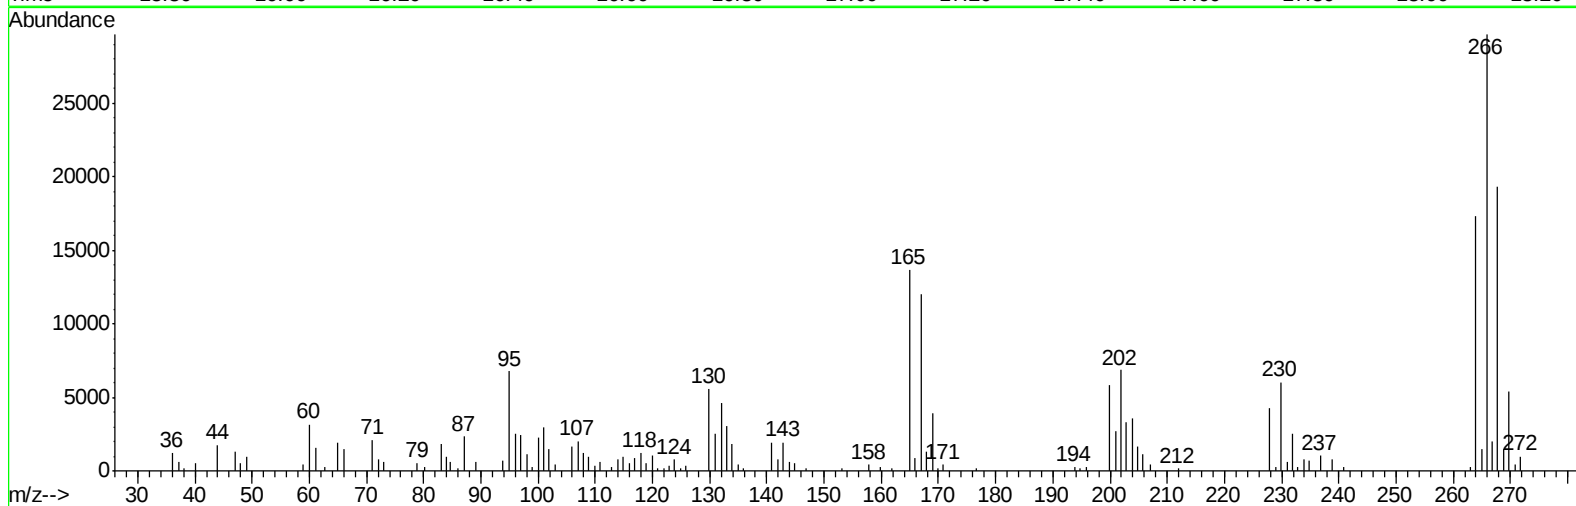


Data File : BG044163.D
Acq On : 23 Jan 2020 11:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 05:50:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

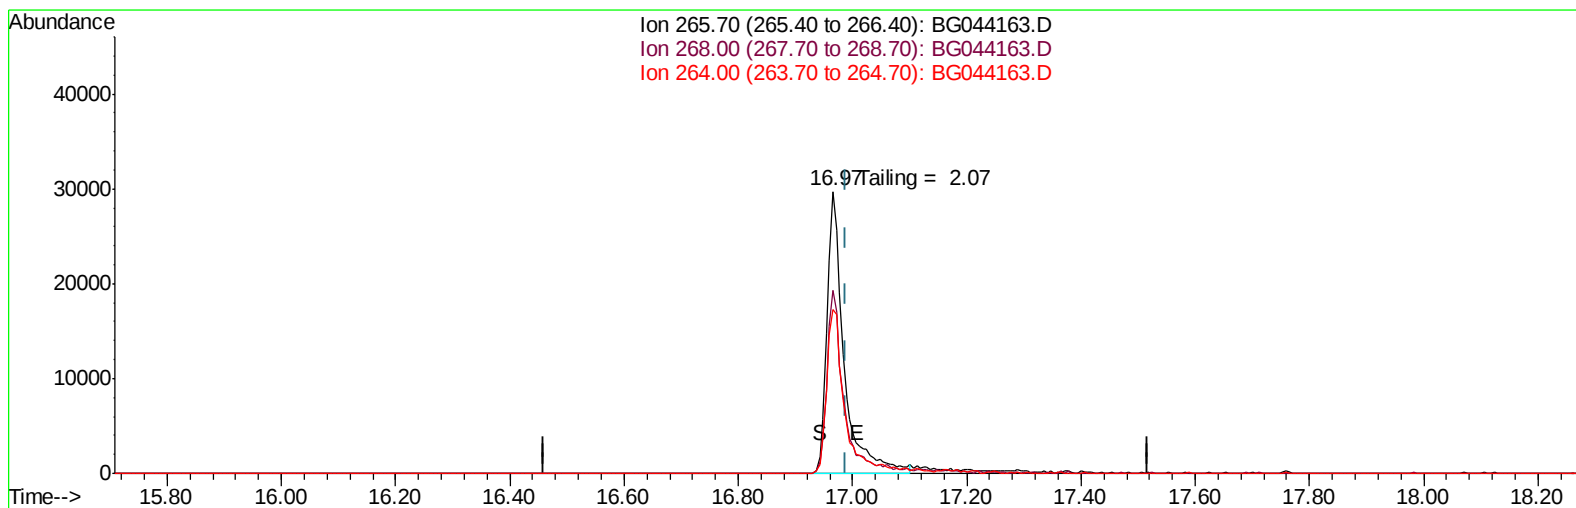

TIC: BG044163.D

(70) Pentachlorophenol (C)



16.966min (-0.023) 18315.25ng

response 60444

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	65.10
264.00	63.50	58.42
0.00	0.00	0.00

Data File : BG044163.D
Acq On : 23 Jan 2020 11:13
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 05:50:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

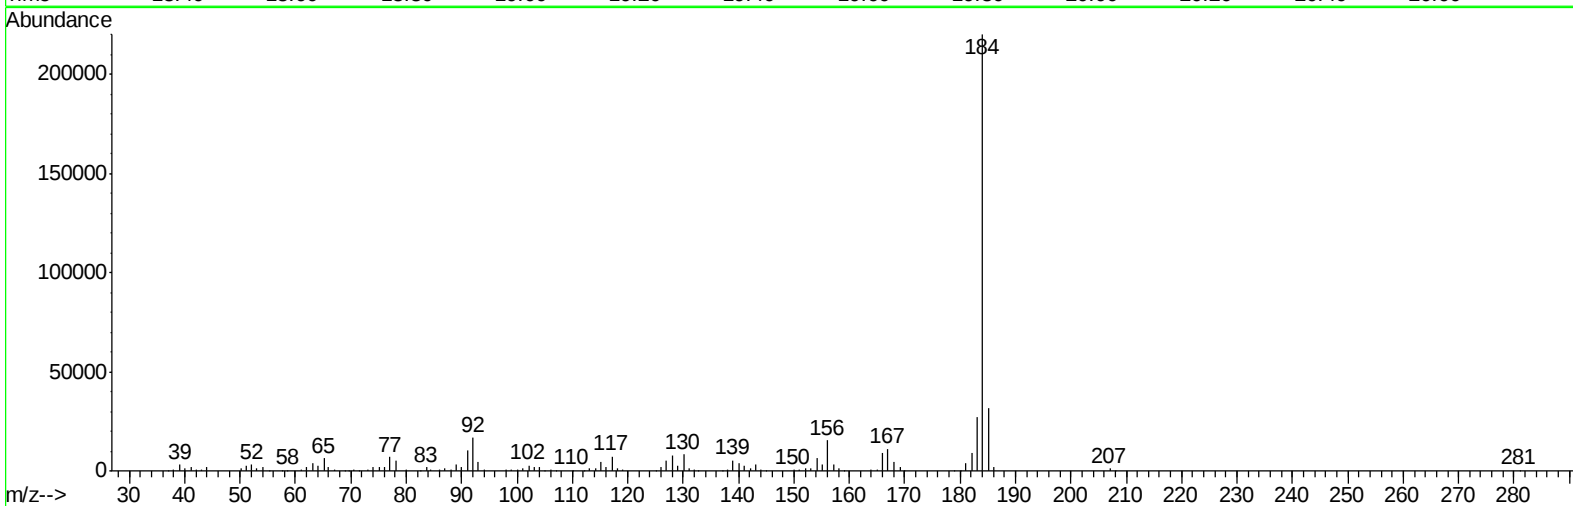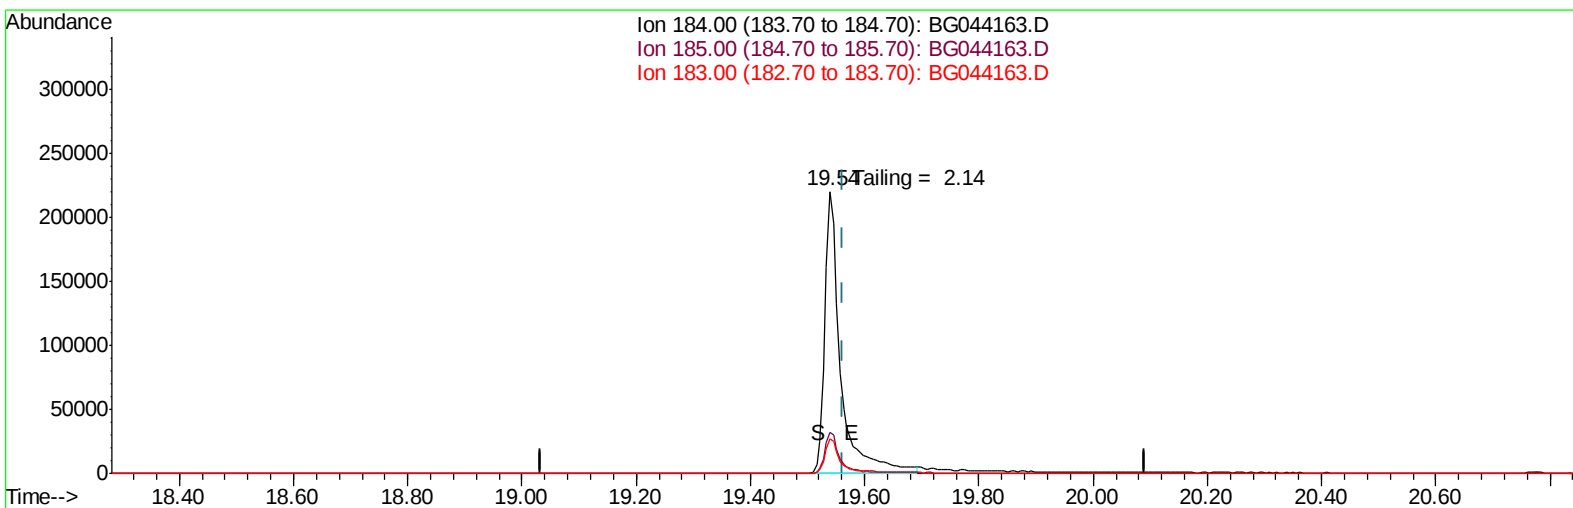

TIC: BG044163.D

(77) Benzidine

19.539min (-0.024) 0.00ng

response 434409

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.47
183.00	13.20	12.45
0.00	0.00	0.00