


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012320\
 Data File : BG044163.D
 Acq On : 23 Jan 2020 11:13
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

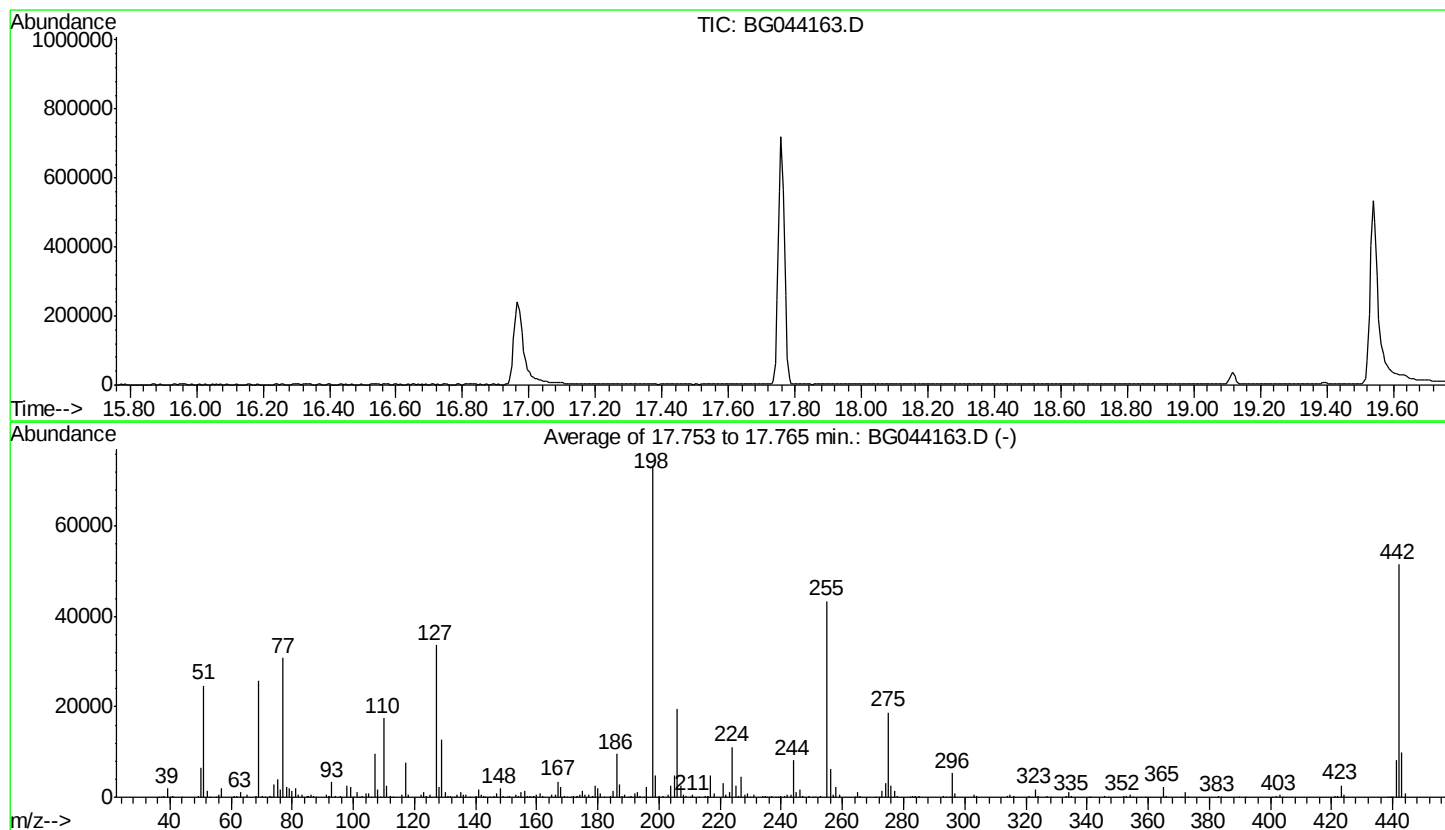

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	24738	PASS
68	69	0.00	2	0.7	187	PASS
69	198	0.00	100	35.3	25917	PASS
70	69	0.00	2	0.8	216	PASS
127	198	10	80	45.8	33650	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73434	PASS
199	198	5	9	6.5	4759	PASS
275	198	10	60	25.5	18717	PASS
365	198	1	100	3.1	2295	PASS
441	198	0.01	100	11.4	8367	PASS
442	198	50	100	70.1	51469	PASS
443	442	15	24	19.3	9934	PASS