
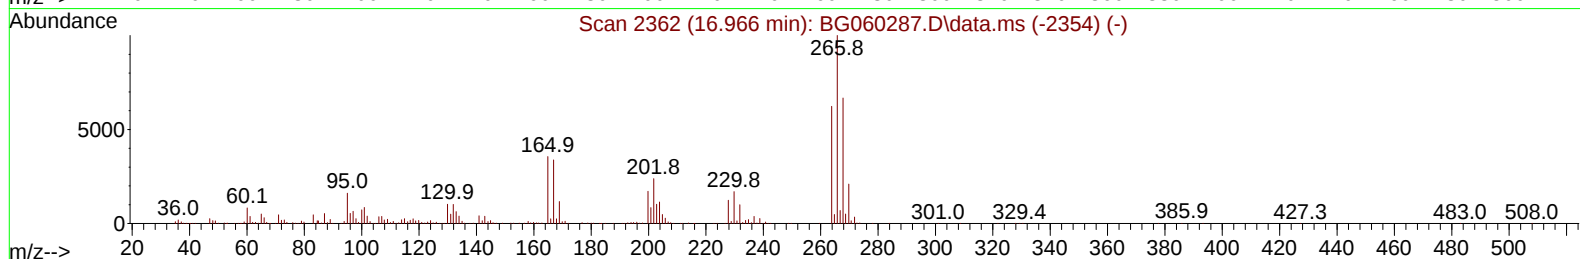
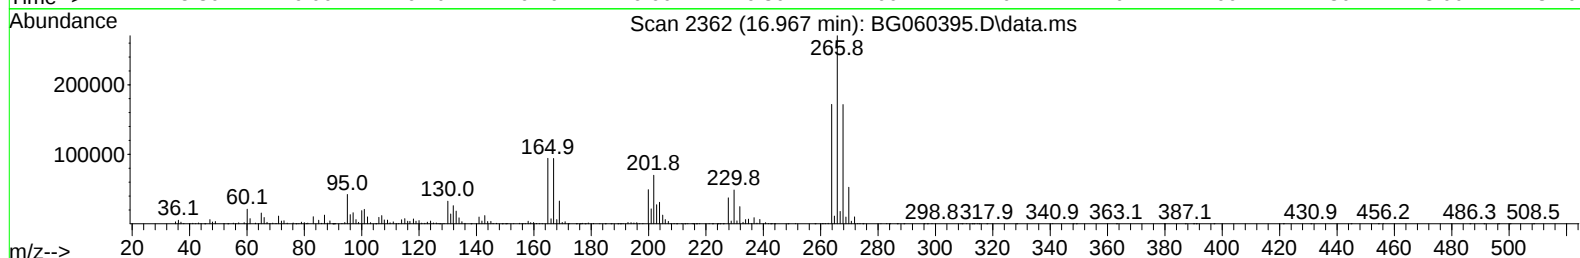


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012324\
Data File : BG060395.D
Acq On : 23 Jan 2024 9:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 10:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

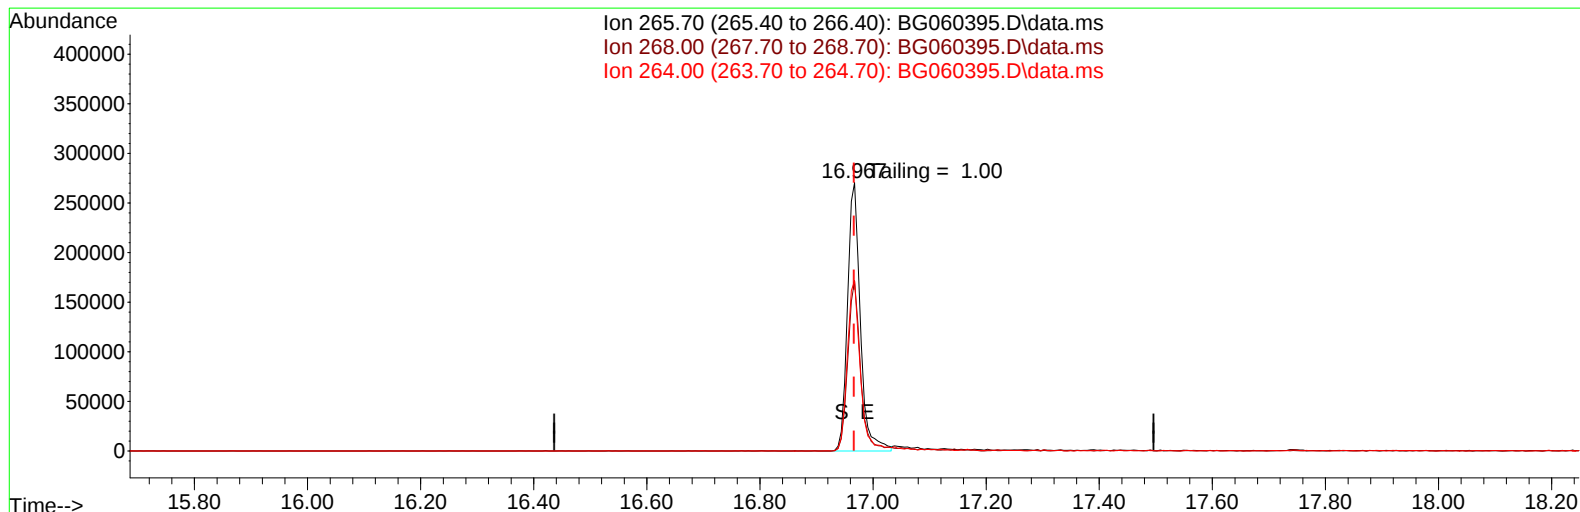




TIC: BG060395.D\data.ms

(70) Pentachlorophenol (C)**16.967min (+ 0.001) 406996.74 ng****response 428008**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.40
264.00	62.30	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012324\
Data File : BG060395.D
Acq On : 23 Jan 2024 9:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 10:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

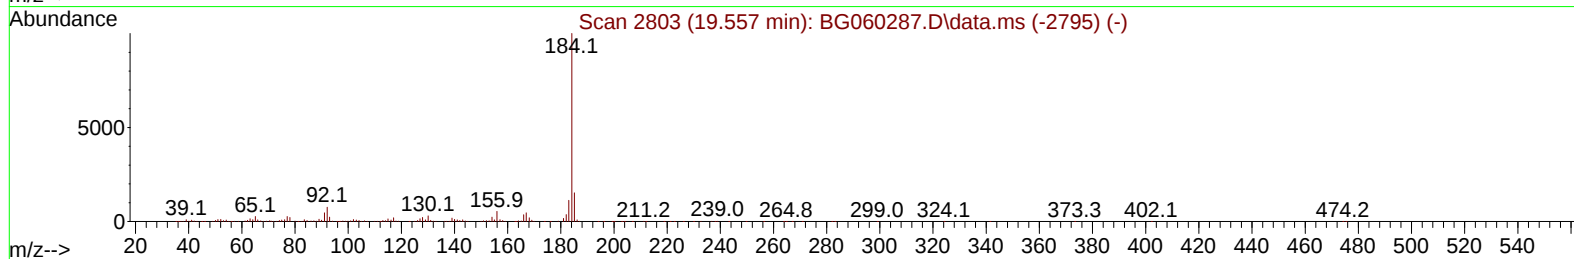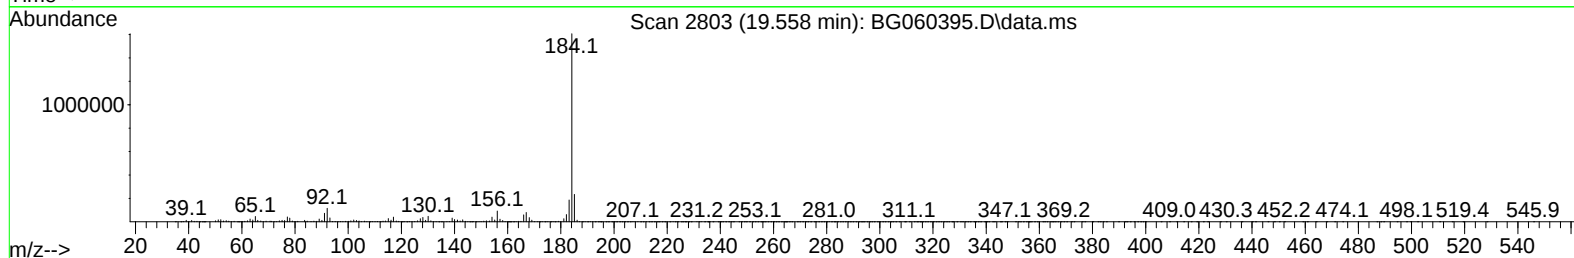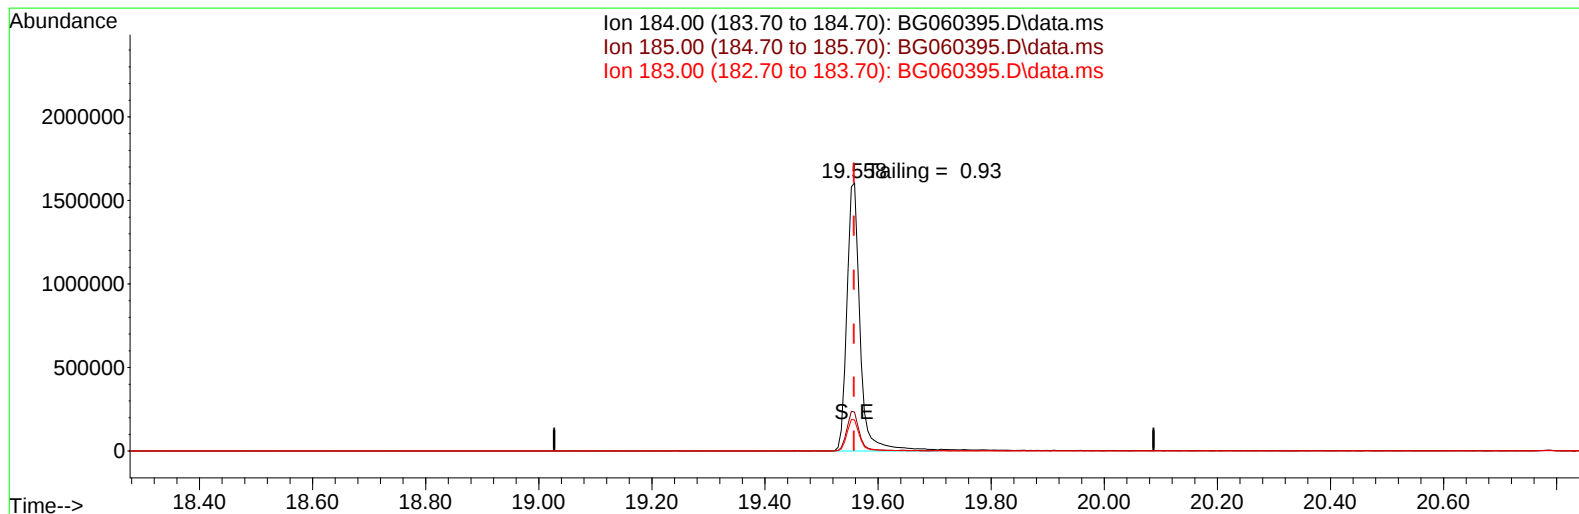

TIC: BG060395.D\data.ms

(77) Benzidine**19.558min (+ 0.001) 531762.15 ng****response 2610897**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.53
183.00	11.20	11.55
0.00	0.00	0.00