


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012324\
Data File : BG060395.D
Acq On : 23 Jan 2024 9:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

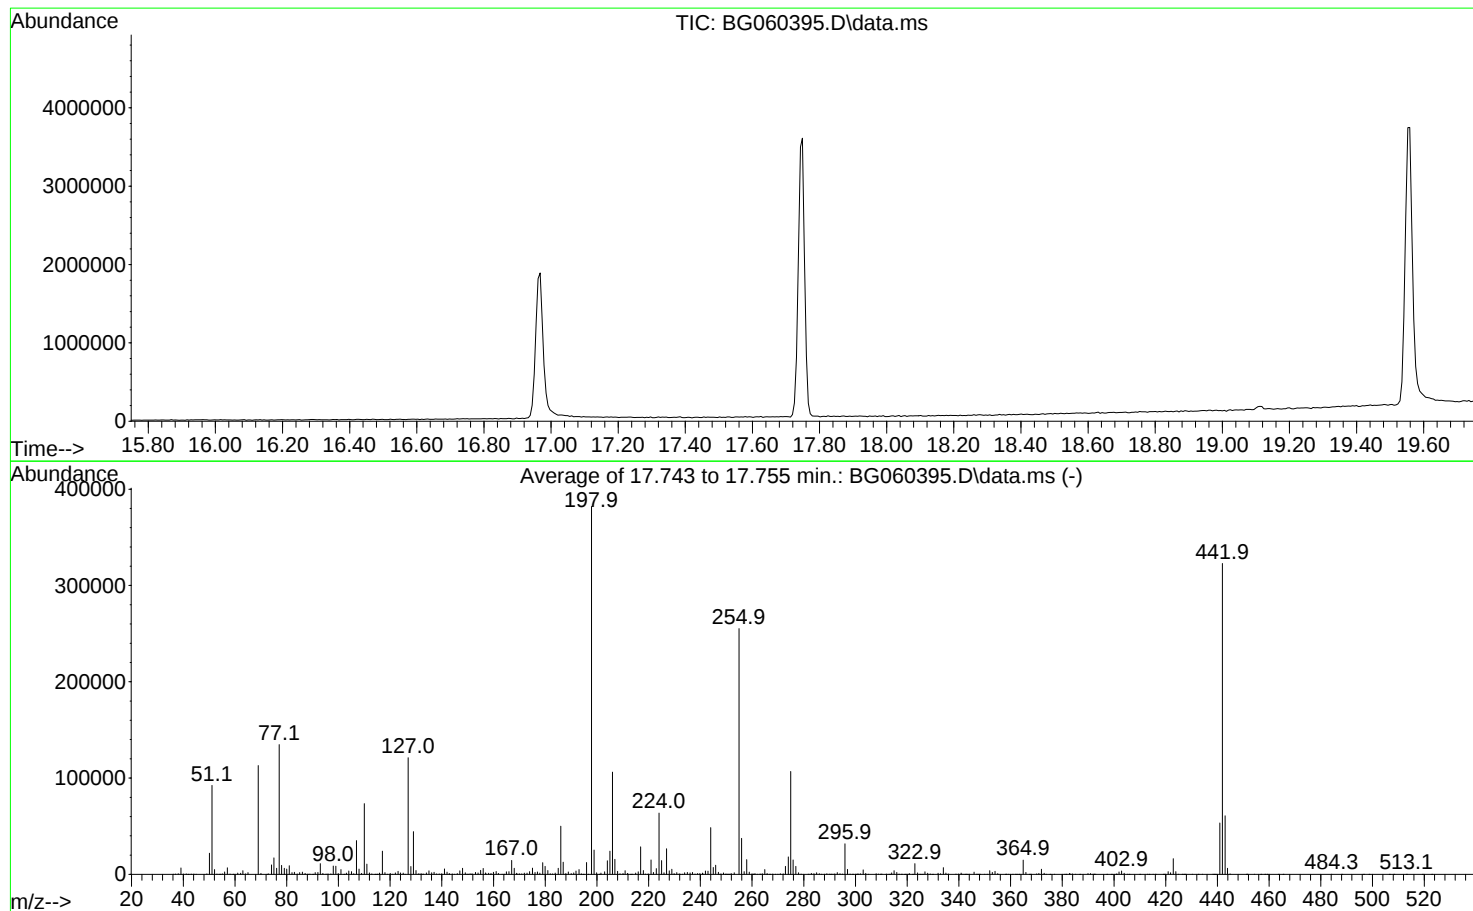




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	92336	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.6	112912	PASS
70	69	0.00	2	1.0	1082	PASS
127	198	10	80	31.7	121080	PASS
197	198	0.00	2	0.1	216	PASS
198	198	100	100	100.0	381995	PASS
199	198	5	9	6.6	25201	PASS
275	198	10	60	28.0	106906	PASS
365	198	1	100	3.9	14778	PASS
441	198	0.01	100	14.0	53315	PASS
442	442	50	100	100.0	322859	PASS
443	442	15	24	18.8	60755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012324\
Data File : BG060395.D
Acq On : 23 Jan 2024 9:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 23 10:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

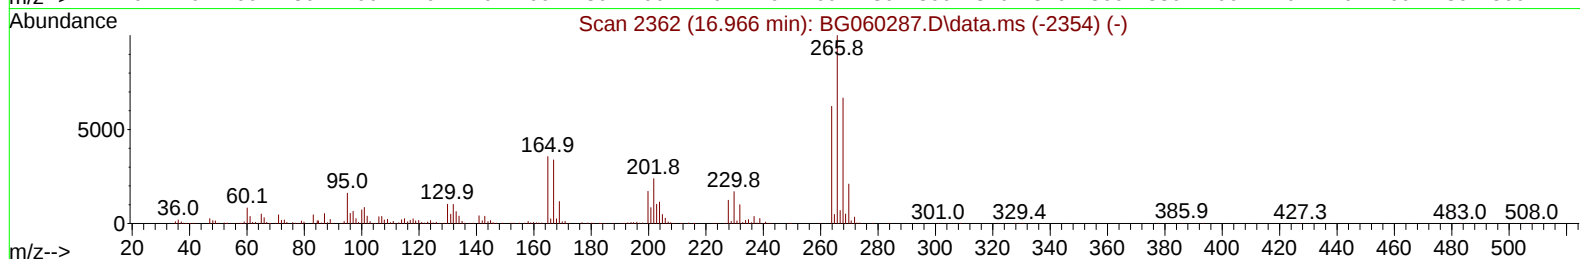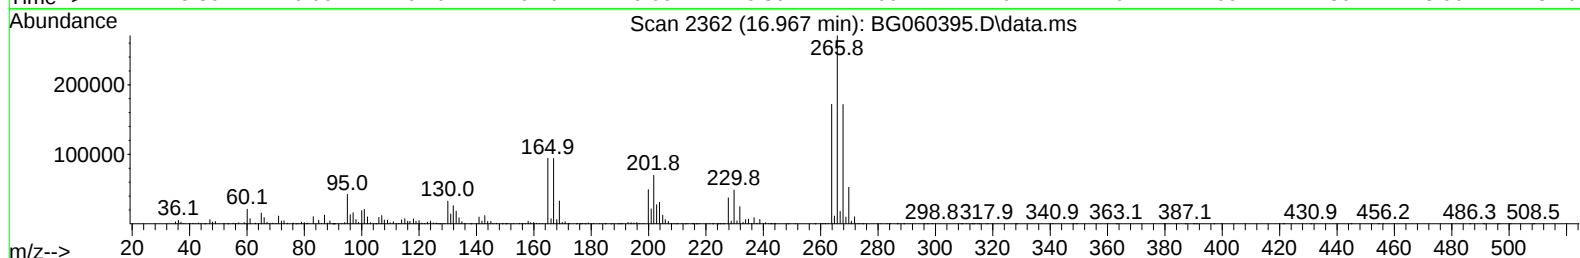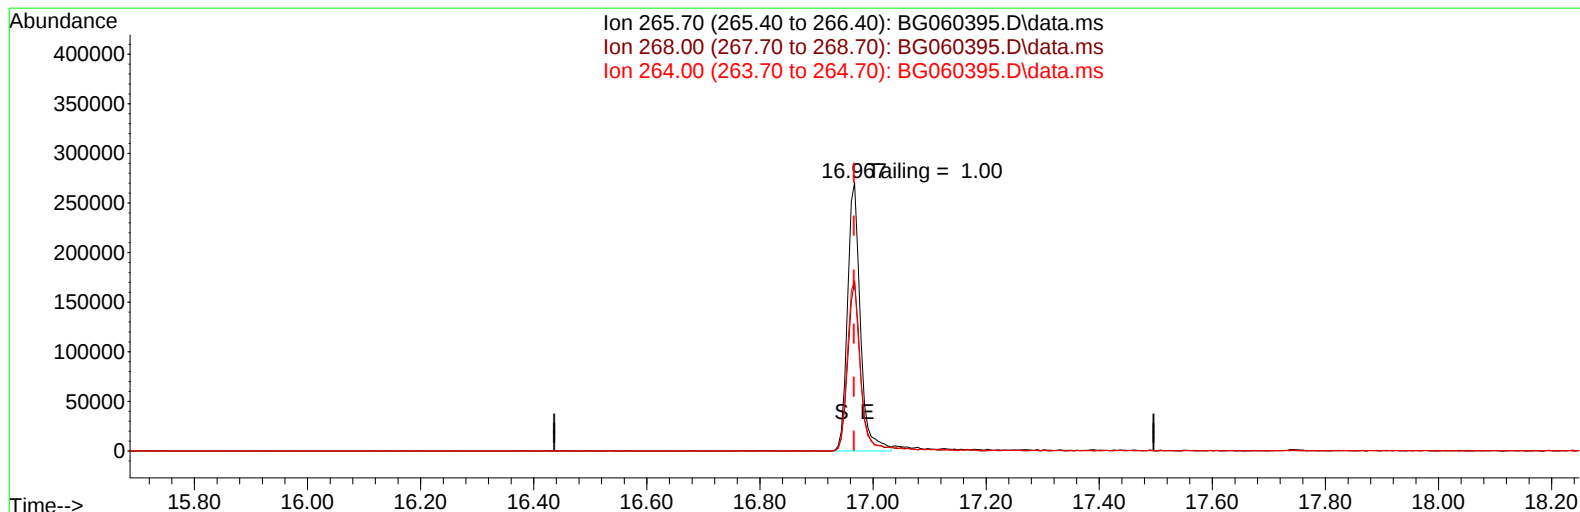

TIC: BG060395.D\data.ms

(70) Pentachlorophenol (C)

16.967min (+ 0.001) 406996.74 ng




response 428008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.40
264.00	62.30	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012324\
Data File : BG060395.D
Acq On : 23 Jan 2024 9:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 23 10:31:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

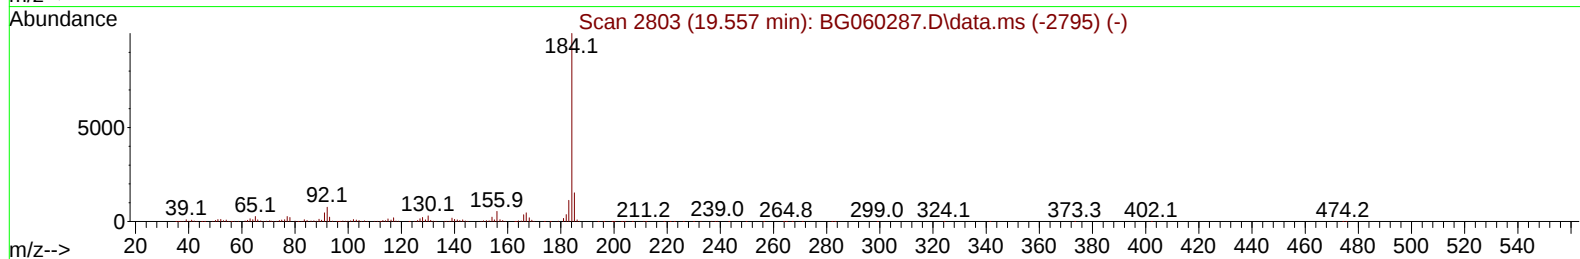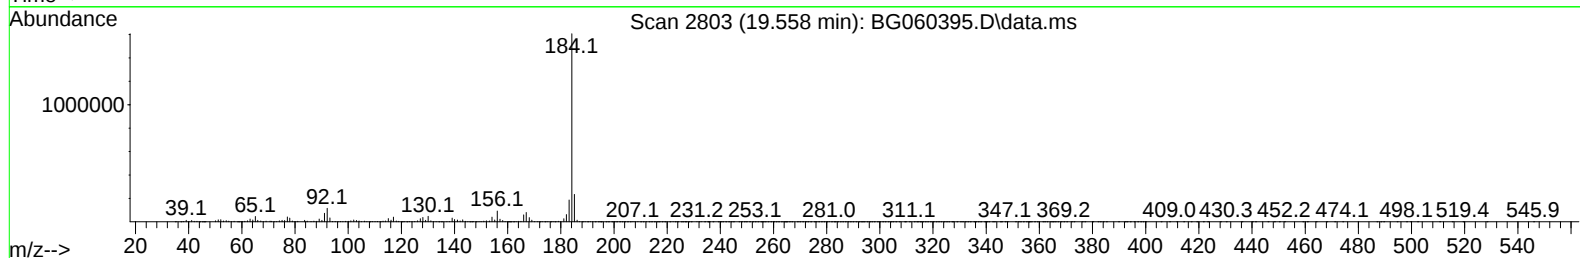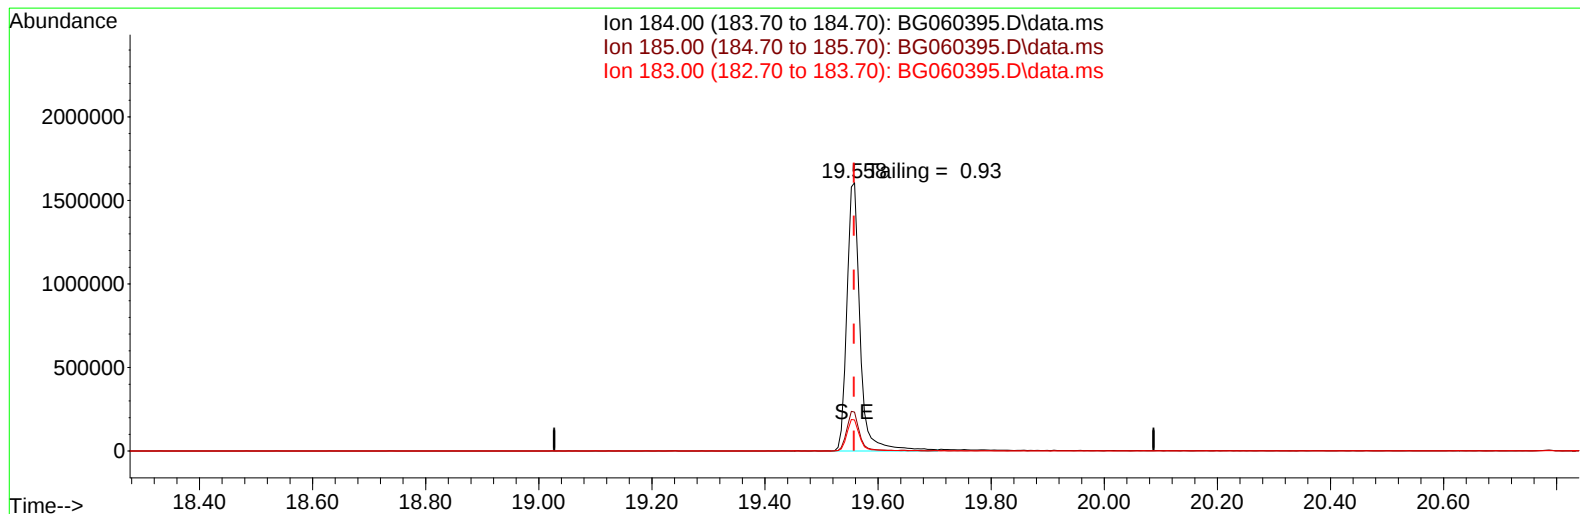

TIC: BG060395.D\data.ms

(77) Benzidine

19.558min (+ 0.001) 531762.15 ng

response 2610897

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.53
183.00	11.20	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2024	BNA_G	<u>BG060395.D</u>
Compound Name	Response	Retention Time
DDT	1259274	20.786
DDD	40752	20.346
DDE	3509	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44261	1303535	3.40

Instrument :
BNA_G
ClientSampleId :
DFTPP