
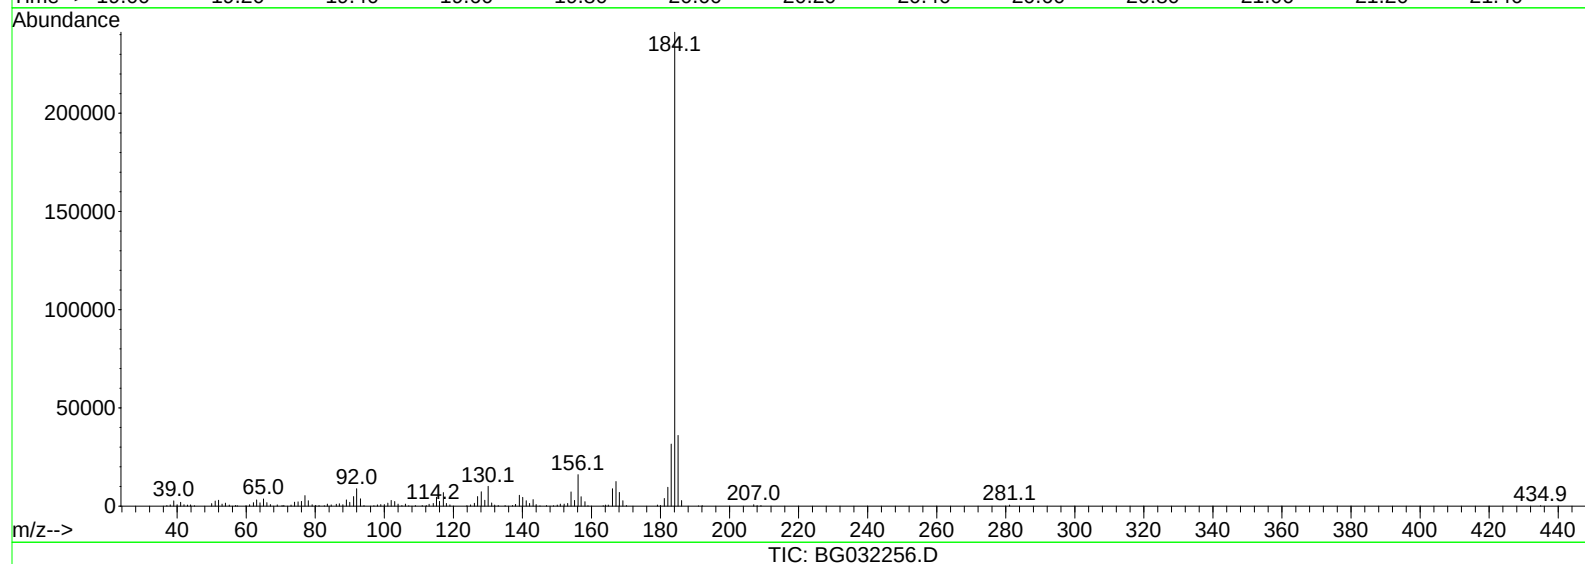


Data Path : U:\HPCHEM1\BNA G\DATA\BG012418\
Data File : BG032256.D
Acq On : 24 Jan 2018 12:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 12:42:46 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

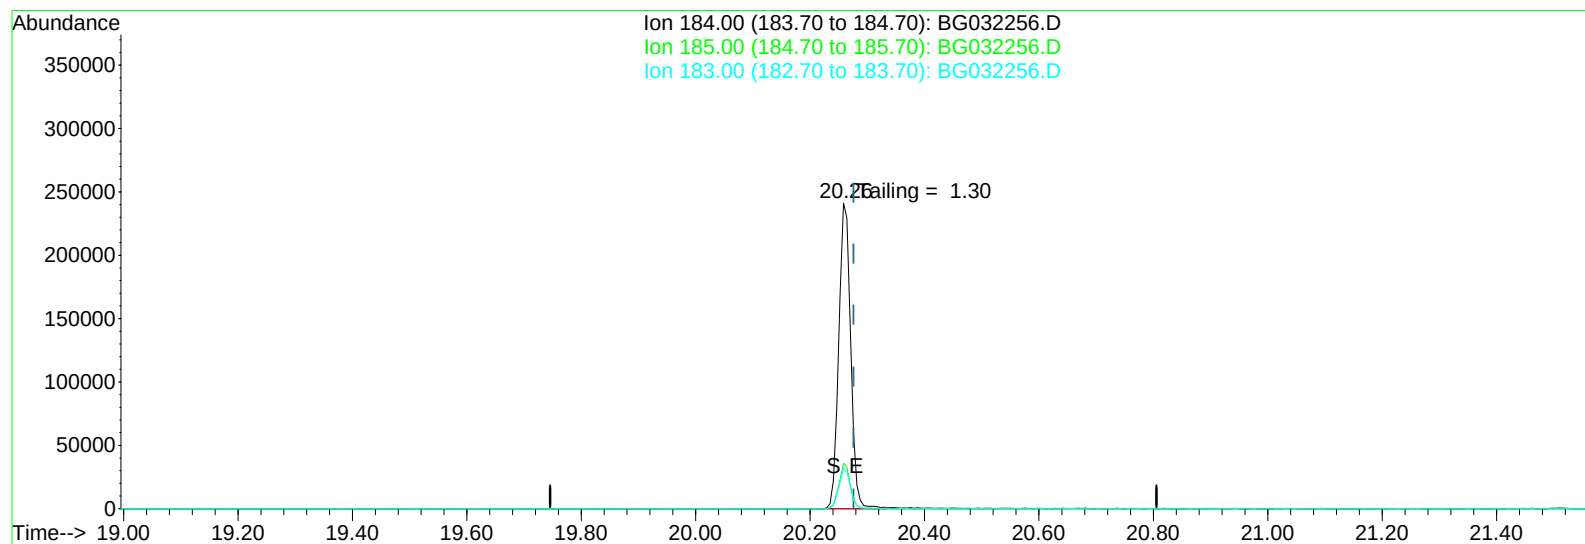

(76) Benzidine



20.258min (-0.017) 0.00ng

response 349528

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.91
183.00	13.30	13.07
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012418\
Data File : BG032256.D
Acq On : 24 Jan 2018 12:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 12:42:46 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

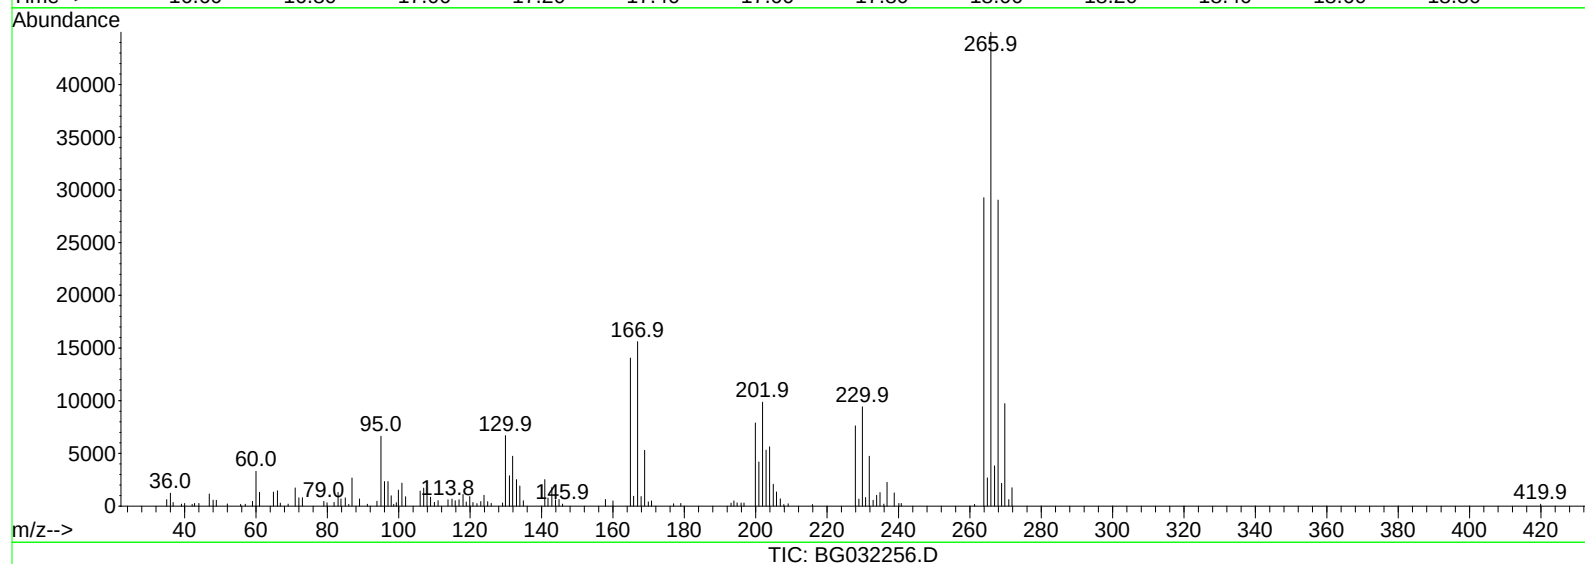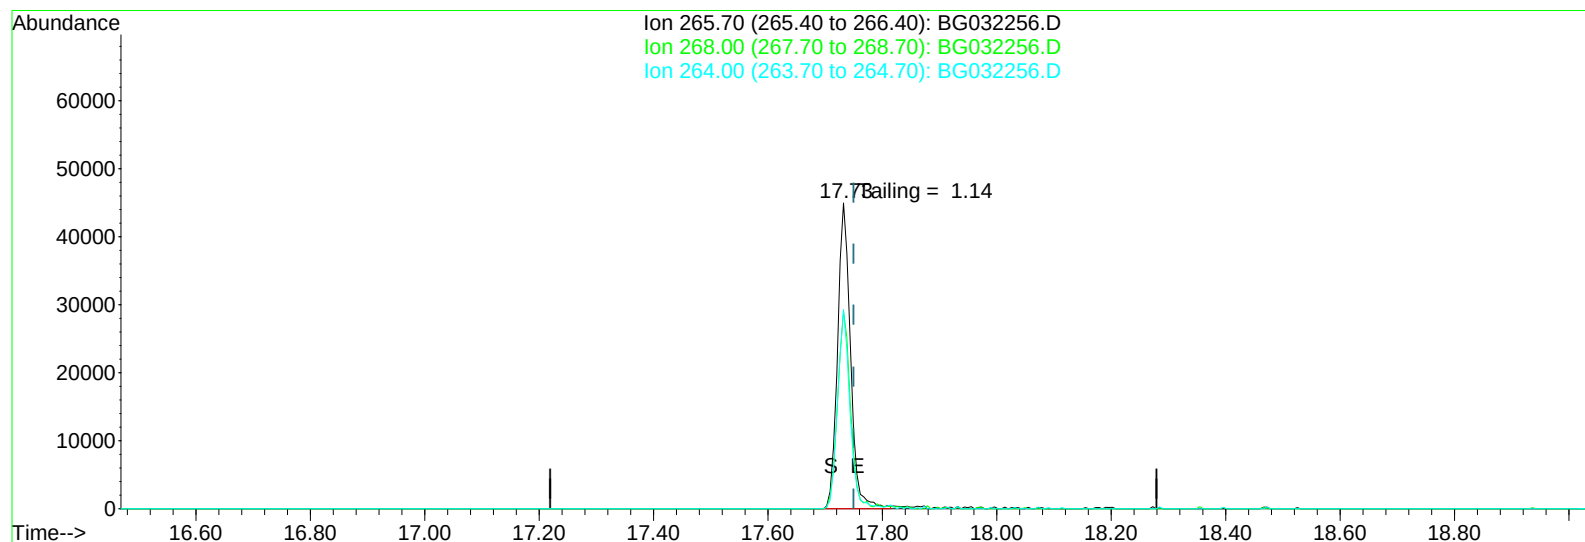

(69) Pentachlorophenol (C)

17.732min (-0.017) 23249.79ng

response 70413

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.59
264.00	62.00	65.07
0.00	0.00	0.00