


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012418\
 Data File : BG032256.D
 Acq On : 24 Jan 2018 12:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

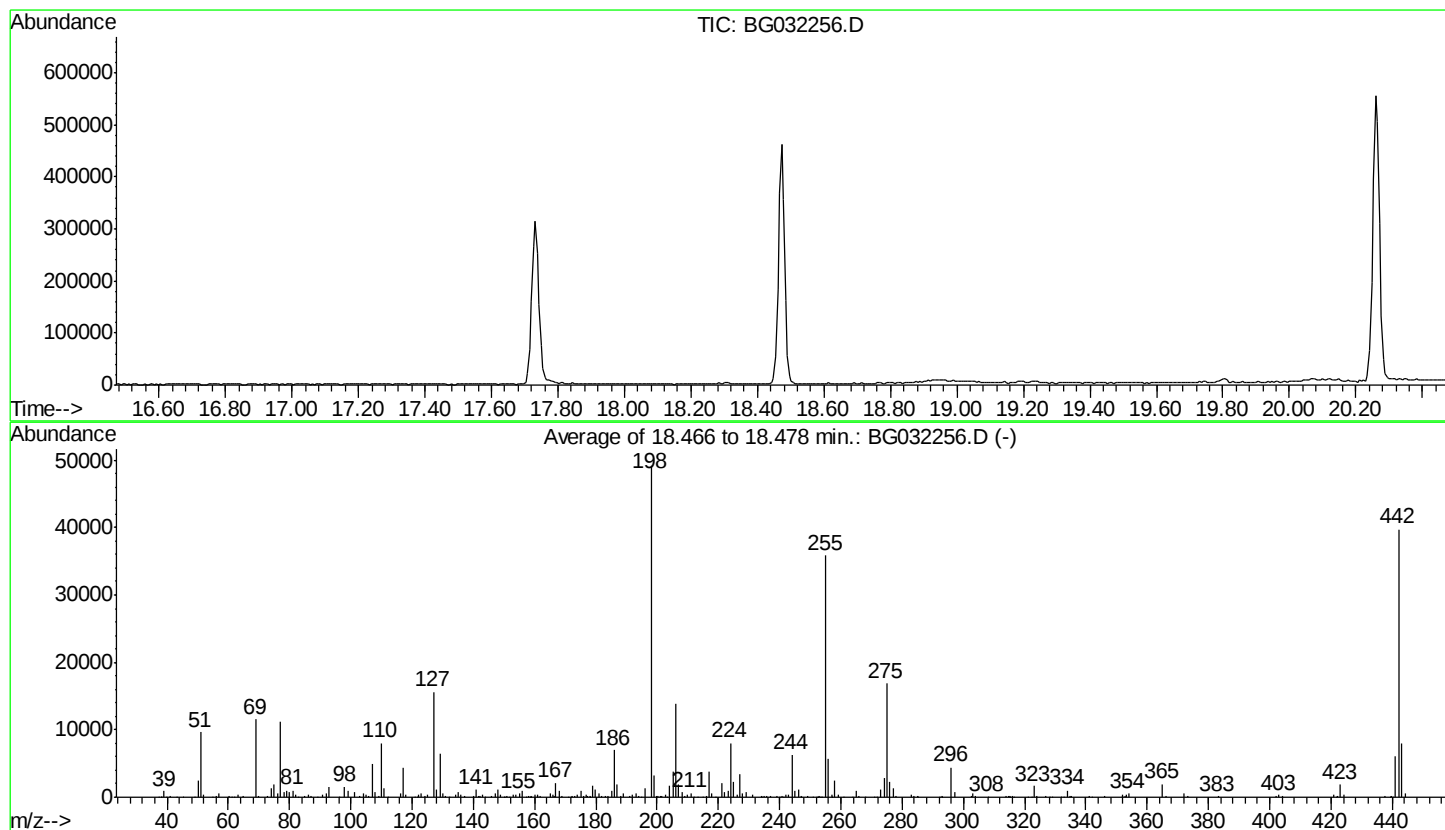

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.5	9602	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.4	11533	PASS
70	69	0.00	2	0.9	106	PASS
127	198	10	80	31.7	15600	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49184	PASS
199	198	5	9	6.5	3194	PASS
275	198	10	60	34.3	16873	PASS
365	198	1	100	3.9	1935	PASS
441	442	0.01	24	15.3	6069	PASS
442	198	50	100	80.7	39712	PASS
443	442	15	24	20.0	7952	PASS