


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012418\
 Data File : BG032275.D
 Acq On : 25 Jan 2018 00:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 24 14:02:41 2018

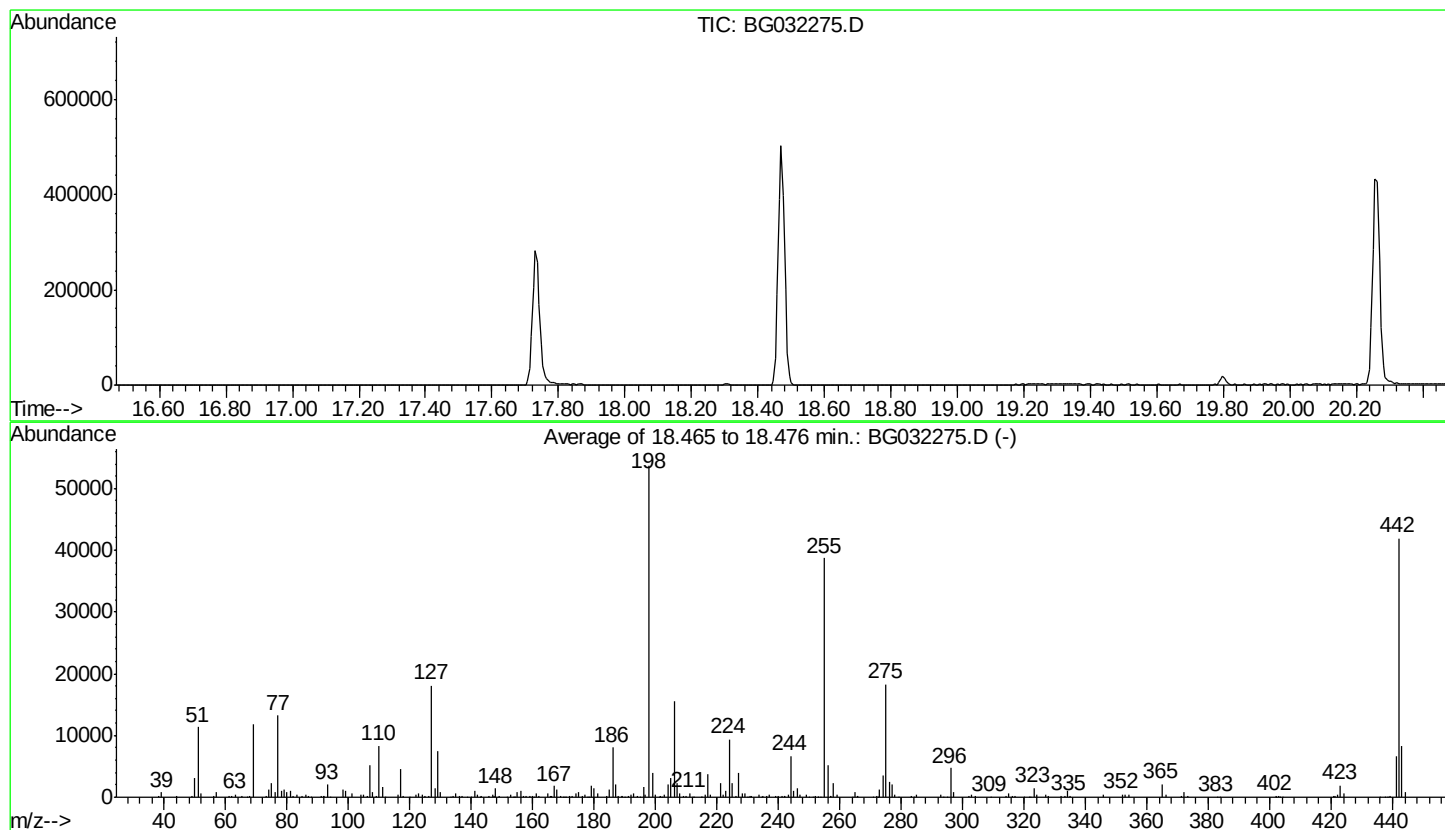

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	11312	PASS
68	69	0.00	2	1.0	116	PASS
69	198	0.00	100	22.0	11798	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.8	18135	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53701	PASS
199	198	5	9	7.2	3852	PASS
275	198	10	60	34.1	18317	PASS
365	198	1	100	3.9	2096	PASS
441	442	0.01	24	15.9	6652	PASS
442	198	50	100	78.0	41882	PASS
443	442	15	24	19.7	8268	PASS