

Data File : BG044179.D
Acq On : 24 Jan 2020 13:13
Operator : CG/JU
Sample : PB126313BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB126313BL

Quant Time: Jan 25 05:33:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	74762	20.00	ng	-0.04
21) Naphthalene-d8	10.73	136	319863	20.00	ng	-0.04
39) Acenaphthene-d10	14.56	164	215966	20.00	ng	-0.04
64) Phenanthrene-d10	17.31	188	477622	20.00	ng	-0.03
76) Chrysene-d12	21.55	240	417300	20.00	ng	-0.04
87) Perylene-d12	24.66	264	454954	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	562130	138.06	ng	-0.03
7) Phenol-d6	7.10	99	737726	129.62	ng	-0.02
23) Nitrobenzene-d5	9.08	82	442557	74.02	ng	-0.04
42) 2,4,6-Tribromophenol	16.06	330	277237	122.67	ng	-0.03
45) 2-Fluorobiphenyl	13.19	172	1055592	88.56	ng	-0.04
79) Terphenyl-d14	19.92	244	1638742	98.66	ng	-0.03
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.08	70	56622	13.359	ng	# 76
51) 2,6-Dinitrotoluene	14.56	165	28229	8.145	ng	# 26
57) 2,4-Dinitrotoluene	14.56	165	28344	6.010	ng	# 27
65) 4,6-Dinitro-2-methylphenol	16.05	198	838	4.699	ng	# 1
67) 4-Bromophenyl-phenylether	16.05	248	19525	3.635	ng	# 1
77) Benzidine	19.92	184	27352	2.608	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG044179.D
Acq On : 24 Jan 2020 13:13
Operator : CG/JU
Sample : PB126313BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB126313BL

Quant Time: Jan 25 05:33:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

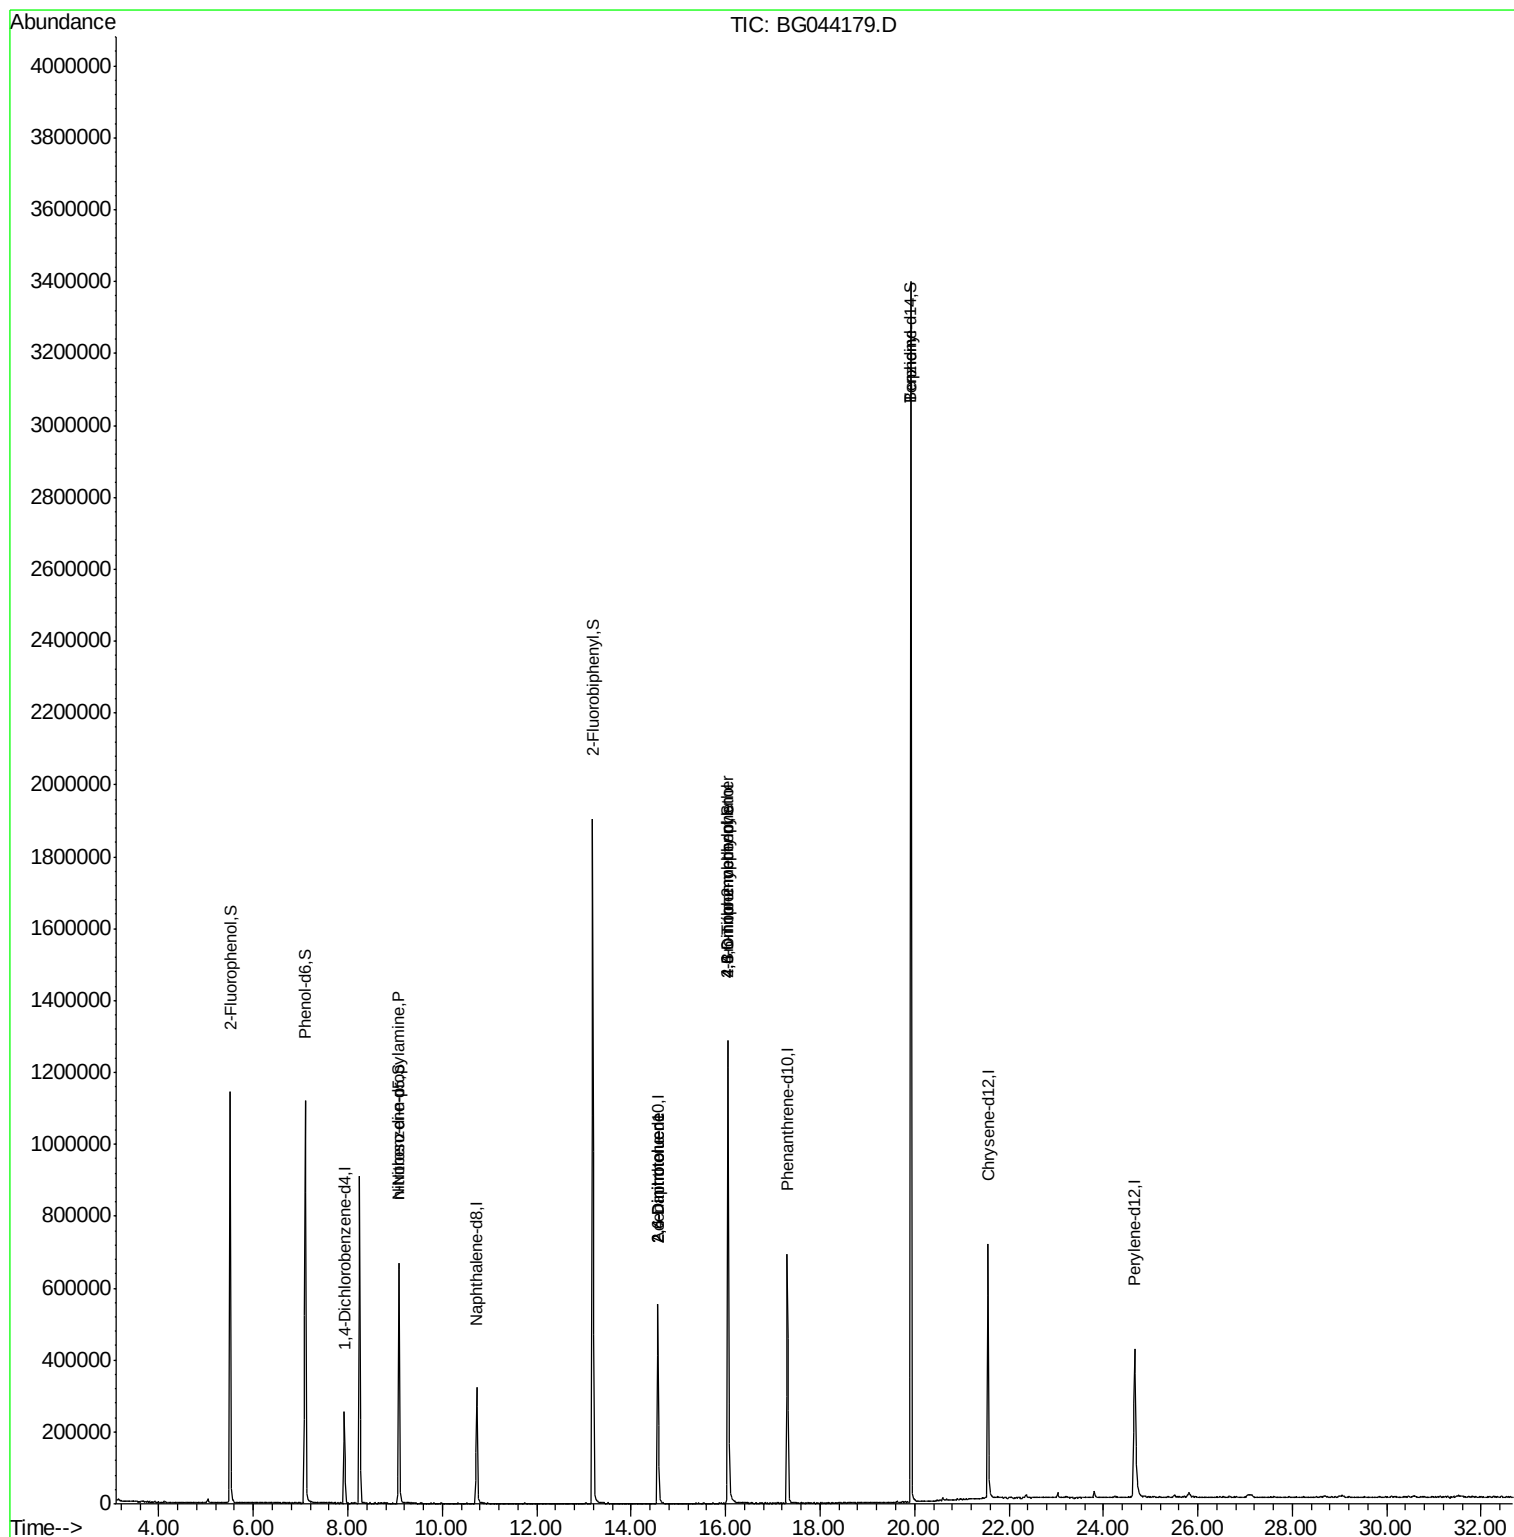

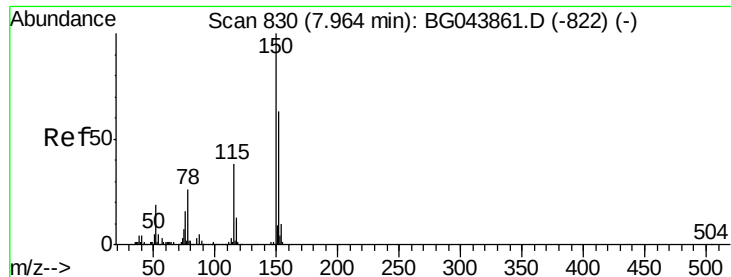


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.93 min Scan# 824
Delta R.T. -0.04 min
Lab File: BG044179.D
Acq: 24 Jan 2020 13:13

Instrument :
BNA_G
ClientSampleId :
PB126313BL

Tgt Ion:152 Resp: 74762
Ion Ratio Lower Upper
152 100
150 156.0 127.0 190.4
115 57.0 47.8 71.8

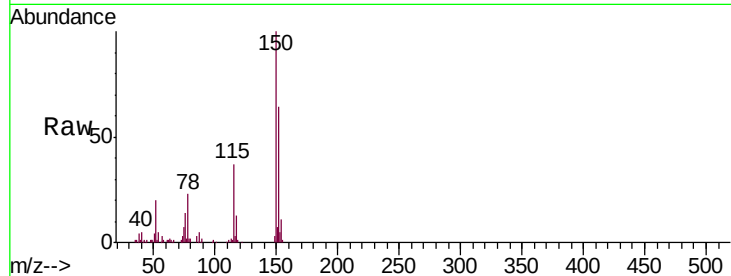


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

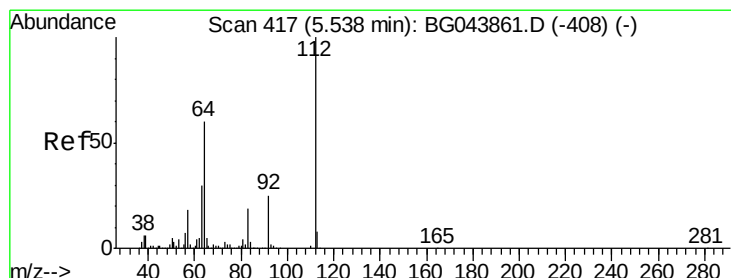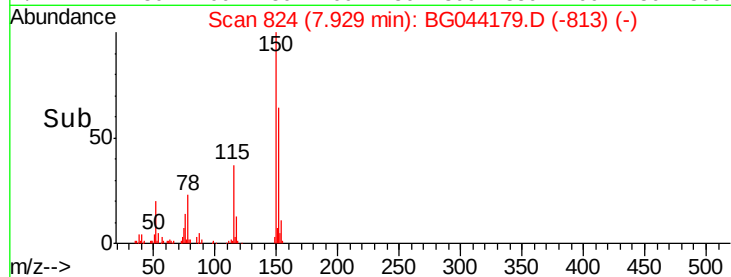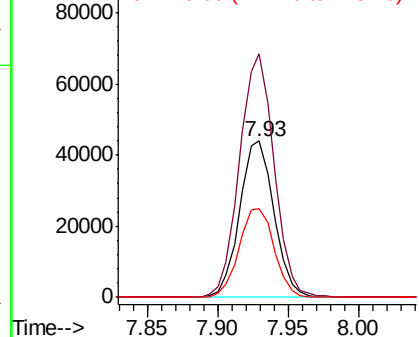



#5


2-Fluorophenol
Concen: 138.057 ng
RT: 5.51 min Scan# 412
Delta R.T. -0.03 min
Lab File: BG044179.D
Acq: 24 Jan 2020 13:13

Tgt Ion:112 Resp: 562130
Ion Ratio Lower Upper
112 100
64 57.7 47.8 71.6
63 29.5 24.3 36.5

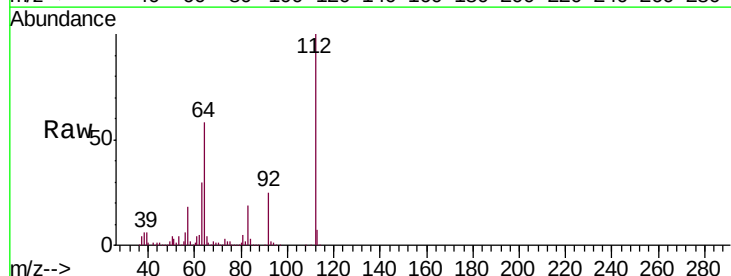

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

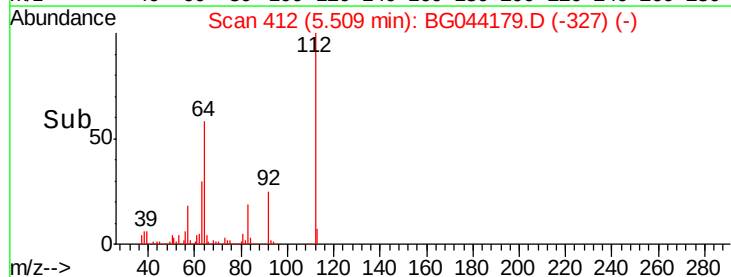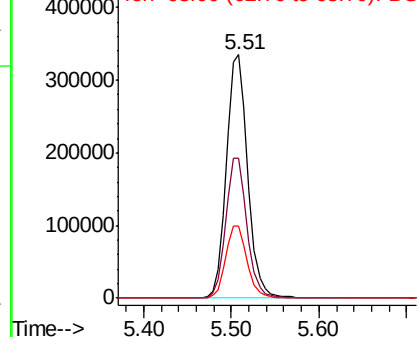



#7

Phenol-d6

Concen: 129.618 ng

RT: 7.10 min Scan# 683

Delta R.T. -0.02 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13

Instrument :

BNA_G

ClientSampleId :

PB126313BL


Tgt Ion: 99 Resp: 737726

Ion Ratio Lower Upper




99 100

42 17.5 14.9 22.3

71 31.6 26.4 39.6



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

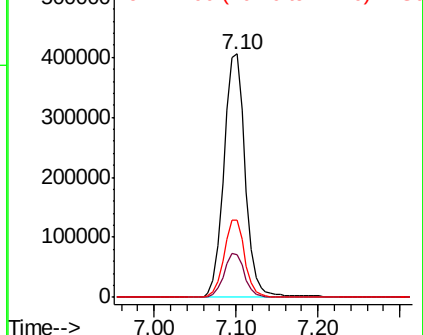

#19

n-Nitroso-di-n-propylamine

Concen: 13.359 ng

RT: 9.08 min Scan# 1020

Delta R.T. 0.31 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13

Tgt Ion: 70 Resp: 56622


Ion Ratio Lower Upper

70 100



42 44.0 47.0 70.4#


101 0.0 7.2 10.8#

130 2.1 15.6 23.4#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC



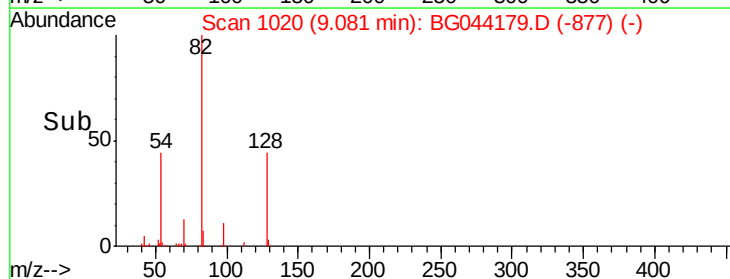
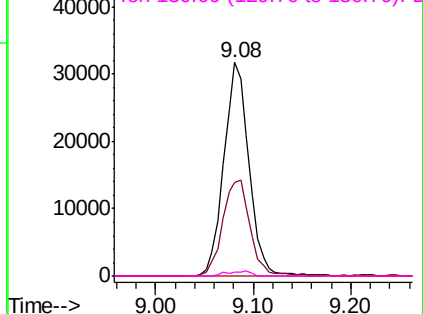




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.73 min Scan# 1300
Delta R.T. -0.04 min
Lab File: BG044179.D
Acq: 24 Jan 2020 13:13




Instrument :
BNA_G
ClientSampleId :
PB126313BL


Tgt Ion:	136	Resp:	319863
Ion	Ratio	Lower	Upper
136	100		
137	12.0	8.8	13.2
54	7.9	7.0	10.4
68	6.3	4.9	7.3

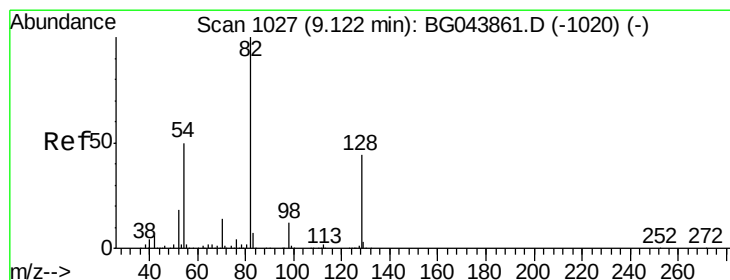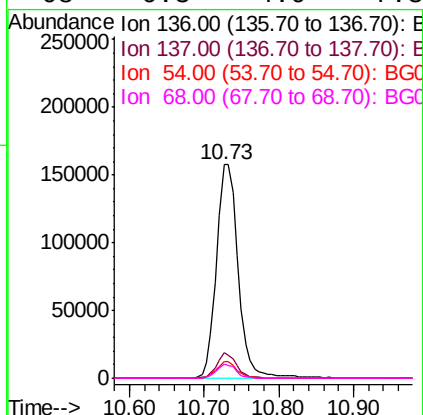

#23
Nitrobenzene-d5
Concen: 74.016 ng
RT: 9.08 min Scan# 1020
Delta R.T. -0.04 min
Lab File: BG044179.D
Acq: 24 Jan 2020 13:13

Tgt Ion:	82	Resp:	442557
Ion	Ratio	Lower	Upper
82	100		
128	44.4	35.1	52.7
54	47.0	40.1	60.1

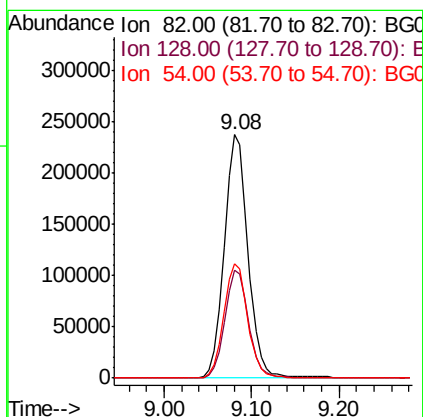

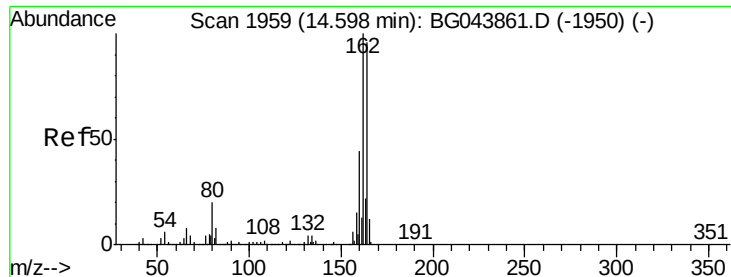

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.56 min Scan# 1953

Delta R.T. -0.04 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13

Instrument :

BNA_G

ClientSampleId :

PB126313BL


Tgt Ion:164 Resp: 215966

Ion Ratio Lower Upper

164 100

162 103.6 83.0 124.4




160 44.1 36.1 54.1

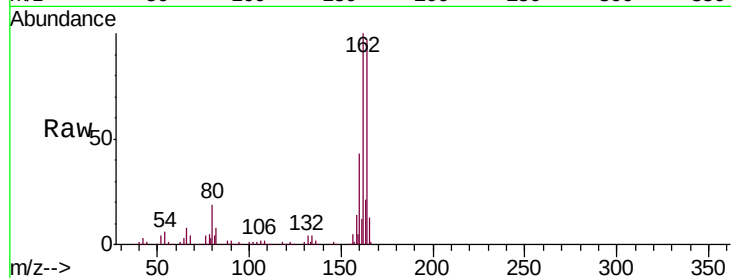

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

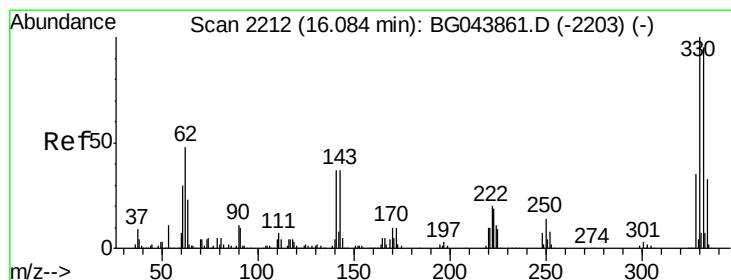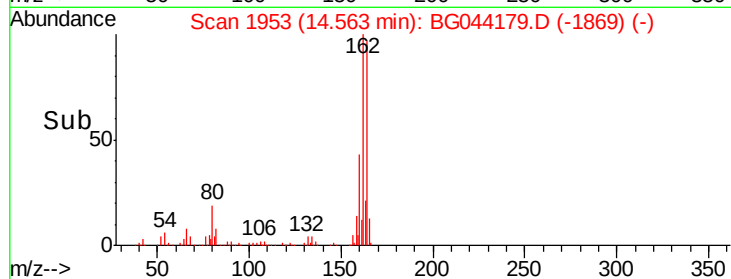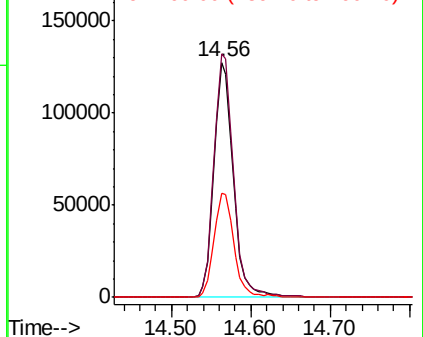

#42

2,4,6-Tribromophenol

Concen: 122.669 ng

RT: 16.06 min Scan# 2207

Delta R.T. -0.03 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13


Tgt Ion:330 Resp: 277237

Ion Ratio Lower Upper

330 100

332 97.1 77.2 115.8



141 38.8 33.1 49.7

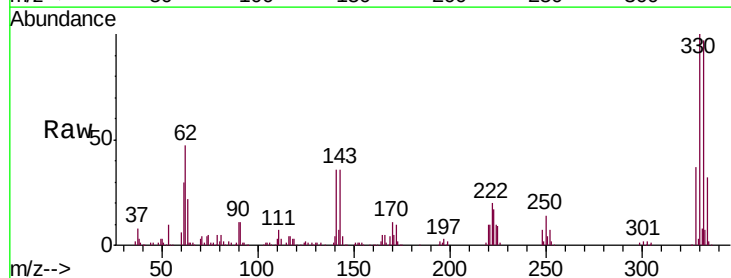


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



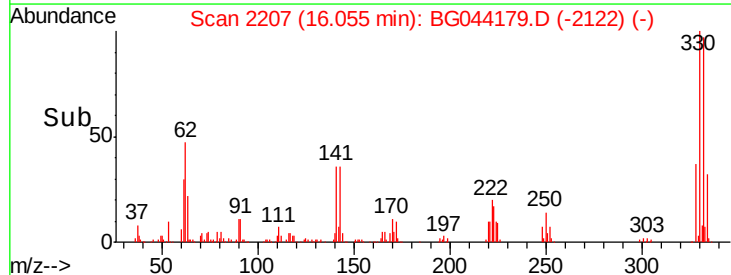
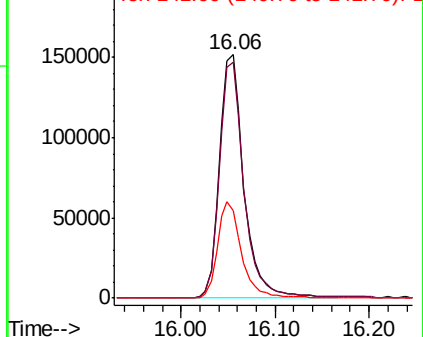




#45
 2-Fluorobiphenyl
 Concen: 88.555 ng
 RT: 13.19 min Scan# 1719
 Delta R.T. -0.04 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13




Instrument :
 BNA_G
 ClientSampleId :
 PB126313BL


Tgt Ion:172 Resp: 1055592
 Ion Ratio Lower Upper
 172 100
 171 39.4 35.8 53.8
 170 26.5 24.2 36.4

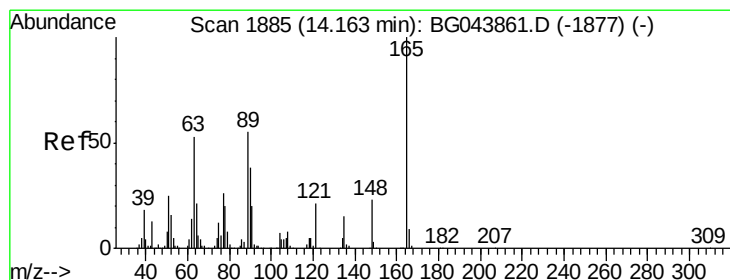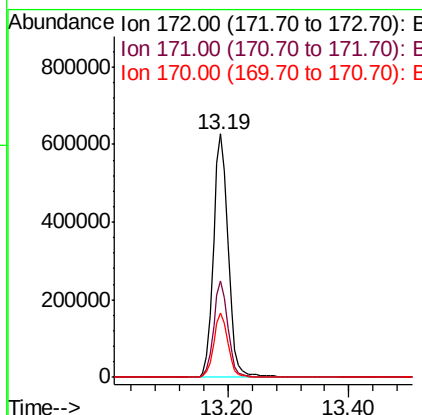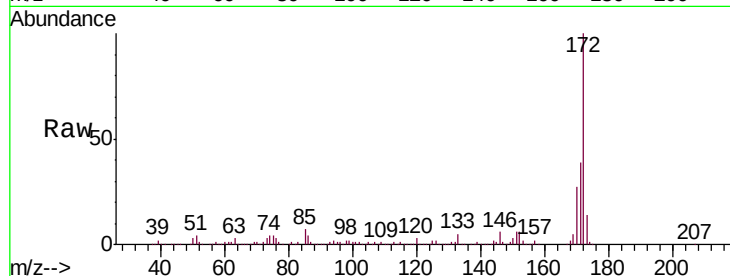

#51
 2,6-Dinitrotoluene
 Concen: 8.145 ng
 RT: 14.56 min Scan# 1953
 Delta R.T. 0.40 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13

Tgt Ion:165 Resp: 28229
 Ion Ratio Lower Upper
 165 100
 63 0.9 43.1 64.7#
 89 1.9 43.8 65.6#

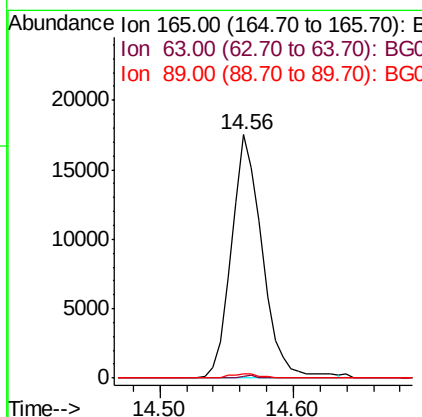




#57
 2,4-Dinitrotoluene
 Concen: 6.010 ng
 RT: 14.56 min Scan# 1953
 Delta R.T. -0.39 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13

Instrument :
 BNA_G
 ClientSampleId :
 PB126313BL

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.9	31.9	47.9#
89	1.9	53.8	80.6#
182	0.0	2.0	3.0#



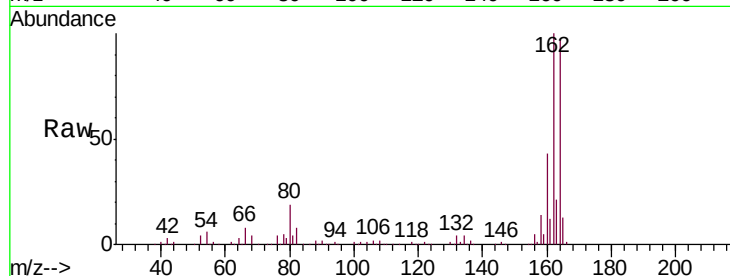


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

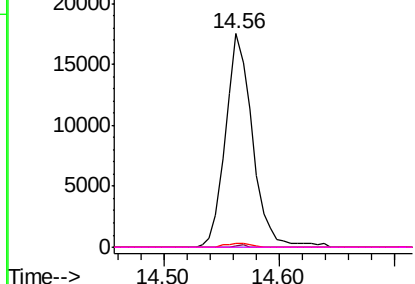

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.31 min Scan# 2420
 Delta R.T. -0.03 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13



Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.3	7.9	11.9
80	10.4	8.2	12.4




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

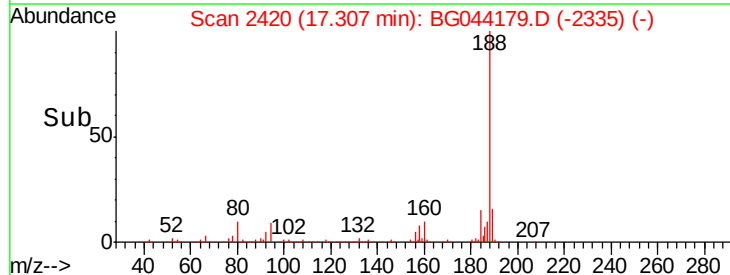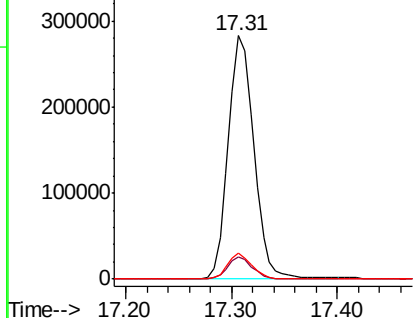


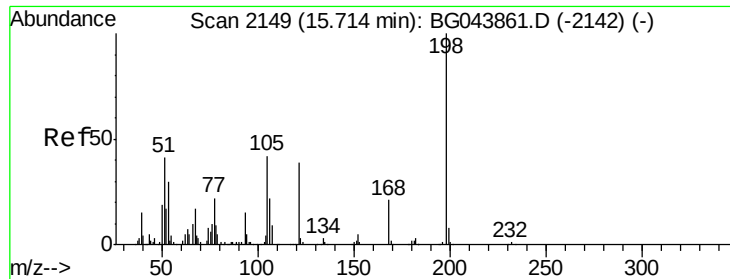




#65
 4,6-Dinitro-2-methylphenol
 Concen: 4.699 ng
 RT: 16.05 min Scan# 2206
 Delta R.T. 0.34 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13

Instrument :
 BNA_G
 ClientSampleId :
 PB126313BL

Tgt Ion:198 Resp: 838
 Ion Ratio Lower Upper
 198 100
 51 114.0 22.5 62.5#
 105 189.7 22.3 62.3#

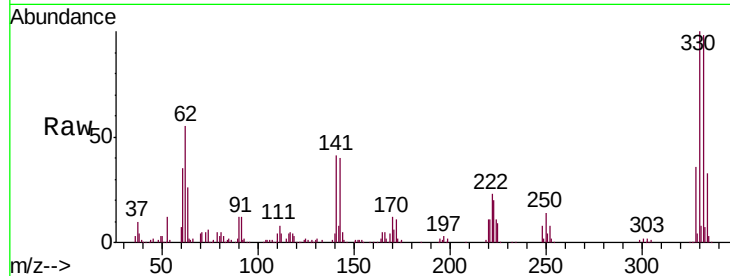


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG0
 Ion 105.00 (104.70 to 105.70): E


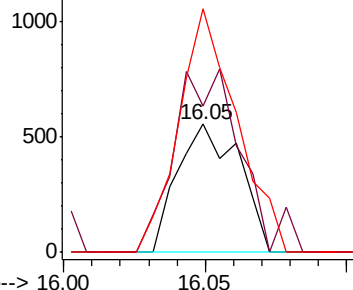



#67
 4-Bromophenyl-phenylether
 Concen: 3.635 ng
 RT: 16.05 min Scan# 2206
 Delta R.T. -0.48 min
 Lab File: BG044179.D
 Acq: 24 Jan 2020 13:13

Tgt Ion:248 Resp: 19525
 Ion Ratio Lower Upper
 248 100
 250 181.3 78.2 117.2#
 141 520.5 59.3 88.9#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

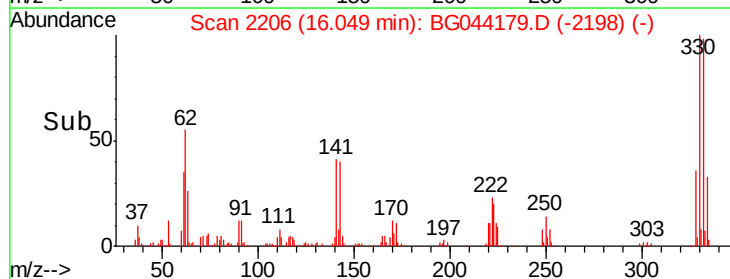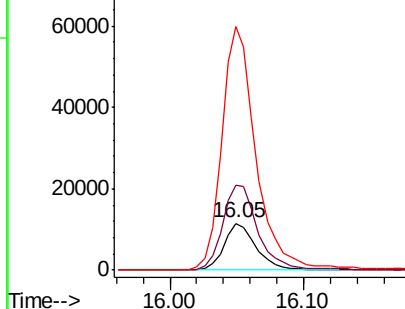

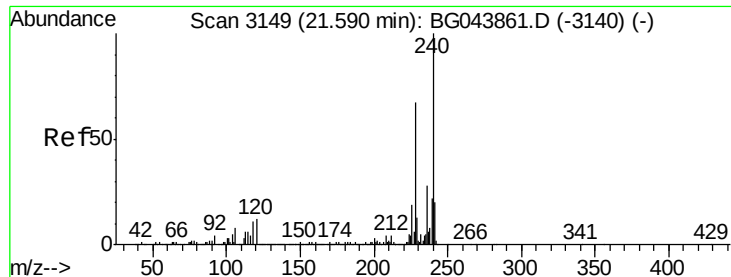

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.55 min Scan# 3143

Delta R.T. -0.04 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13

Instrument :

BNA_G

ClientSampleId :

PB126313BL


Tgt Ion:240 Resp: 417300

Ion Ratio Lower Upper

240 100

120 11.1 9.6 14.4




236 26.4 22.2 33.2

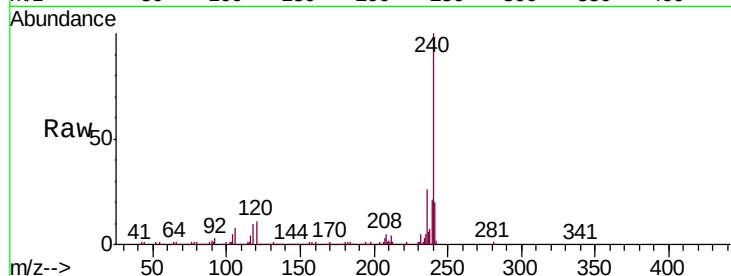

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

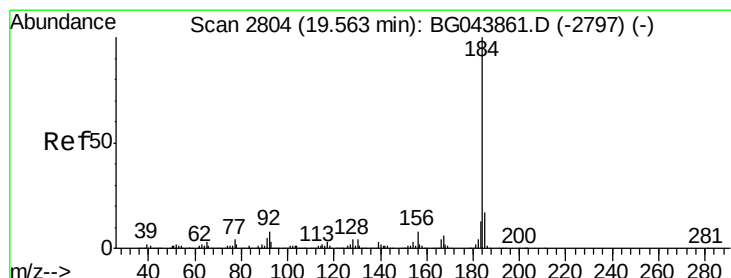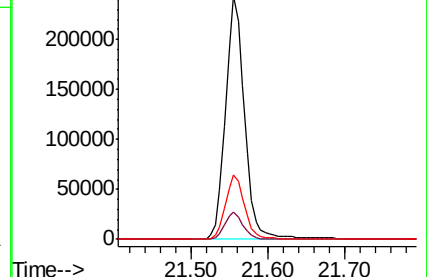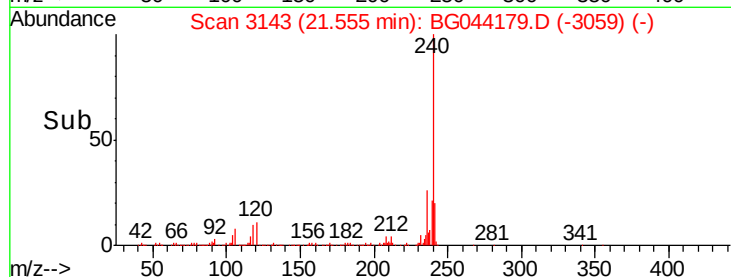

#77

Benzidine

Concen: 2.608 ng

RT: 19.92 min Scan# 2865

Delta R.T. 0.36 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13


Tgt Ion:184 Resp: 27352

Ion Ratio Lower Upper

184 100

185 14.7 13.4 20.0



183 7.0 10.6 15.8#

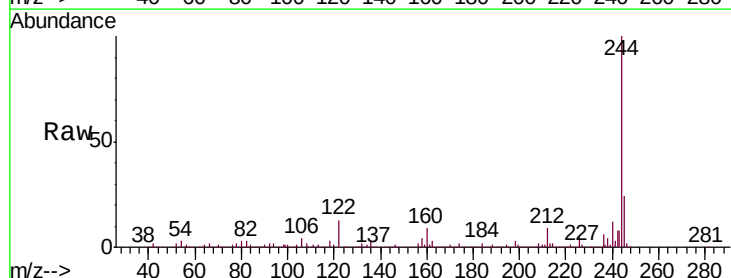


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

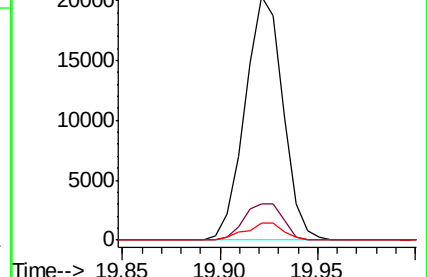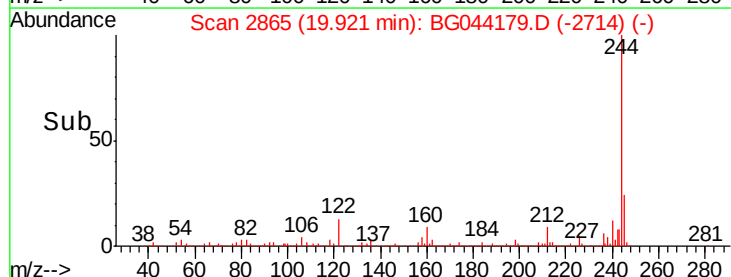

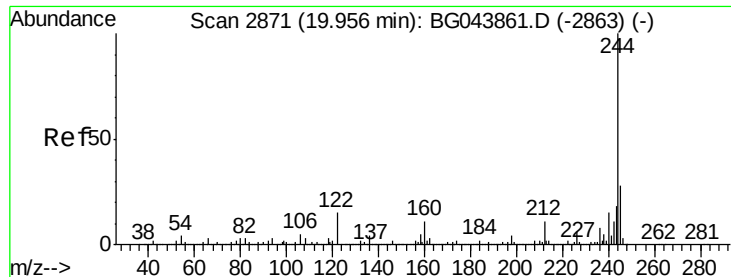

#79

Terphenyl-d14

Concen: 98.658 ng

RT: 19.92 min Scan# 2865

Delta R.T. -0.03 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13

Instrument :

BNA_G

ClientSampleId :

PB126313BL


Tgt Ion:244 Resp: 1638742

Ion Ratio Lower Upper

244 100

212 8.8 8.6 13.0




122 12.6 11.9 17.9

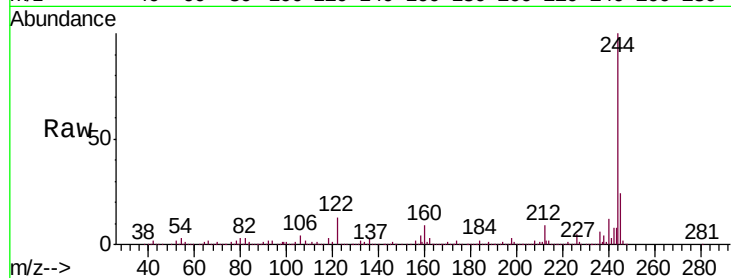

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

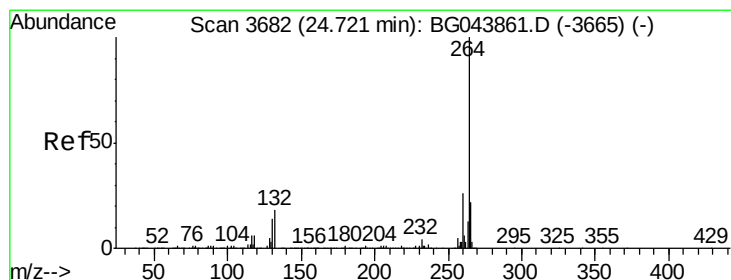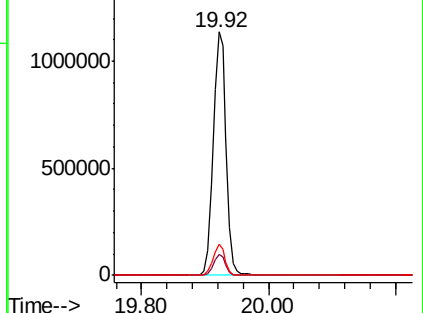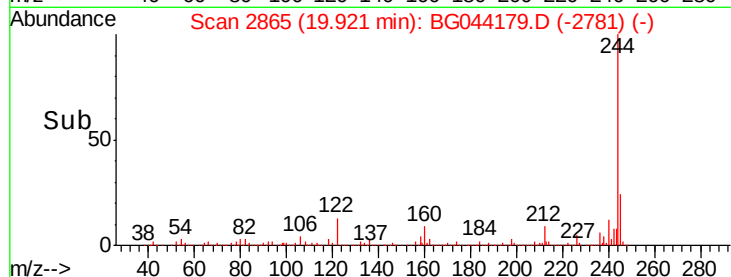

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.66 min Scan# 3672

Delta R.T. -0.06 min

Lab File: BG044179.D

Acq: 24 Jan 2020 13:13


Tgt Ion:264 Resp: 454954

Ion Ratio Lower Upper

264 100

260 24.2 20.4 30.6

265 22.3 17.4 26.2

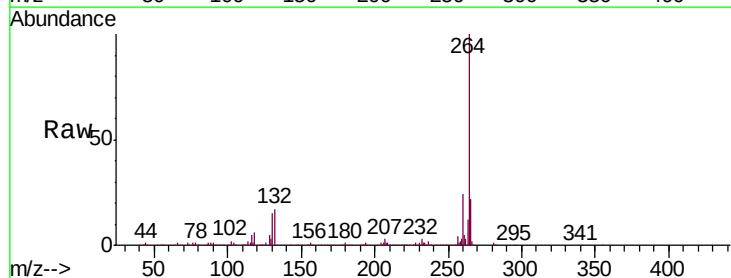

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

