
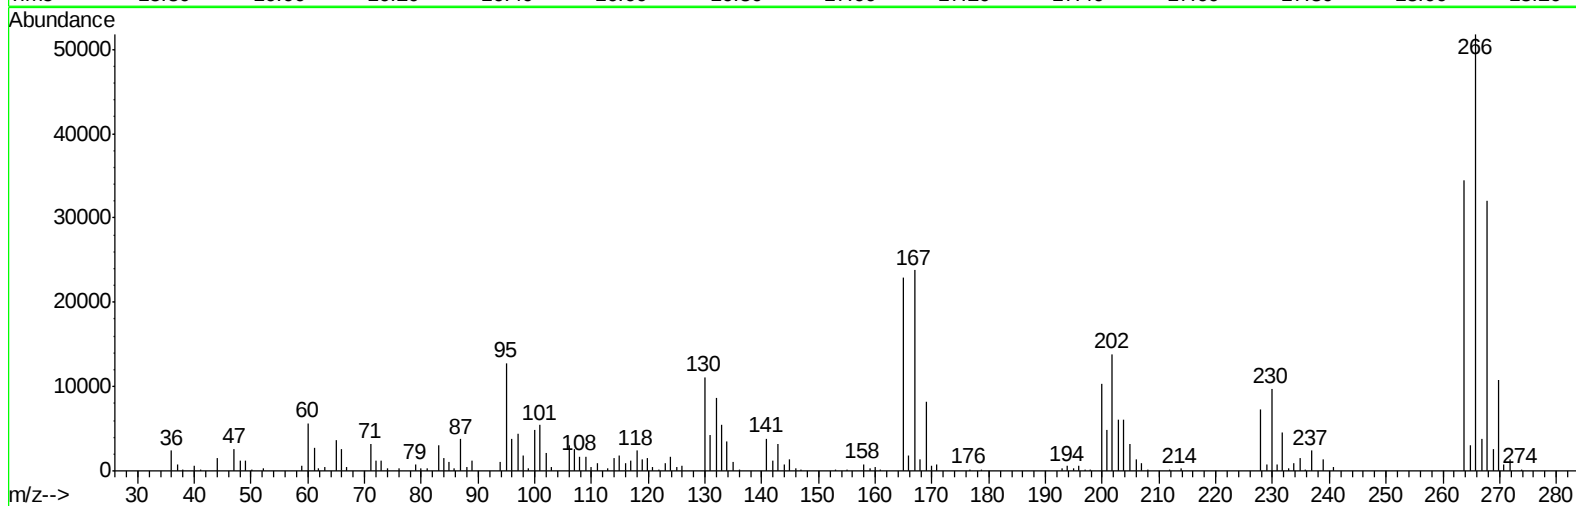


Data File : BG044175.D
Acq On : 24 Jan 2020 10:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:24:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

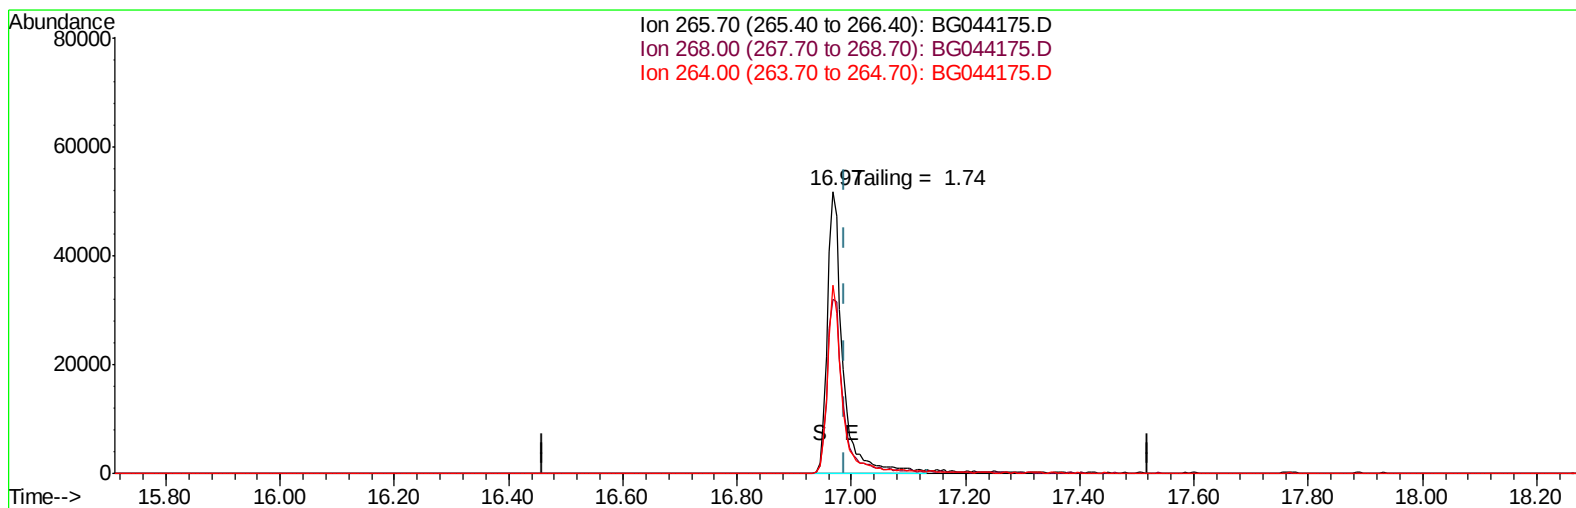

TIC: BG044175.D

(70) Pentachlorophenol (C)



16.968min (-0.021) 81723.69ng

response 97181

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	61.94
264.00	63.50	66.60
0.00	0.00	0.00

Data File : BG044175.D
Acq On : 24 Jan 2020 10:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:24:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

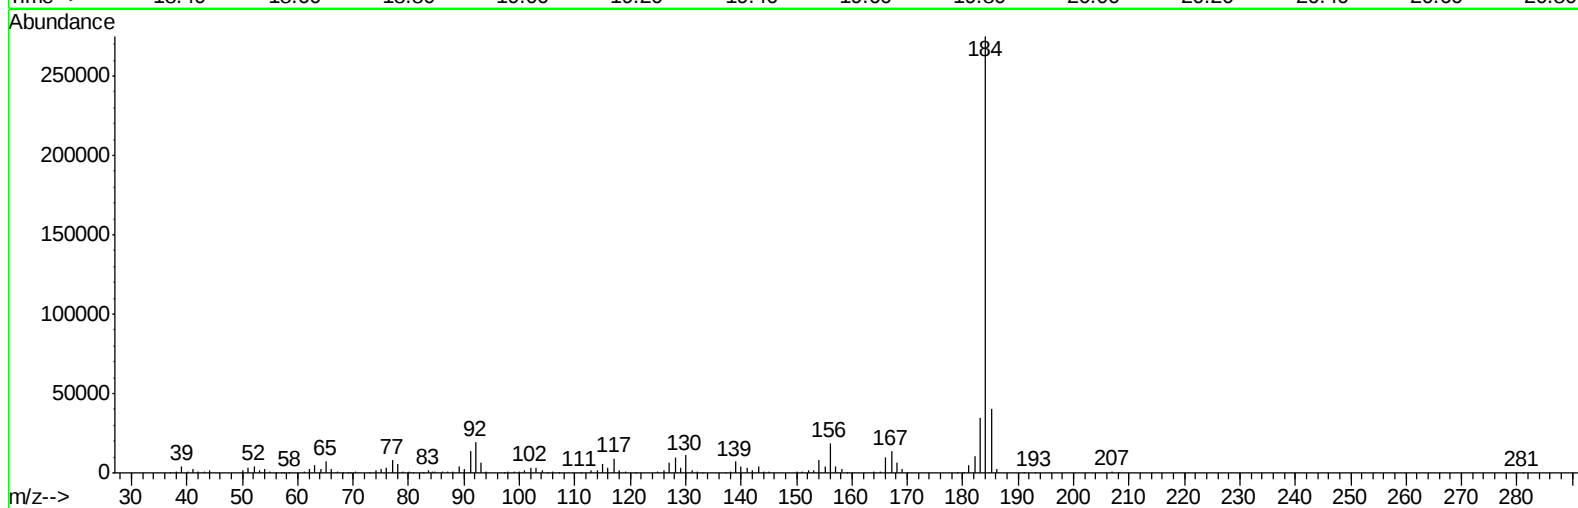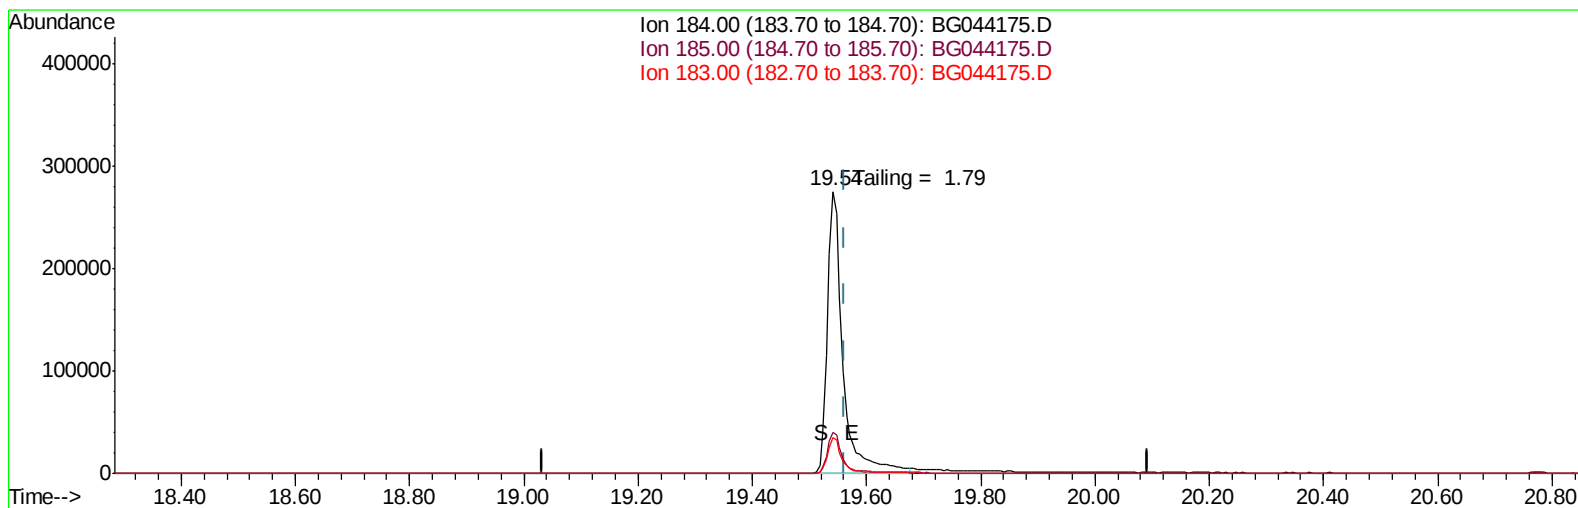

TIC: BG044175.D

(77) Benzidine

19.541min (-0.021) 83363.86ng

response 528042

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.75
183.00	13.20	12.65
0.00	0.00	0.00