
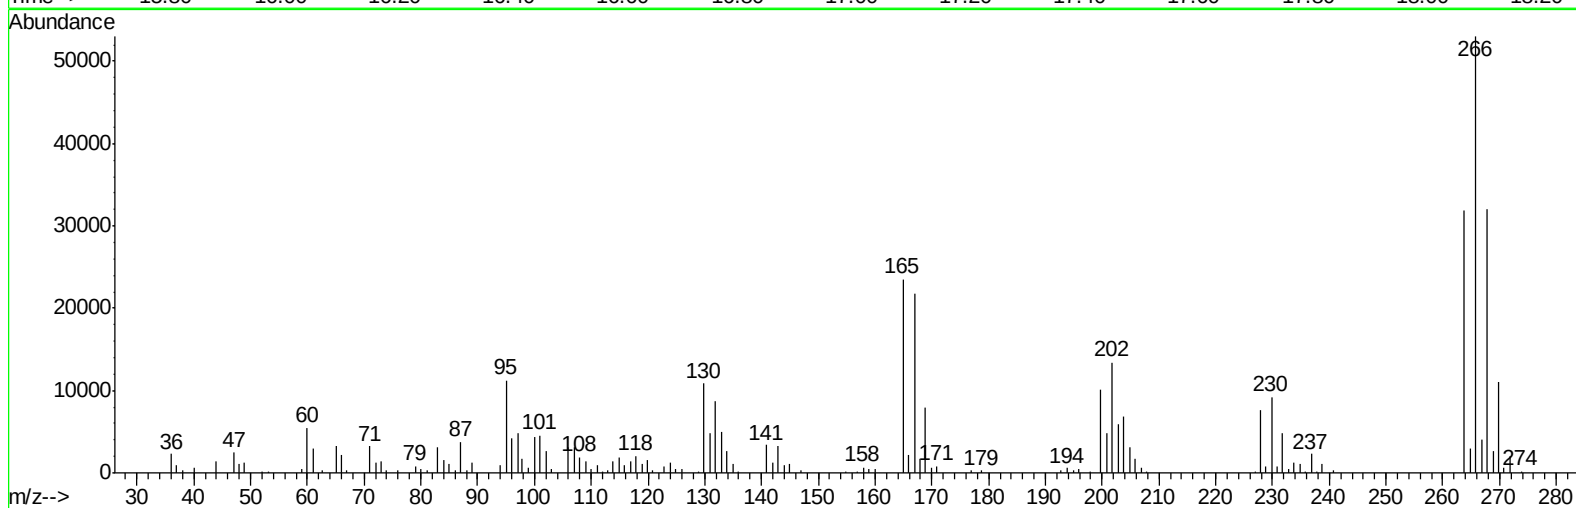


Data File : BG044194.D
Acq On : 24 Jan 2020 23:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:25:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

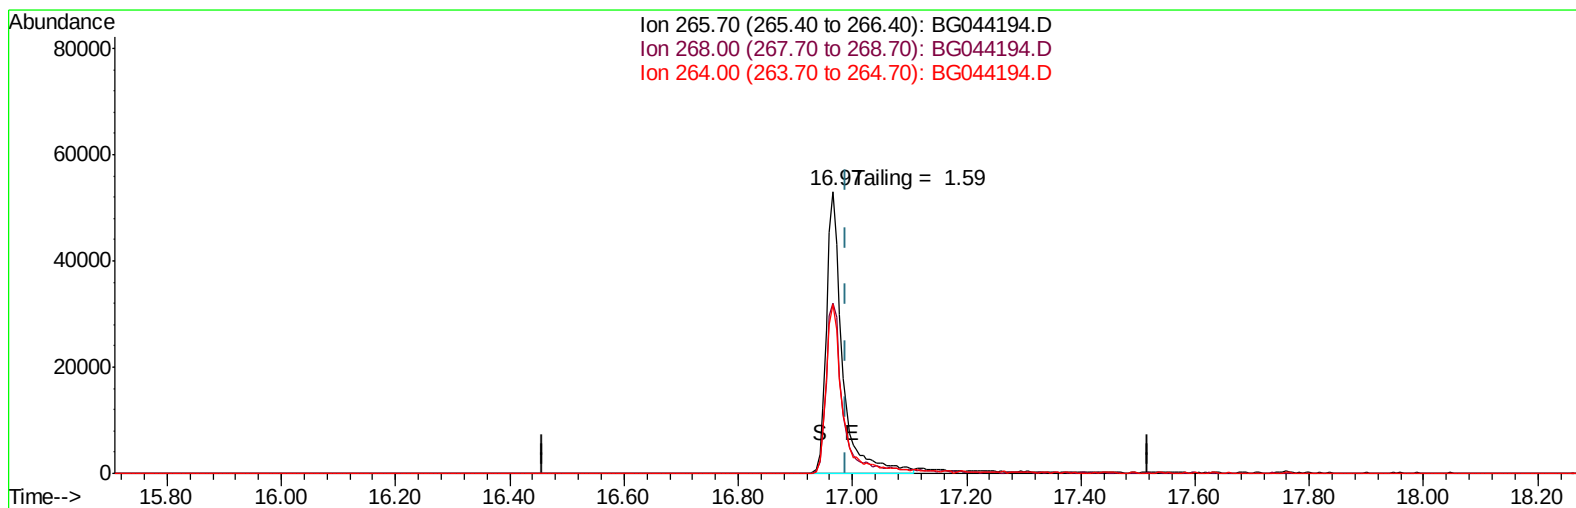

TIC: BG044194.D

(70) Pentachlorophenol (C)



16.966min (-0.023) 27396.33ng

response 103225

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	60.49
264.00	63.50	60.02
0.00	0.00	0.00

Data File : BG044194.D
Acq On : 24 Jan 2020 23:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:25:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

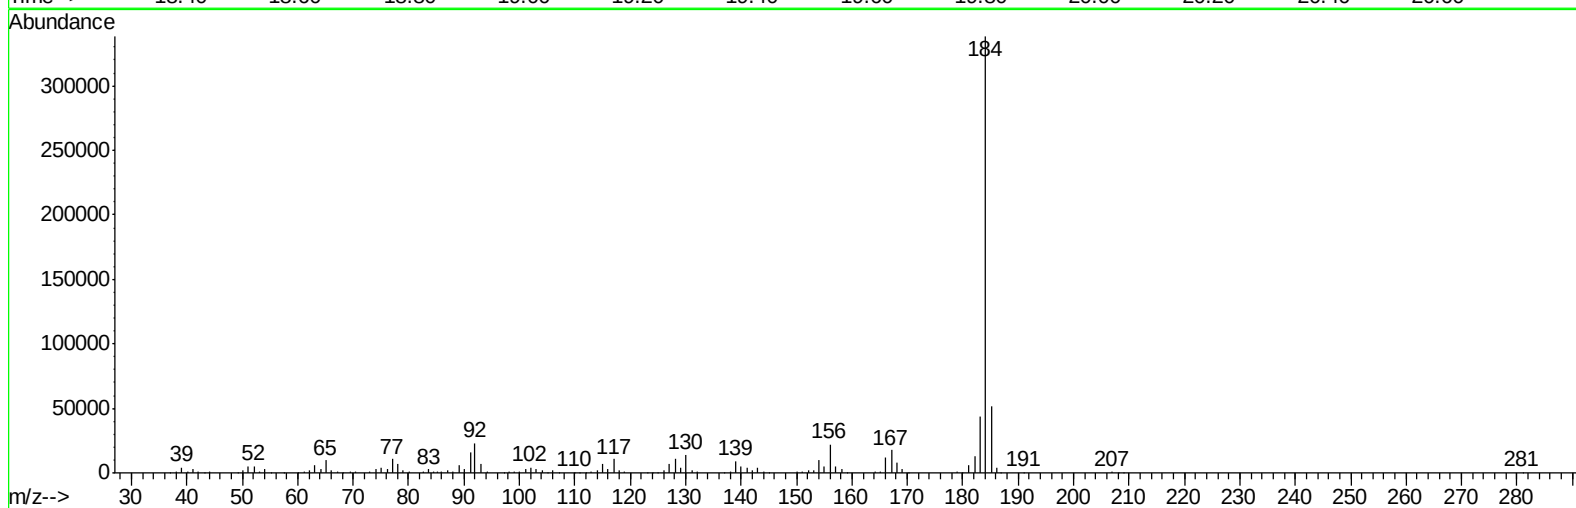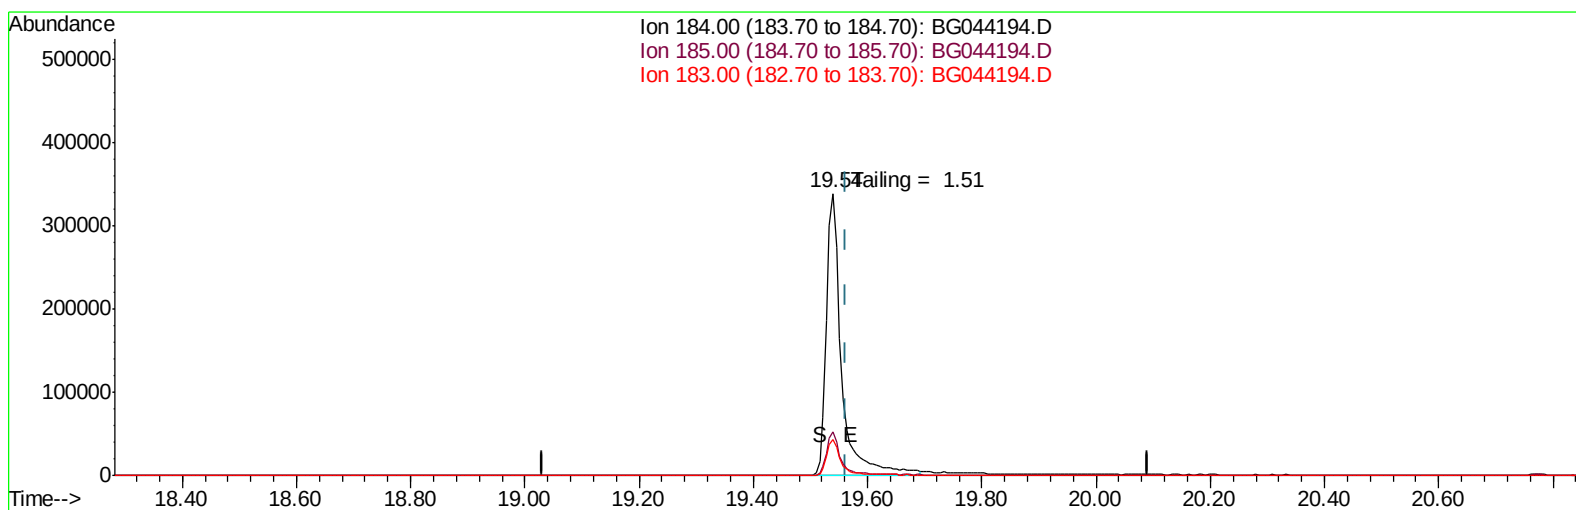

TIC: BG044194.D

(77) Benzidine

19.539min (-0.023) 0.00ng

response 640706

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.30
183.00	13.20	12.92
0.00	0.00	0.00