

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
 Data File : BG044193.D
 Acq On : 24 Jan 2020 22:21
 Operator : CG/JU
 Sample : L1245-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20200047-FIELD-BLANK

Quant Time: Jan 27 04:53:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 13:32:23 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	84037	20.00	ng	-0.03
21) Naphthalene-d8	10.73	136	378495	20.00	ng	-0.03
39) Acenaphthene-d10	14.56	164	257276	20.00	ng	-0.03
64) Phenanthrene-d10	17.31	188	520702	20.00	ng	-0.03
76) Chrysene-d12	21.55	240	451651	20.00	ng	-0.03
87) Perylene-d12	24.66	264	503236	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	269337	58.85	ng	-0.03
7) Phenol-d6	7.10	99	218598	34.17	ng	-0.03
23) Nitrobenzene-d5	9.08	82	585035	82.69	ng	-0.04
42) 2,4,6-Tribromophenol	16.05	330	367705	136.57	ng	-0.03
45) 2-Fluorobiphenyl	13.19	172	1381699	97.30	ng	-0.03
79) Terphenyl-d14	19.92	244	1972899	115.01	ng	-0.03
Target Compounds						
10) Phenol	7.12	94	14740	2.236	ng	Qvalue 93
50) Dimethylphthalate	14.02	163	57304	3.137	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
Data File : BG044193.D
Acq On : 24 Jan 2020 22:21
Operator : CG/JU
Sample : L1245-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20200047-FIELD-BLANK

Quant Time: Jan 27 04:53:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

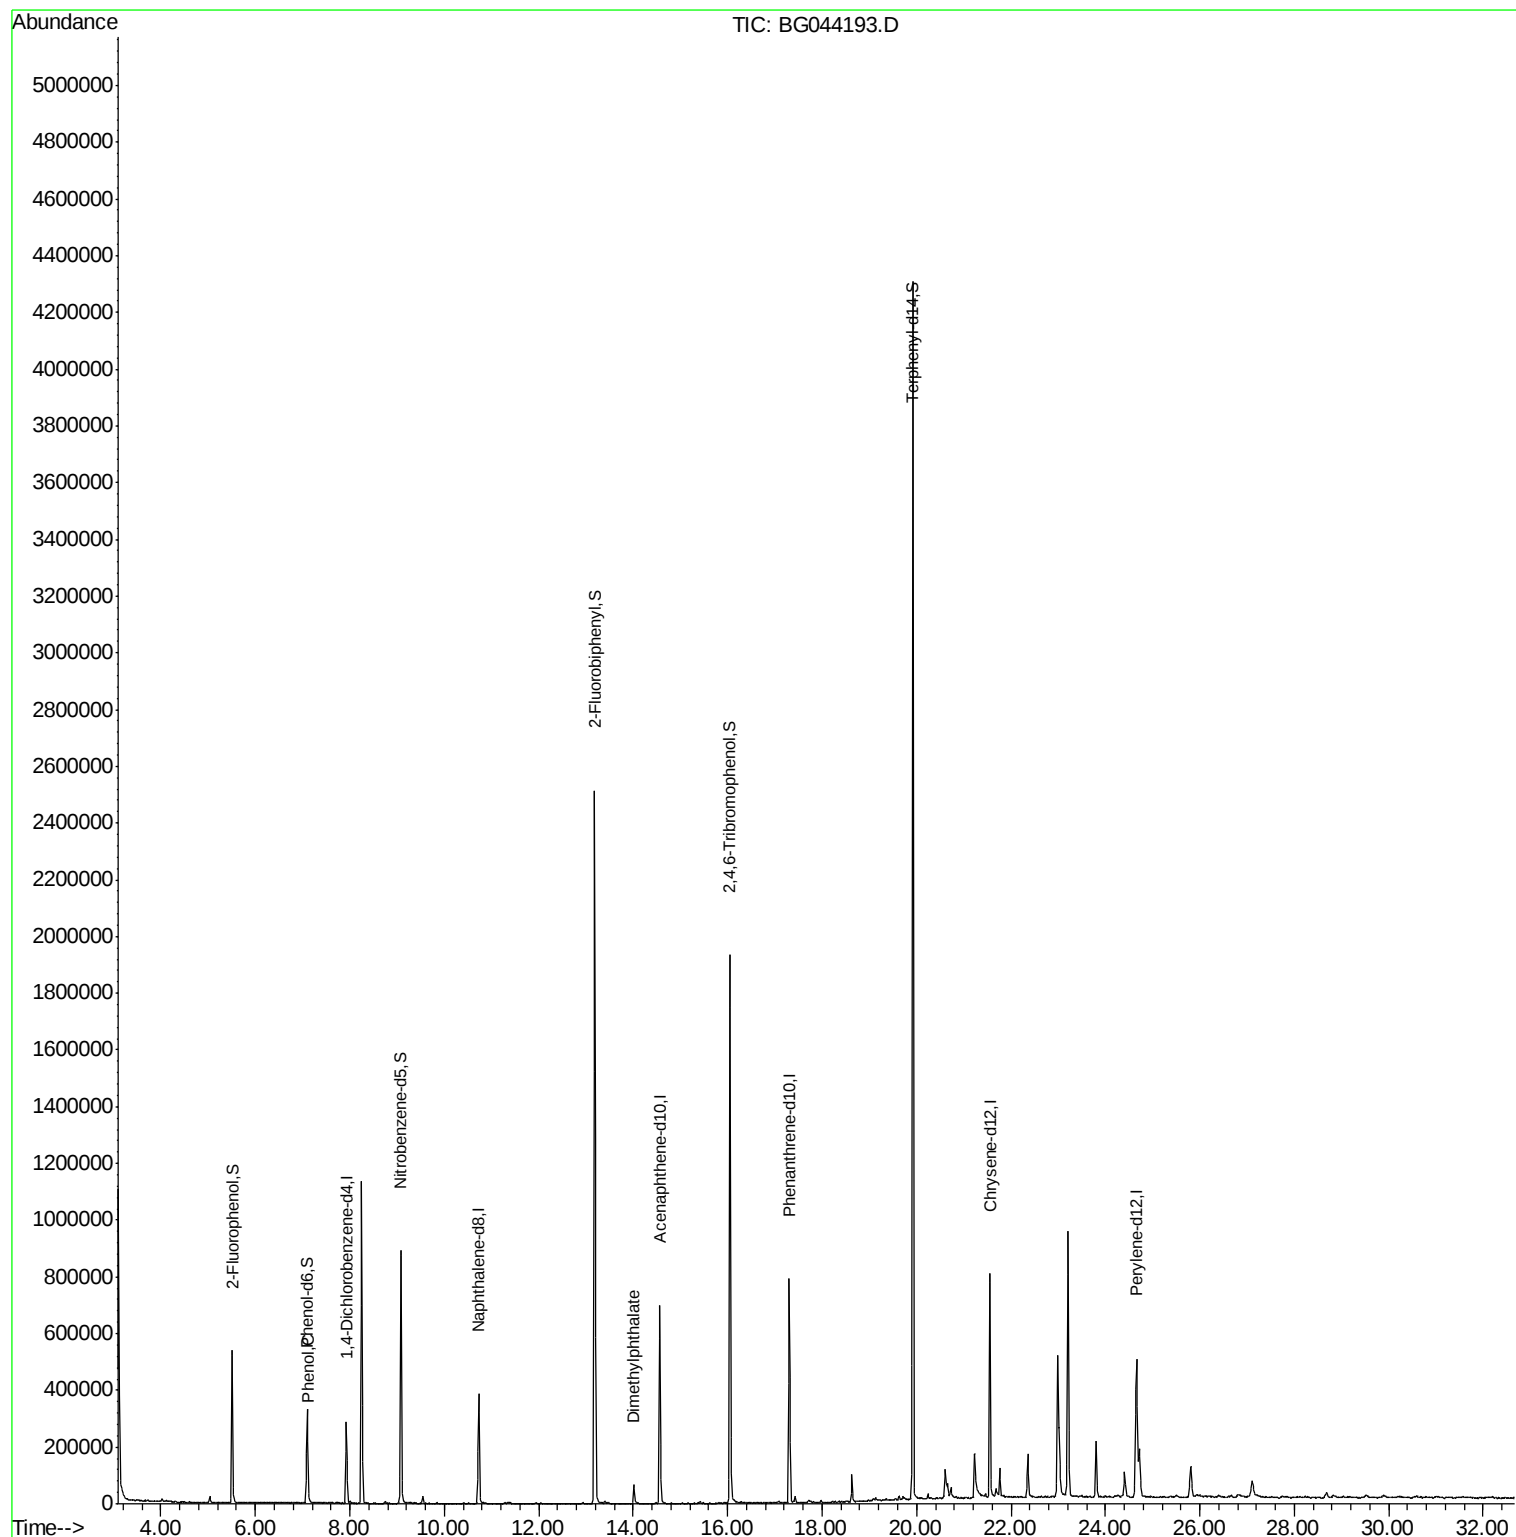




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.93 min Scan# 824
Delta R.T. -0.03 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21

Instrument :
BNA_G
ClientSampleId :
20200047-FIELD-BLANK

Tot Ion:152 Resp: 84037
Ion Ratio Lower Upper
152 100
150 160.3 127.0 190.4
115 60.6 47.8 71.8

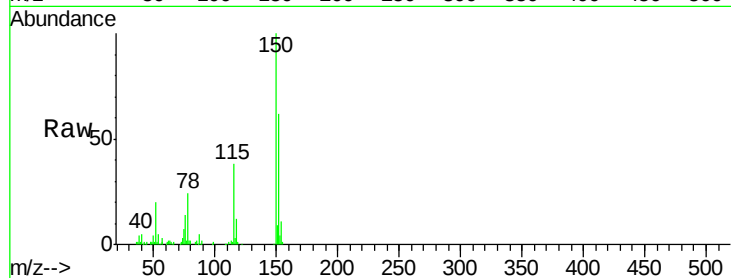


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

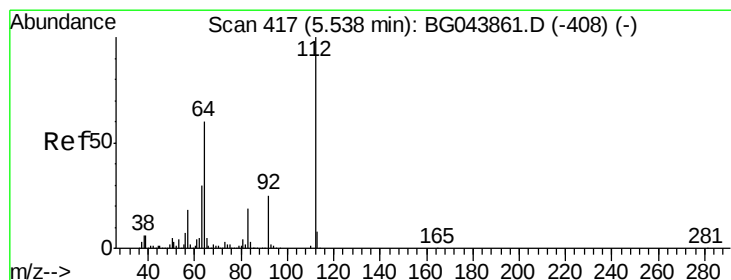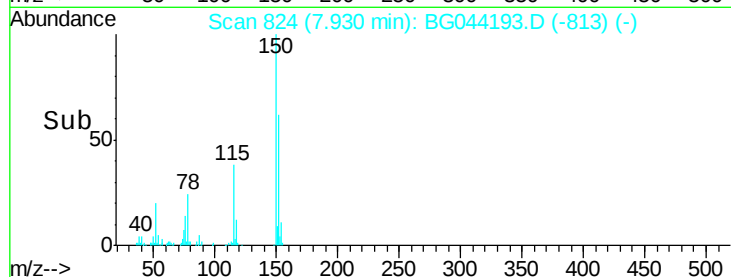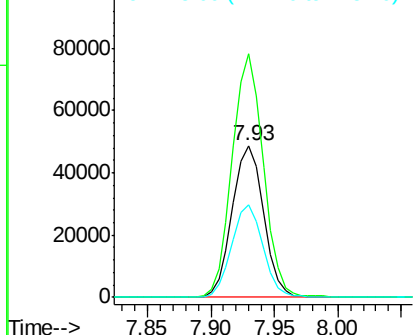



#5


2-Fluorophenol
Concen: 58.847 ng
RT: 5.51 min Scan# 412
Delta R.T. -0.03 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21

Tgt Ion:112 Resp: 269337
Ion Ratio Lower Upper
112 100
64 57.7 47.8 71.6
63 29.3 24.3 36.5

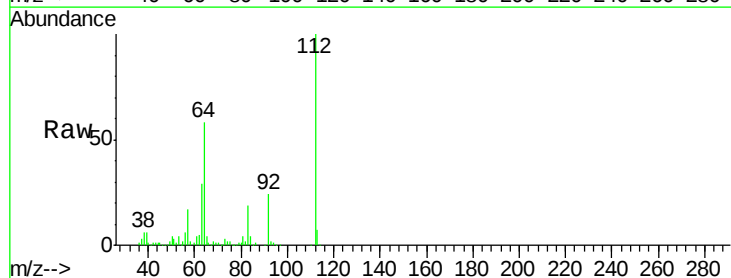

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

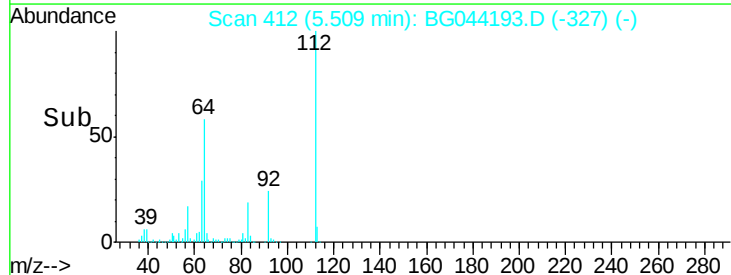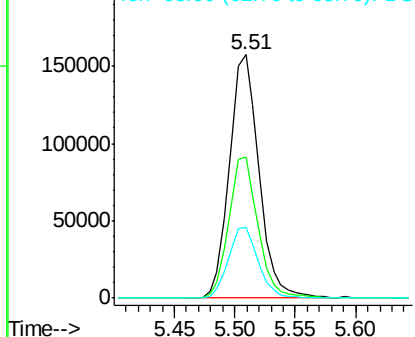

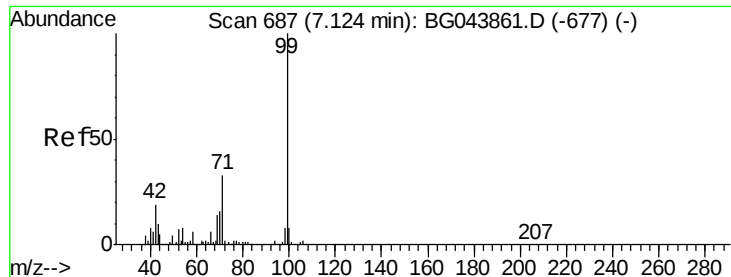

#7

Phenol-d6

Concen: 34.169 ng

RT: 7.10 min Scan# 682

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21

Instrument :

BNA_G

ClientSampleId :

20200047-FIELD-BLANK


Tot Ion: 99 Resp: 218598

Ion Ratio Lower Upper




99 100

42 17.3 14.9 22.3

71 31.3 26.4 39.6

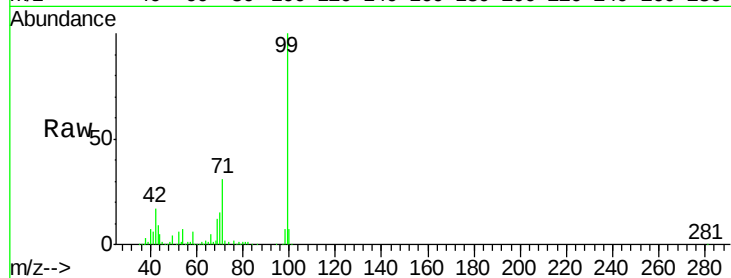

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

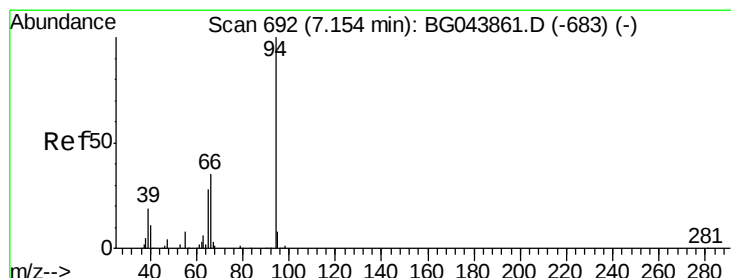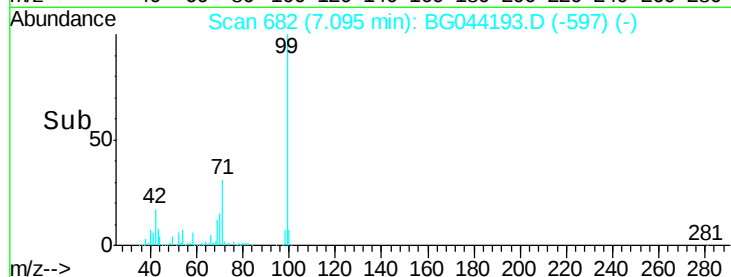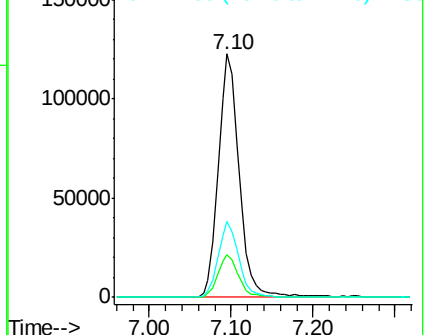

#10

Phenol

Concen: 2.236 ng

RT: 7.12 min Scan# 686

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21


Tgt Ion: 94 Resp: 14740

Ion Ratio Lower Upper



94 100

65 28.5 8.1 48.1

66 43.1 15.6 55.6

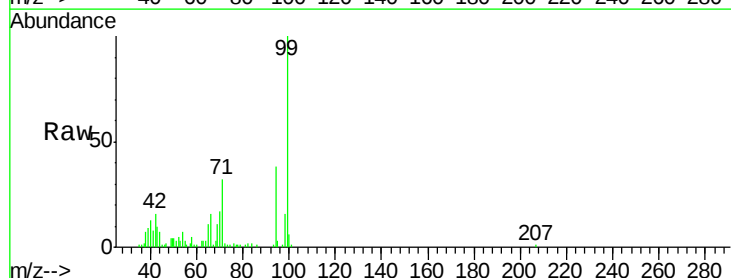

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC


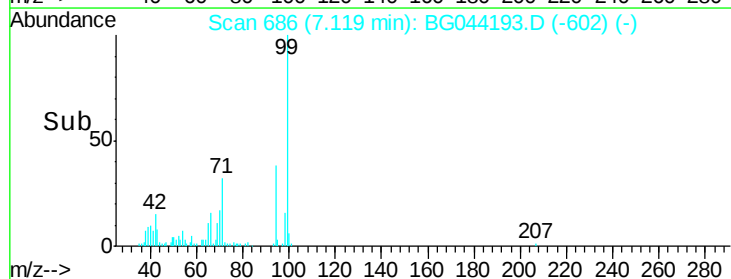
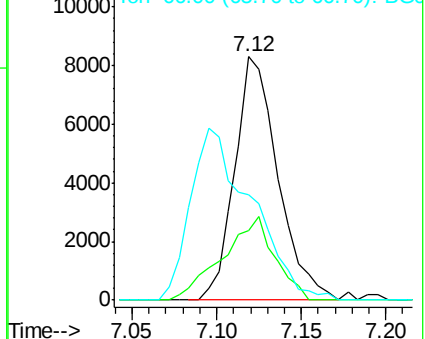




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.73 min Scan# 1301
Delta R.T. -0.03 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21




Instrument :
BNA_G
ClientSampleId :
20200047-FIELD-BLANK


Tot Ion:136	Resp:	378495
Ion	Ratio	Lower Upper
136	100	
137	11.3	8.8 13.2
54	7.6	7.0 10.4
68	6.0	4.9 7.3

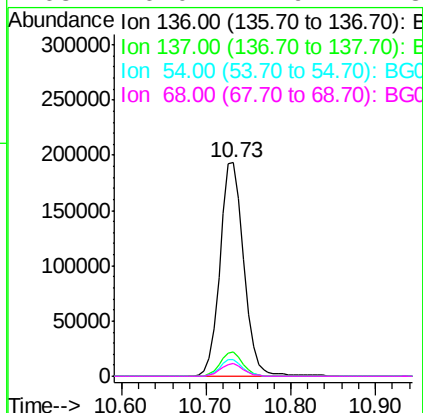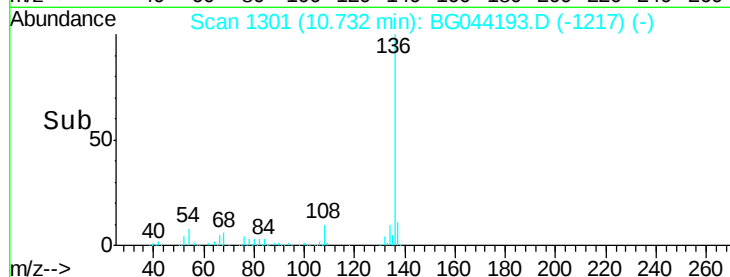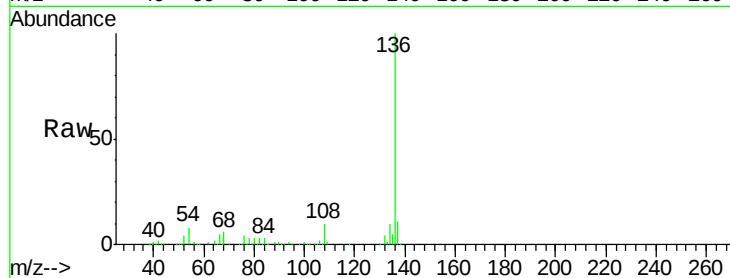

#23
Nitrobenzene-d5
Concen: 82.688 ng
RT: 9.08 min Scan# 1020
Delta R.T. -0.04 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21

Tgt Ion: 82	Resp:	585035
Ion	Ratio	Lower Upper
82	100	
128	44.3	35.1 52.7
54	48.2	40.1 60.1

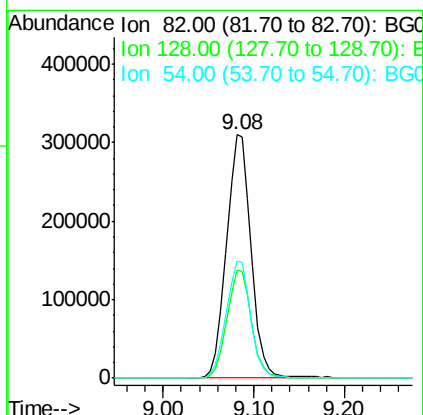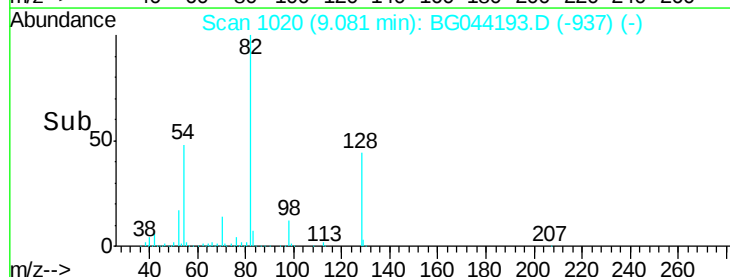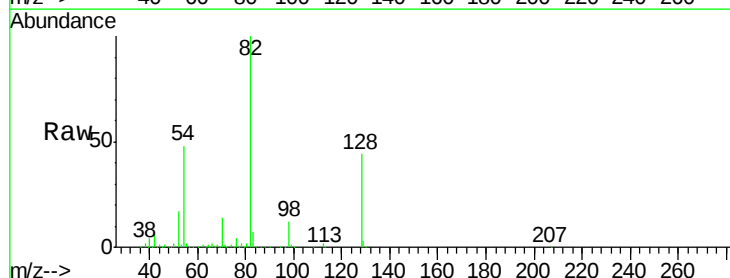

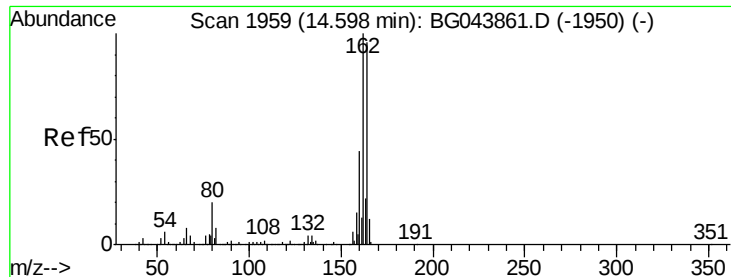

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.56 min Scan# 1953

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21

Instrument :

BNA_G

ClientSampleId :

20200047-FIELD-BLANK


Tot Ion:164 Resp: 257276

Ion Ratio Lower Upper

164 100

162 103.0 83.0 124.4




160 44.7 36.1 54.1

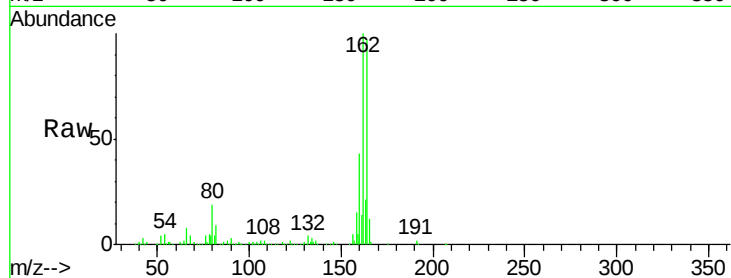

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

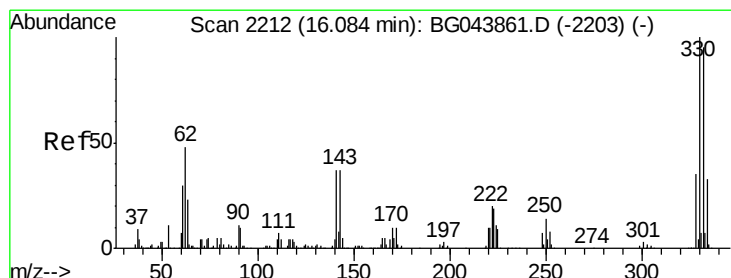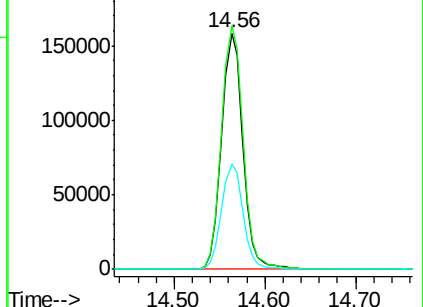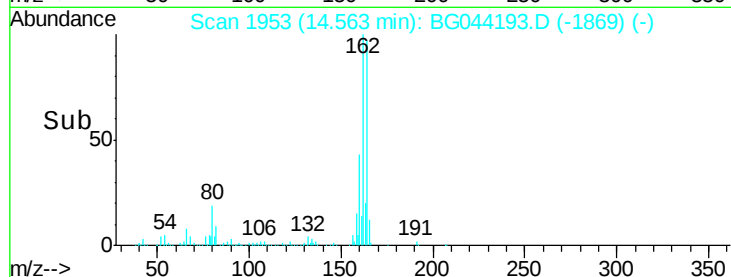

#42

2,4,6-Tribromophenol

Concen: 136.574 ng

RT: 16.05 min Scan# 2206

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21


Tgt Ion:330 Resp: 367705

Ion Ratio Lower Upper

330 100

332 95.6 77.2 115.8



141 39.3 33.1 49.7

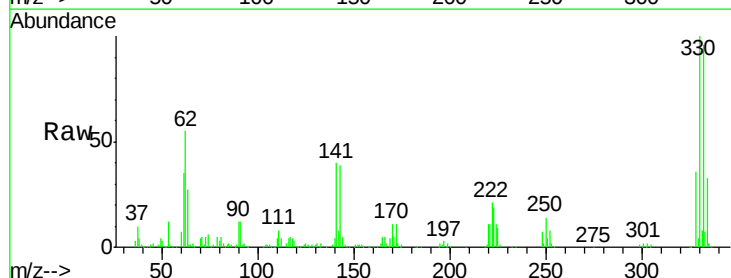

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E


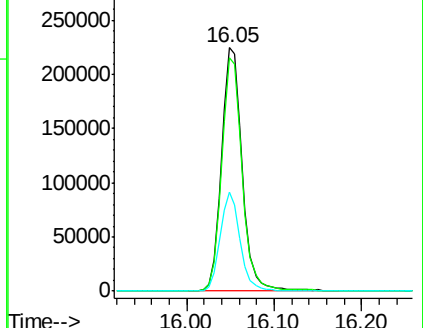
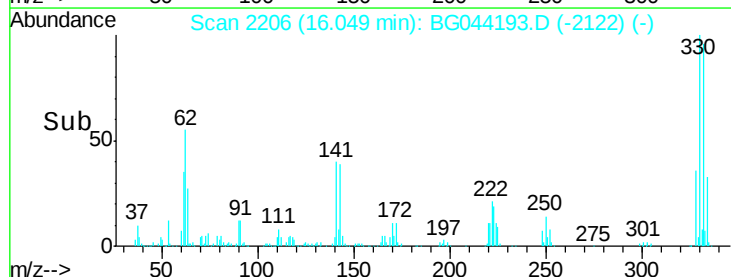




#45
2-Fluorobiphenyl
Concen: 97.301 ng
RT: 13.19 min Scan# 1719
Delta R.T. -0.03 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21




Instrument :
BNA_G
ClientSampleId :
20200047-FIELD-BLANK

Tot Ion:172 Resp: 1381699
Ion Ratio Lower Upper
172 100
171 40.0 35.8 53.8
170 26.9 24.2 36.4

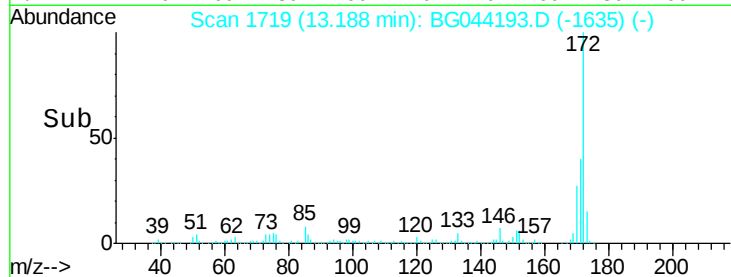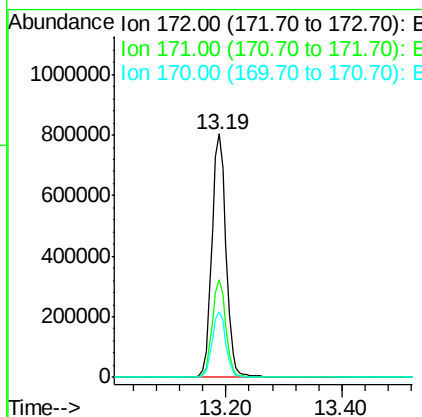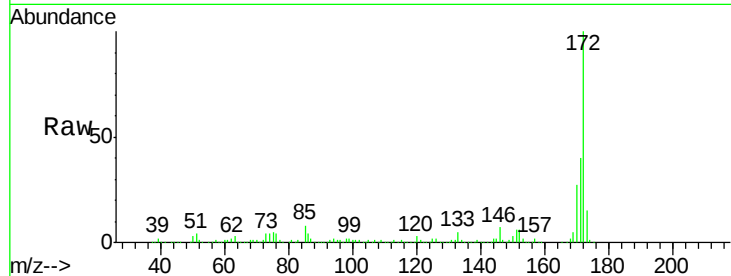

#50
Dimethylphthalate
Concen: 3.137 ng
RT: 14.02 min Scan# 1860
Delta R.T. -0.03 min
Lab File: BG044193.D
Acq: 24 Jan 2020 22:21

Tgt Ion:163 Resp: 57304
Ion Ratio Lower Upper
163 100
194 3.7 3.7 5.5#
164 8.5 9.3 13.9#

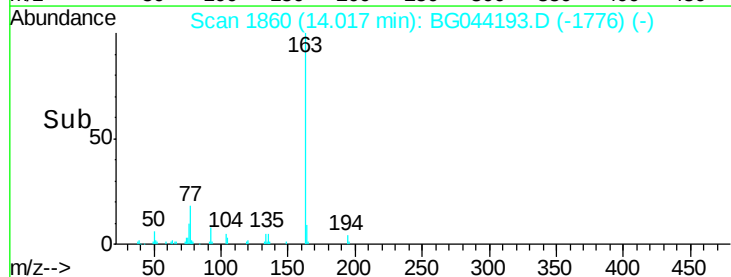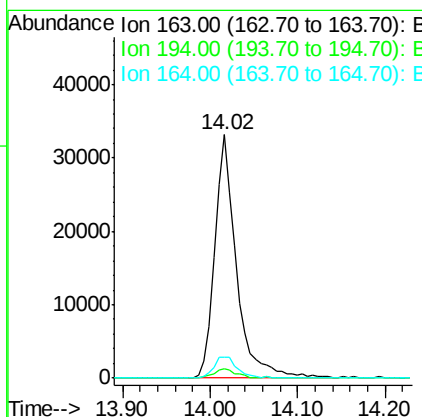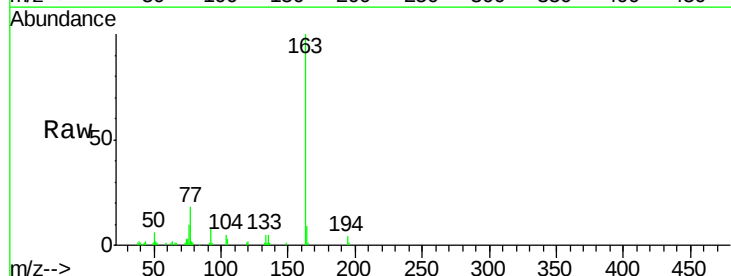



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.31 min Scan# 2420

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21

Instrument :

BNA_G

ClientSampleId :

20200047-FIELD-BLANK


Tot Ion:188 Resp: 520702

Ion Ratio Lower Upper

188 100

94 9.6 7.9 11.9




80 9.8 8.2 12.4

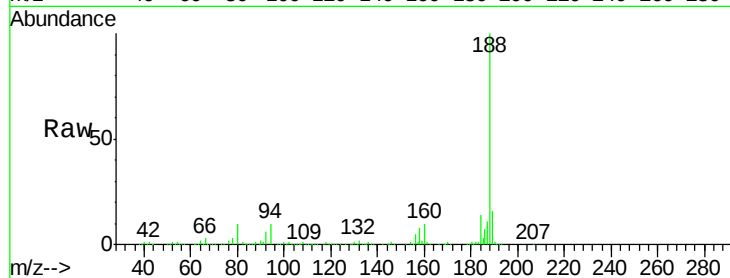

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

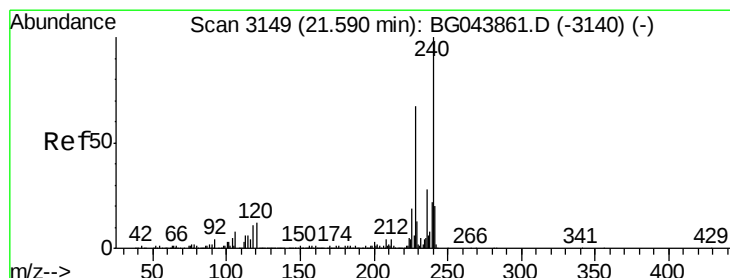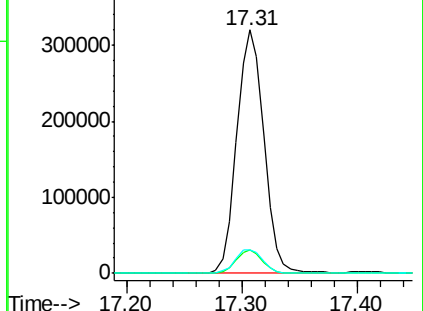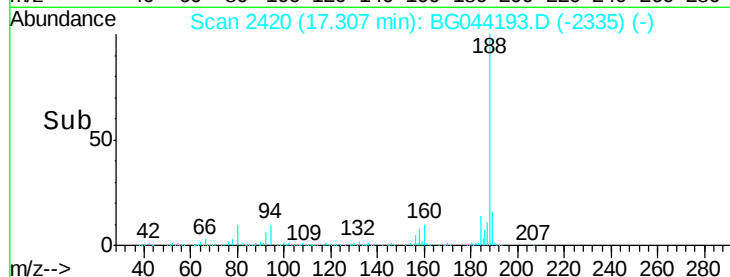

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.55 min Scan# 3143

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21


Tgt Ion:240 Resp: 451651

Ion Ratio Lower Upper

240 100

120 10.9 9.6 14.4



236 27.2 22.2 33.2

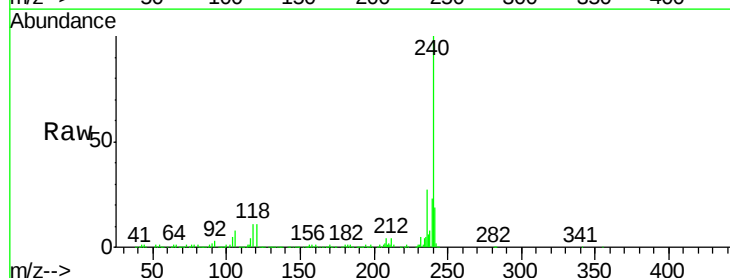


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

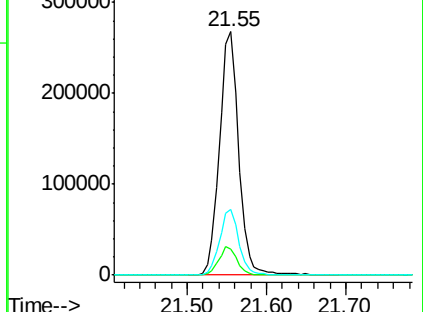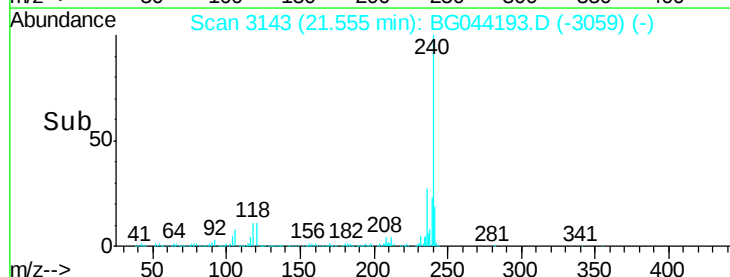

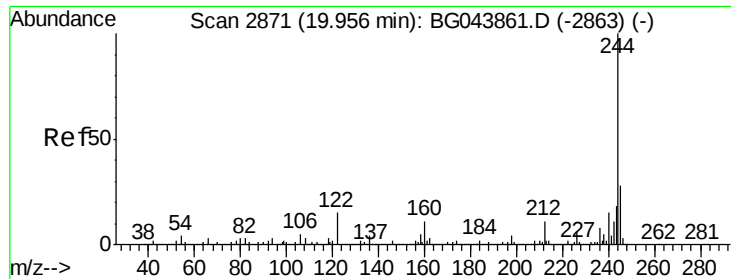

#79

Terphenyl-d14

Concen: 115.006 ng

RT: 19.92 min Scan# 2865

Delta R.T. -0.03 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21

Instrument :

BNA_G

ClientSampleId :

20200047-FIELD-BLANK


Tot Ion:244 Resp: 1972899

Ion Ratio Lower Upper

244 100

212 9.7 8.6 13.0




122 13.3 11.9 17.9

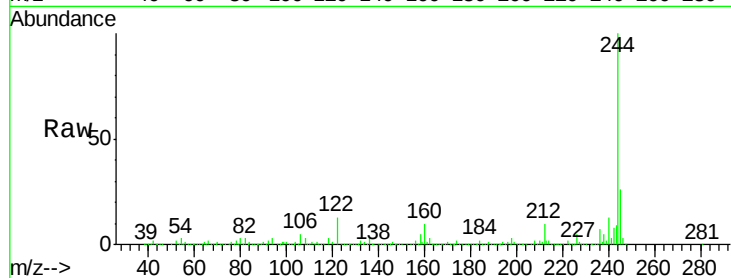

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

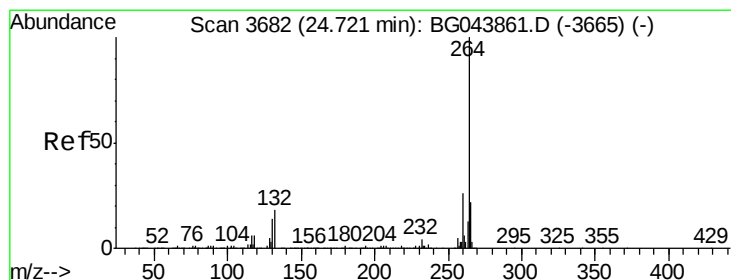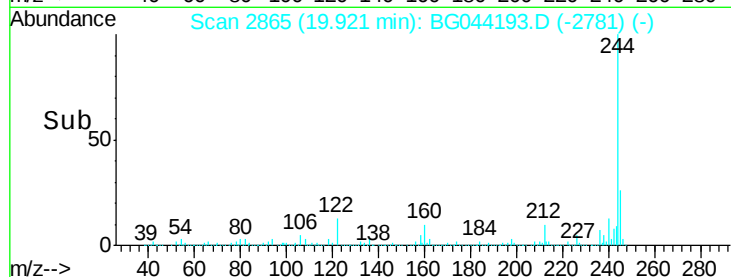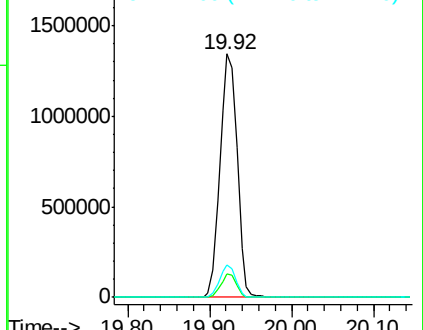

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.66 min Scan# 3671

Delta R.T. -0.06 min

Lab File: BG044193.D

Acq: 24 Jan 2020 22:21


Tgt Ion:264 Resp: 503236

Ion Ratio Lower Upper

264 100

260 24.1 20.4 30.6

265 20.4 17.4 26.2

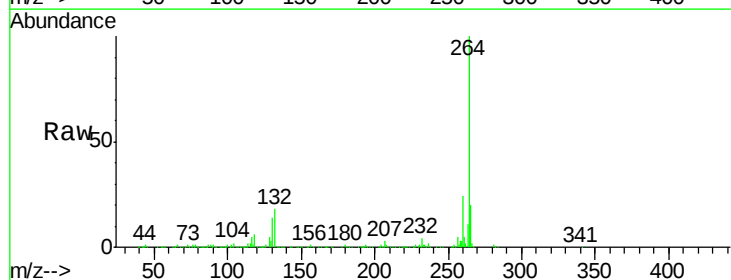

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

