

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
 Data File : BG044204.D
 Acq On : 25 Jan 2020 6:23
 Operator : CG/JU
 Sample : L1242-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20200059-COMP-5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.036	325	331	336	rBV2	12782	22406	1.00%	0.125%
2	5.506	404	411	424	rBV	795758	1352164	60.53%	7.573%
3	7.098	674	682	698	rBV	858167	1576553	70.58%	8.830%
4	7.216	698	702	712	rVB	15766	31671	1.42%	0.177%
5	7.927	817	823	832	rBV	262213	473417	21.19%	2.652%
6	8.256	871	879	888	rBV	536758	981503	43.94%	5.497%
7	9.084	1010	1020	1039	rBV	493884	913080	40.87%	5.114%
8	10.730	1293	1300	1313	rBV	388963	722884	32.36%	4.049%
9	13.185	1711	1718	1740	rBV	1038921	1820057	81.48%	10.194%
10	14.014	1853	1859	1876	rBV	195642	322225	14.42%	1.805%
11	14.566	1946	1953	1971	rBV	649201	1096327	49.08%	6.140%
12	16.053	2199	2206	2224	rBV	1032580	1740641	77.92%	9.749%
13	17.310	2413	2420	2432	rBV	760417	1246773	55.81%	6.983%
14	19.361	2764	2769	2776	rBV	19828	30223	1.35%	0.169%
15	19.719	2823	2830	2838	rVB	21601	42389	1.90%	0.237%
16	19.925	2858	2865	2878	rBV	1614349	2233856	100.00%	12.511%
17	21.229	3083	3087	3092	rBV2	39966	73968	3.31%	0.414%
18	21.552	3135	3142	3157	rBV2	758283	1330502	59.56%	7.452%
19	21.764	3174	3178	3185	rVB2	27412	39299	1.76%	0.220%
20	22.357	3274	3279	3284	rBV2	36277	57708	2.58%	0.323%
21	23.027	3388	3393	3403	rVB	47619	87825	3.93%	0.492%
22	23.209	3420	3424	3431	rVB	22426	39952	1.79%	0.224%
23	23.808	3520	3526	3534	rVB	48464	99986	4.48%	0.560%
24	24.660	3660	3671	3692	rBV2	448731	1424171	63.75%	7.977%
25	25.812	3858	3867	3876	rBV4	32674	94999	4.25%	0.532%


Sum of corrected areas: 17854579

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
Data File : BG044204.D
Acq On : 25 Jan 2020 6:23
Operator : CG/JU
Sample : L1242-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20200059-COMP-5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

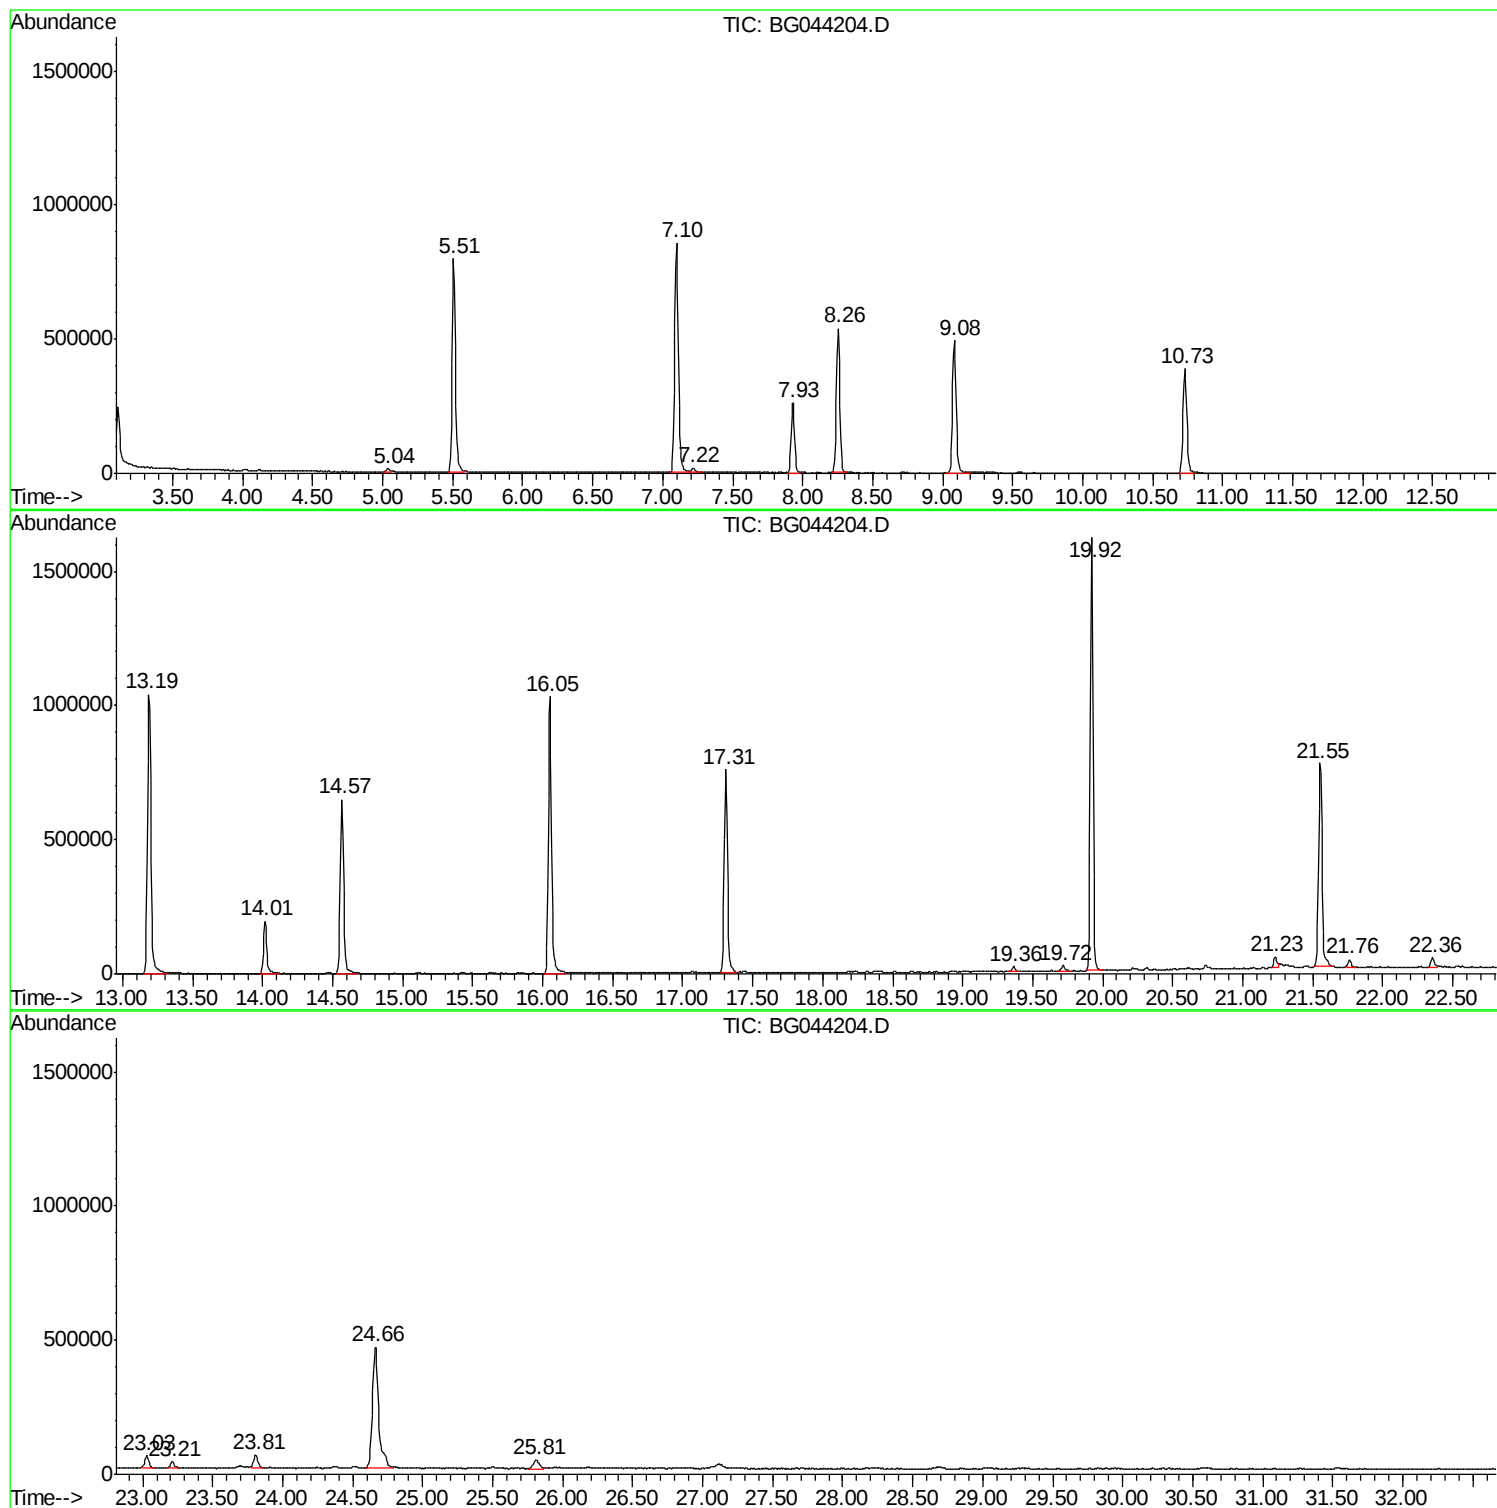

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012420\
Data_File : BG044204.D
Acq_On : 25-Jan-2020 6:233
Operator : CG/JUU
Sample : L1242-055
Misc :
ALS_Vial : 28 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
20200059-COMP-5

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
