

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
 Data File : BG044206.D
 Acq On : 25 Jan 2020 7:41
 Operator : CG/JU
 Sample : L1242-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20200056-COMP-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.509	405	412	425	rBV	1200336	1981044	56.81%	8.576%
2	7.101	674	683	698	rBV	1207893	2286650	65.58%	9.899%
3	7.219	698	703	720	rVB2	18867	44467	1.28%	0.192%
4	7.930	817	824	832	rBV	273471	468397	13.43%	2.028%
5	8.253	871	879	888	rBV	858019	1517772	43.53%	6.571%
6	9.087	1012	1021	1038	rBV	701993	1347980	38.66%	5.835%
7	10.732	1292	1301	1316	rBV	375010	717265	20.57%	3.105%
8	13.188	1711	1719	1736	rBV	1788719	2923800	83.85%	12.657%
9	14.017	1850	1860	1872	rBV	303779	489259	14.03%	2.118%
10	14.563	1944	1953	1970	rBV	665119	1098756	31.51%	4.757%
11	16.049	2199	2206	2222	rBV	1421576	2365131	67.83%	10.239%
12	17.307	2413	2420	2431	rBV	772211	1214666	34.83%	5.258%
13	17.430	2437	2441	2447	rVB5	24850	39452	1.13%	0.171%
14	19.363	2763	2770	2777	rBV	30635	46875	1.34%	0.203%
15	19.722	2822	2831	2836	rBV3	30845	55956	1.60%	0.242%
16	19.921	2859	2865	2877	rBV	2703841	3486926	100.00%	15.095%
17	21.232	3083	3088	3093	rBV3	45527	94534	2.71%	0.409%
18	21.555	3135	3143	3159	rVB	742895	1279105	36.68%	5.537%
19	22.354	3275	3279	3285	rVB2	28077	43466	1.25%	0.188%
20	23.024	3388	3393	3400	rVB3	33781	67543	1.94%	0.292%
21	23.206	3421	3424	3433	rVB5	22006	45004	1.29%	0.195%
22	23.805	3520	3526	3532	rBV2	40012	80882	2.32%	0.350%
23	24.663	3662	3672	3692	rBV2	429900	1335113	38.29%	5.780%
24	25.809	3860	3867	3876	rBV3	25140	69734	2.00%	0.302%


Sum of corrected areas: 23099777

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012420\
Data File : BG044206.D
Acq On : 25 Jan 2020 7:41
Operator : CG/JU
Sample : L1242-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20200056-COMP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

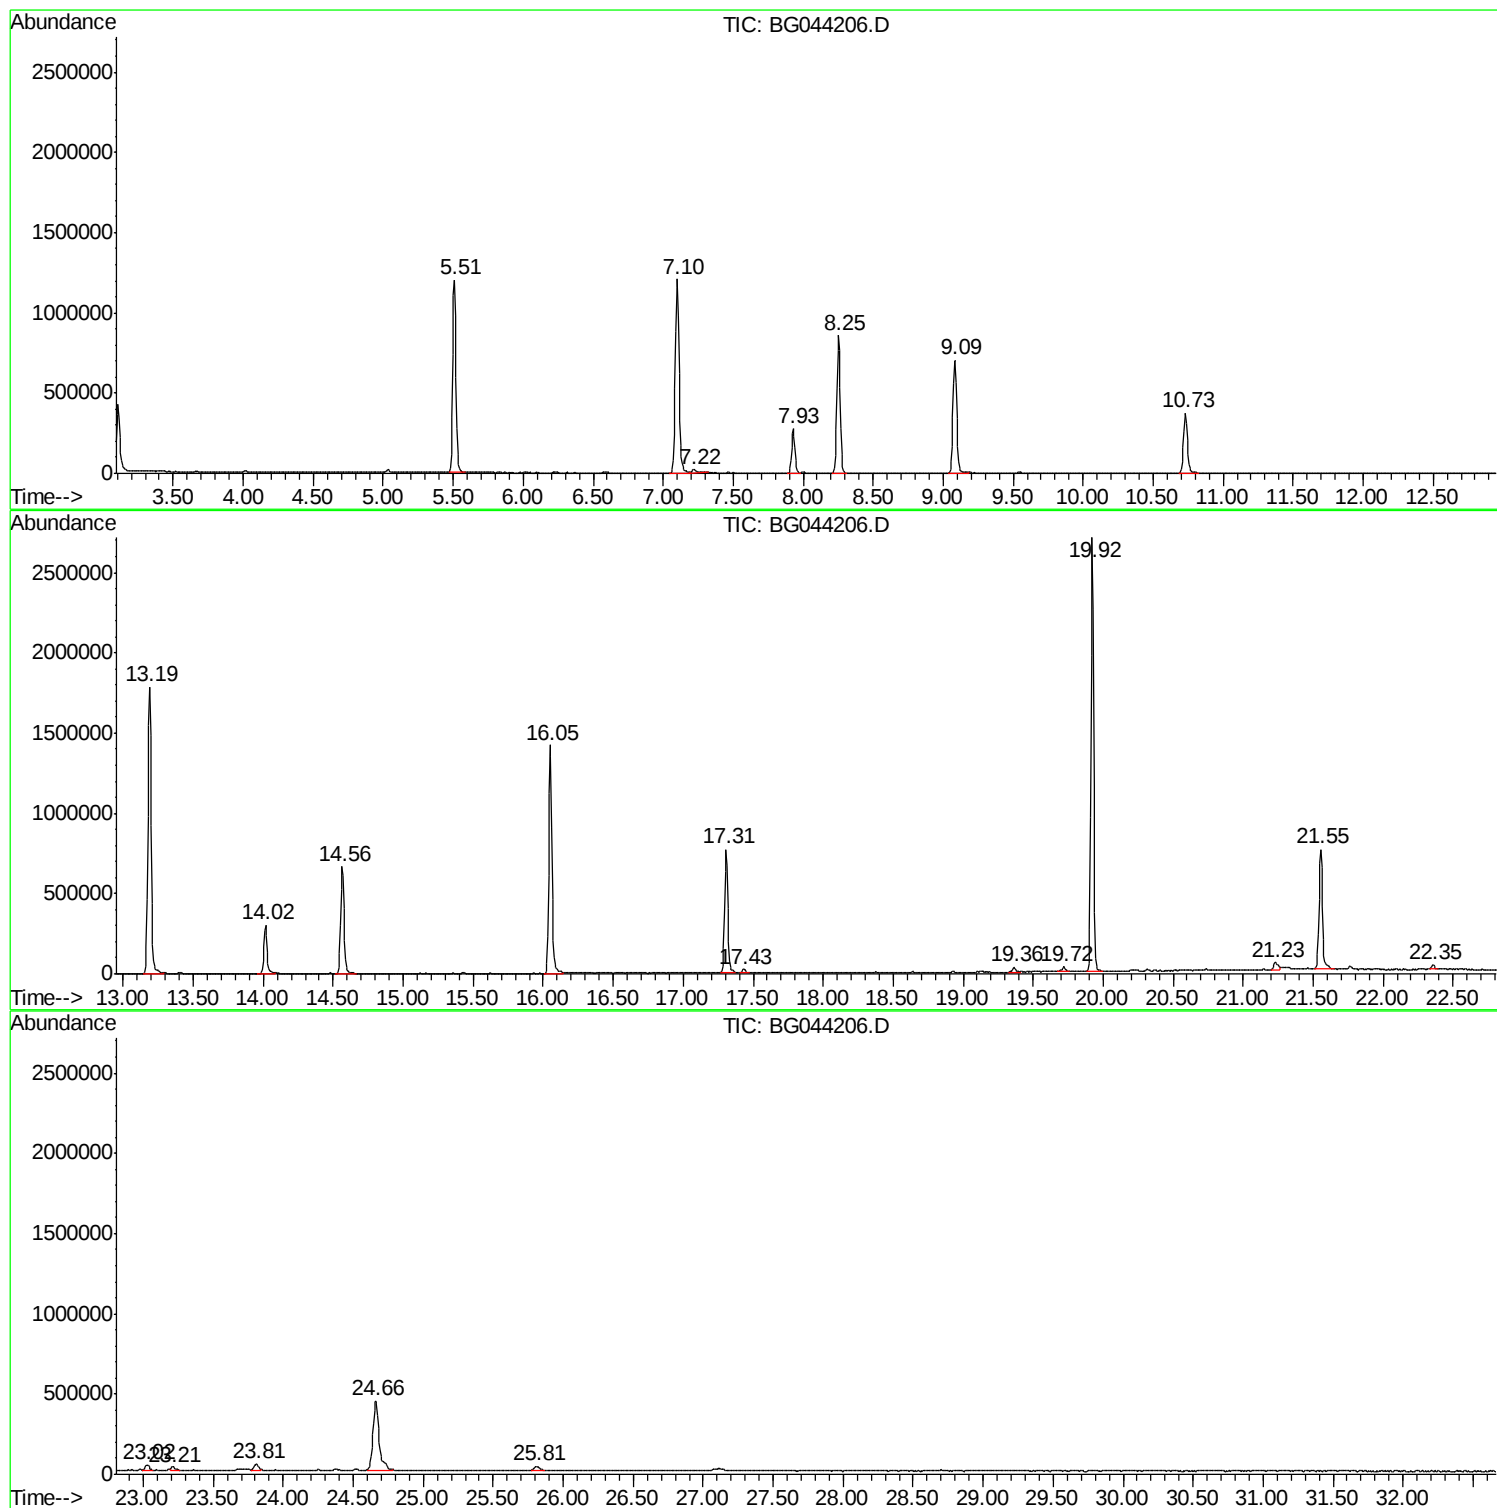

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012420\
Data_File : BG044206.D
Acq_On : 25-Jan-2020 7:411
Operator : CG/JUU
Sample : L1242-022
Misc :
ALS_Vial : 30 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
20200056-COMP-2

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
