


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012420\
 Data File : BG044175.D
 Acq On : 24 Jan 2020 10:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

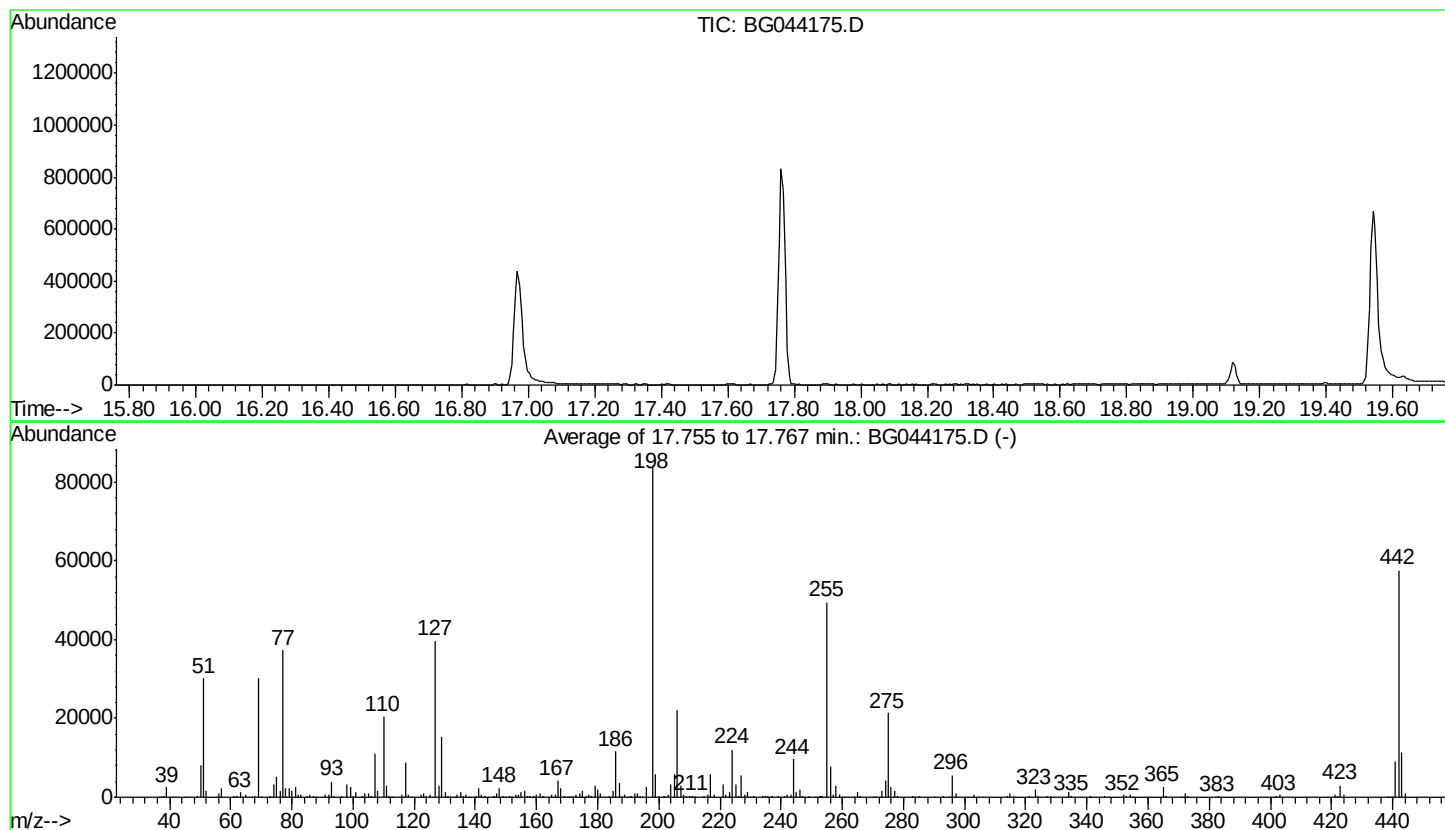

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	30080	PASS
68	69	0.00	2	0.7	208	PASS
69	198	0.00	100	36.0	30333	PASS
70	69	0.00	2	0.5	155	PASS
127	198	10	80	47.1	39642	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84157	PASS
199	198	5	9	6.9	5807	PASS
275	198	10	60	25.4	21363	PASS
365	198	1	100	3.3	2765	PASS
441	198	0.01	100	10.7	8986	PASS
442	198	50	100	68.5	57669	PASS
443	442	15	24	19.9	11489	PASS