


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG012420\
 Data File : BG044194.D
 Acq On : 24 Jan 2020 23:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

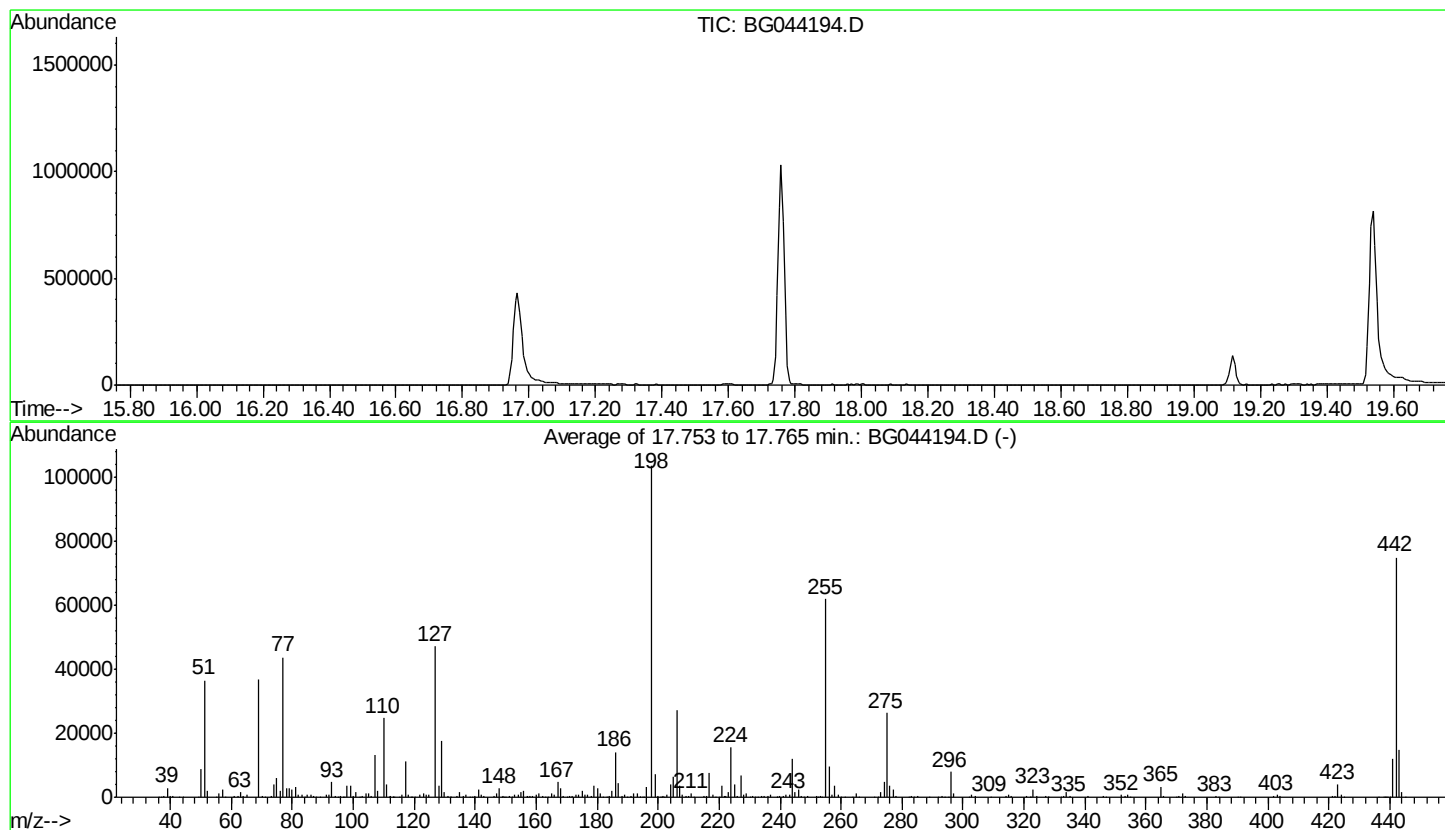

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	36546	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	36661	PASS
70	69	0.00	2	0.8	293	PASS
127	198	10	80	45.5	47138	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103674	PASS
199	198	5	9	7.0	7285	PASS
275	198	10	60	25.3	26269	PASS
365	198	1	100	3.3	3370	PASS
441	198	0.01	100	11.8	12194	PASS
442	198	50	100	72.4	75034	PASS
443	442	15	24	19.8	14846	PASS