

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
 Data File : BG056410.D
 Acq On : 24 Jan 2023 19:51
 Operator : CG/JU
 Sample : 01260-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-27

Quant Time: Jan 25 05:34:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 04:54:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.291	152	33462	20.000	ng	0.00
21) Naphthalene-d8	11.123	136	132505	20.000	ng	0.00
39) Acenaphthene-d10	14.907	164	105746	20.000	ng	0.00
64) Phenanthrene-d10	17.645	188	257731	20.000	ng	0.00
76) Chrysene-d12	21.934	240	254348	20.000	ng	# 0.00
86) Perylene-d12	25.353	264	276515	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.811	112	205704	109.761	ng	0.00
7) Phenol-d6	7.433	99	287234	99.800	ng	0.00
23) Nitrobenzene-d5	9.466	82	150212	57.987	ng	0.00
42) 2,4,6-Tribromophenol	16.387	330	145812	108.875	ng	0.00
45) 2-Fluorobiphenyl	13.532	172	514099	67.134	ng	0.00
79) Terphenyl-d14	20.218	244	985591	69.403	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	9.466	70	18473	10.555	ng	# 67
51) 2,6-Dinitrotoluene	14.907	165	14415	7.925	ng	# 31
57) 2,4-Dinitrotoluene	14.907	165	14415	5.667	ng	# 28
67) 4-Bromophenyl-phenylether	16.387	248	11516	3.509	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056410.D
Acq On : 24 Jan 2023 19:51
Operator : CG/JU
Sample : 01260-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-27

Quant Time: Jan 25 05:34:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration




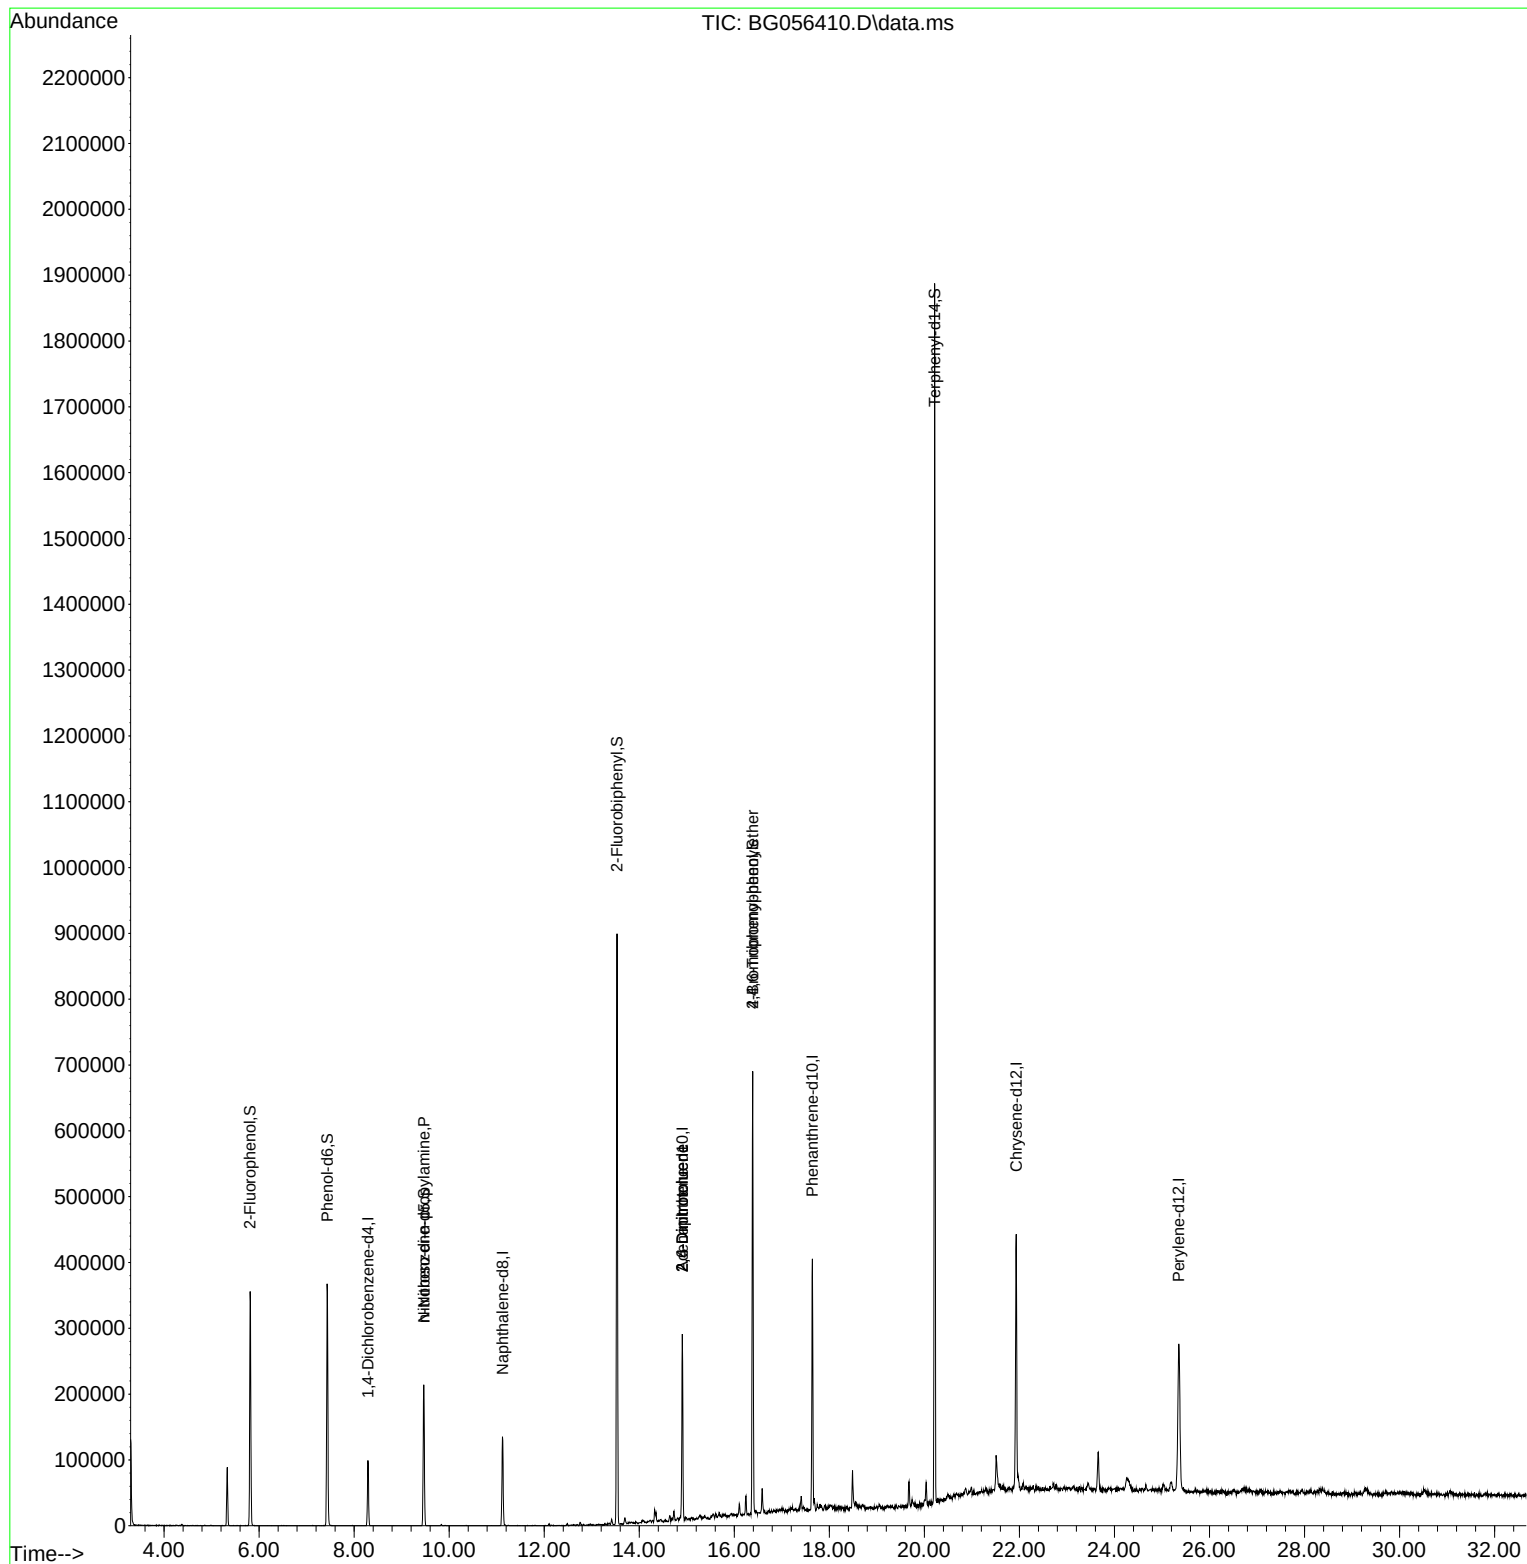




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.291 min Scan# 81
Delta R.T. -0.002 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion:152 Resp: 33462
Ion Ratio Lower Upper
152 100
150 155.5 127.9 191.9
115 55.1 44.2 66.2

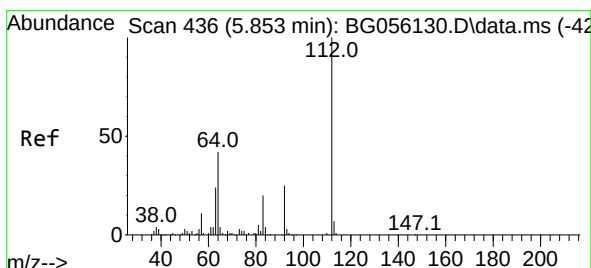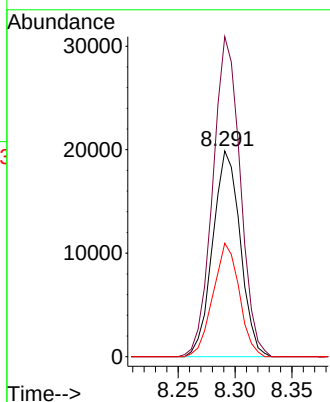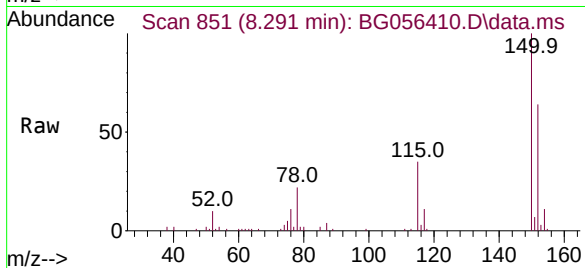

#5
2-Fluorophenol
Concen: 109.761 ng
RT: 5.811 min Scan# 429
Delta R.T. -0.002 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion:112 Resp: 205704
Ion Ratio Lower Upper
112 100
64 39.0 33.3 49.9
63 22.8 19.0 28.4


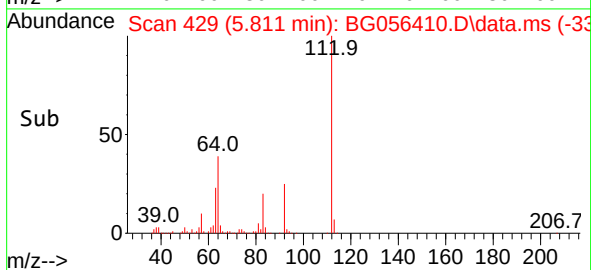
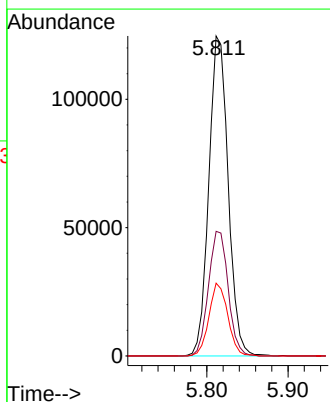
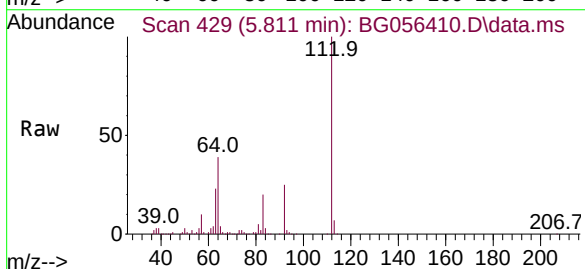




#7
Phenol-d6
Concen: 99.800 ng
RT: 7.433 min Scan# 70
Delta R.T. -0.002 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion: 99 Resp: 287234
Ion Ratio Lower Upper
99 100
42 8.2 5.9 8.9
71 29.0 25.4 38.2

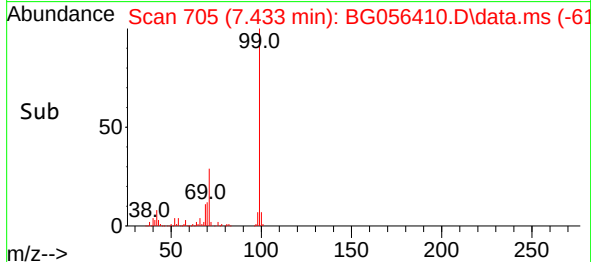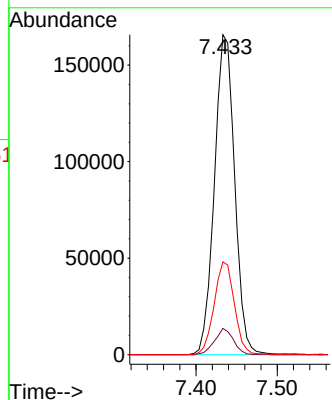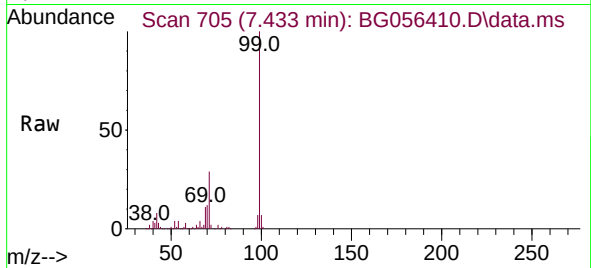

#19
n-Nitroso-di-n-propylamine
Concen: 10.555 ng
RT: 9.466 min Scan# 1051
Delta R.T. 0.368 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion: 70 Resp: 18473
Ion Ratio Lower Upper
70 100
42 34.8 18.2 27.2#
101 0.0 8.3 12.5#
130 1.7 18.2 27.4#


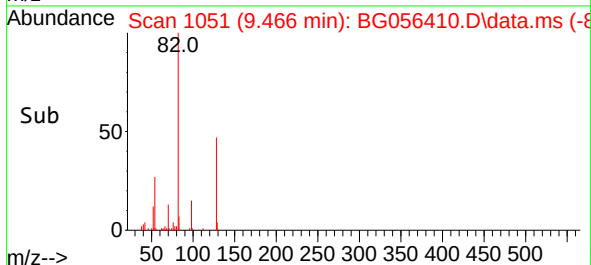
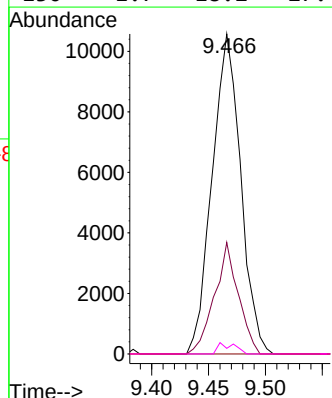
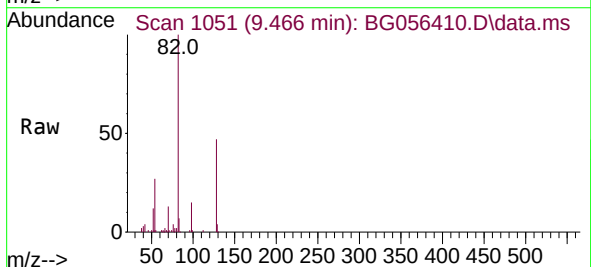




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.123 min Scan# 11
Delta R.T. -0.008 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion:	136	Resp:	132505
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.4	14.0
54	3.0	2.2	3.2
68	4.1	3.4	5.0

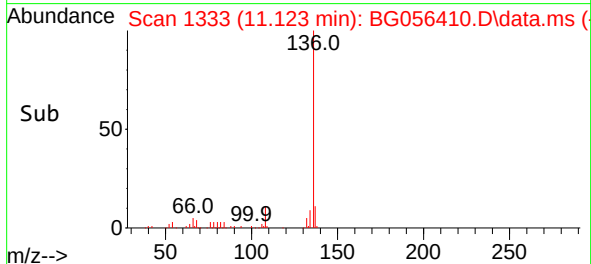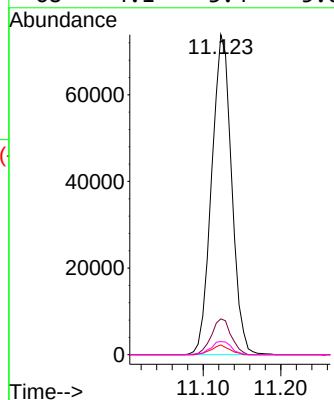

#23
Nitrobenzene-d5
Concen: 57.987 ng
RT: 9.466 min Scan# 1051
Delta R.T. -0.008 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion:	82	Resp:	150212
Ion	Ratio	Lower	Upper
82	100		
128	46.9	33.4	50.2
54	27.4	20.3	30.5

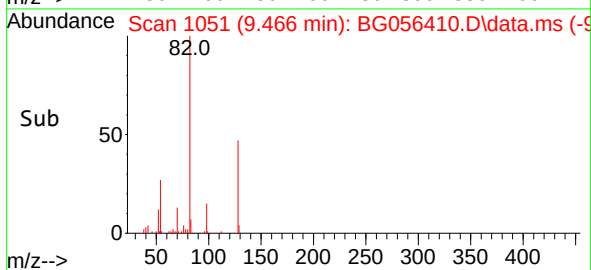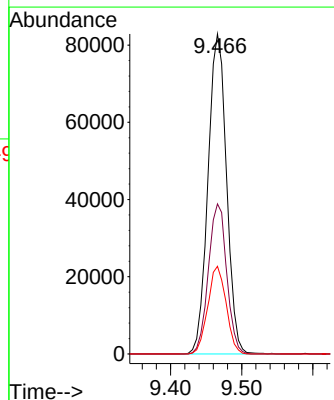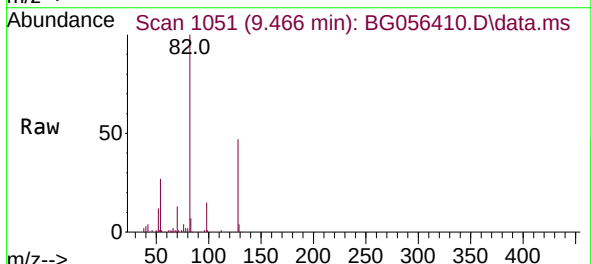

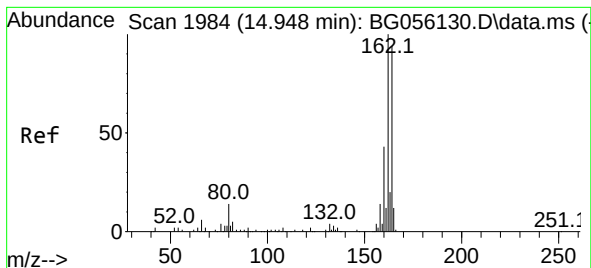

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.907 min Scan# 1984

Delta R.T. -0.008 min

Lab File: BG056410.D

Acq: 24 Jan 2023 19:51

Instrument :

BNA_G

ClientSampleId :

TP-27





Tgt Ion:164 Resp: 105746

Ion Ratio Lower Upper

164 100

162 97.3 84.7 127.1

160 41.4 36.3 54.5

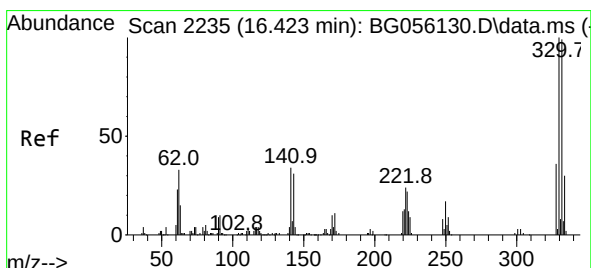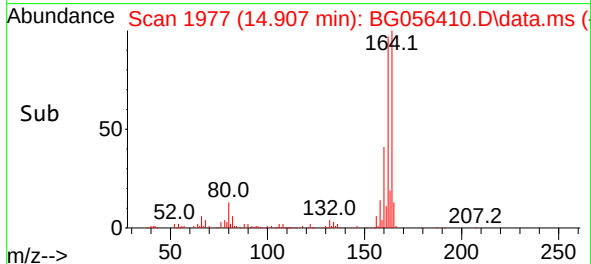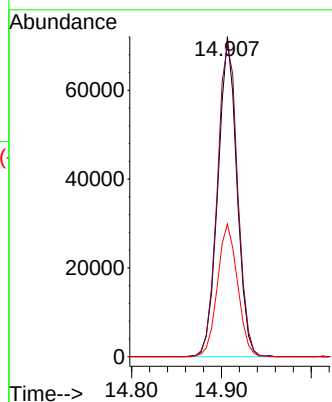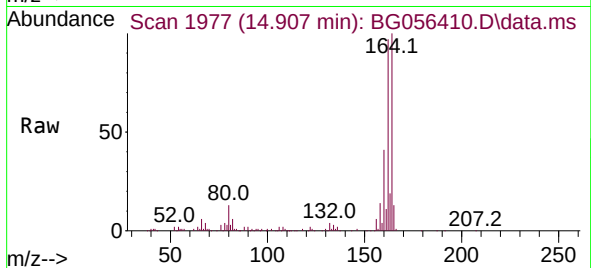

#42

2,4,6-Tribromophenol

Concen: 108.875 ng

RT: 16.387 min Scan# 2229

Delta R.T. -0.008 min

Lab File: BG056410.D

Acq: 24 Jan 2023 19:51




Tgt Ion:330 Resp: 145812


Ion Ratio Lower Upper

330 100

332 97.1 77.3 115.9

141 32.0 27.9 41.9


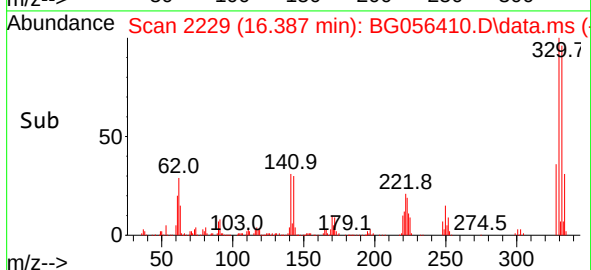
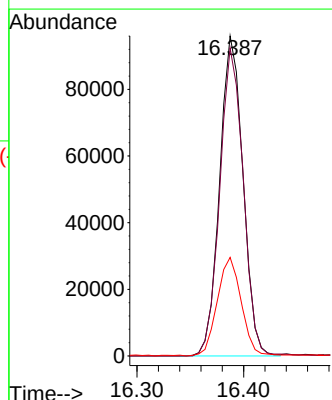





#45
2-Fluorobiphenyl
Concen: 67.134 ng
RT: 13.532 min Scan# 1
Delta R.T. -0.008 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion:172 Resp: 514099
Ion Ratio Lower Upper
172 100
171 36.6 29.6 44.4
170 23.4 19.4 29.2

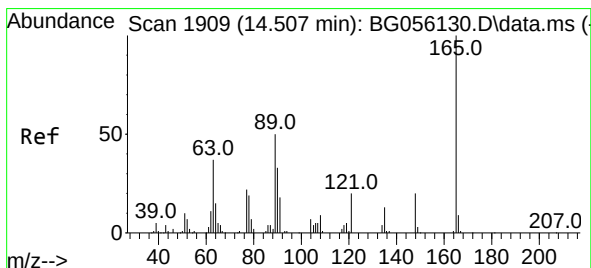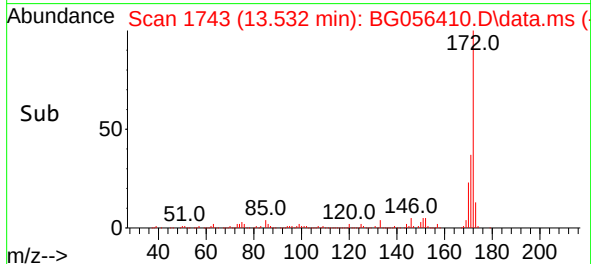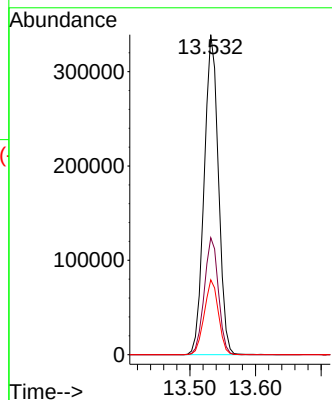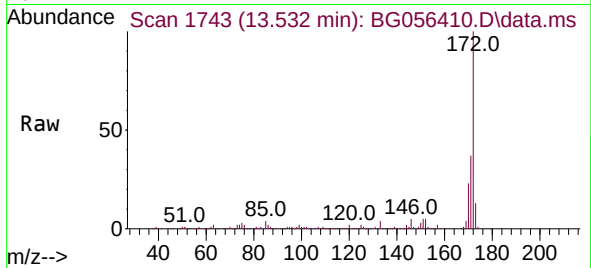

#51
2,6-Dinitrotoluene
Concen: 7.925 ng
RT: 14.907 min Scan# 1977
Delta R.T. 0.427 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion:165 Resp: 14415
Ion Ratio Lower Upper
165 100
63 0.0 32.2 48.2#
89 0.0 39.8 59.8#


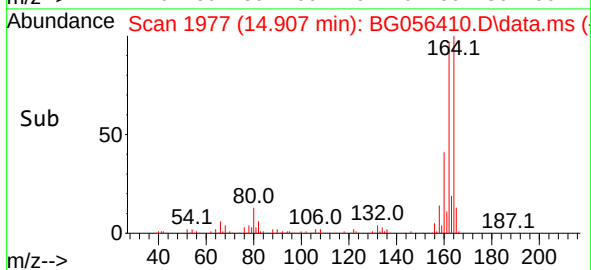
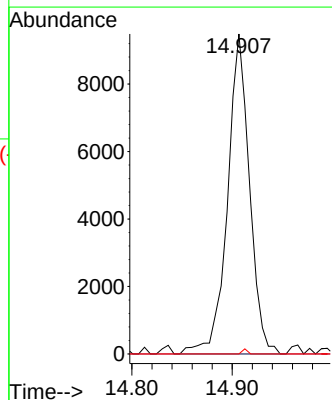
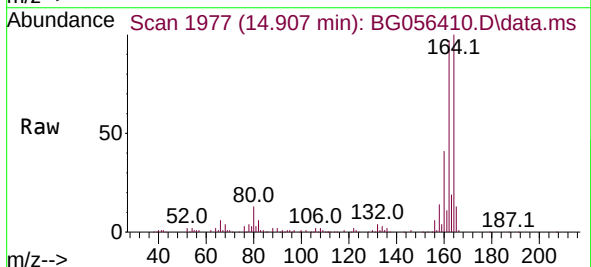


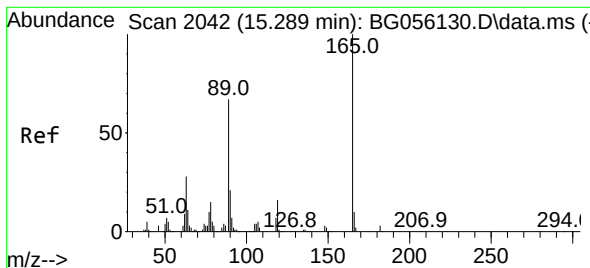

#57
2,4-Dinitrotoluene
Concen: 5.667 ng
RT: 14.907 min Scan# 1977
Delta R.T. -0.361 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion:165 Resp: 14415
Ion Ratio Lower Upper
165 100
63 0.0 22.6 34.0#
89 0.0 53.2 79.8#
182 0.0 2.3 3.5#

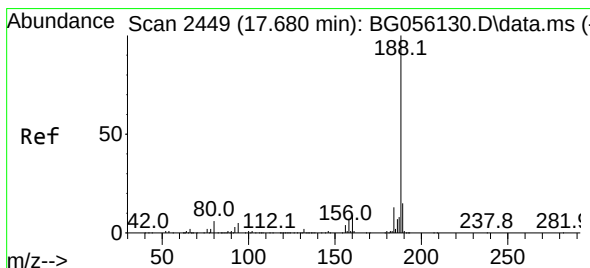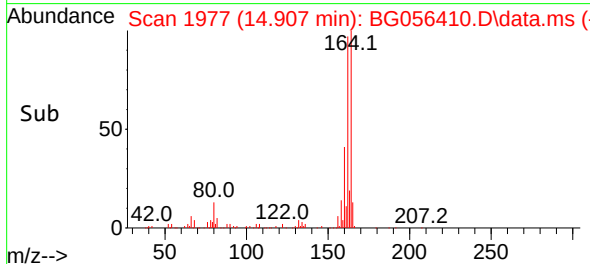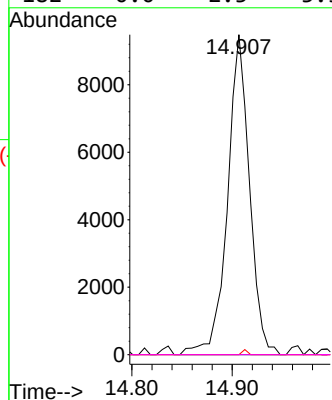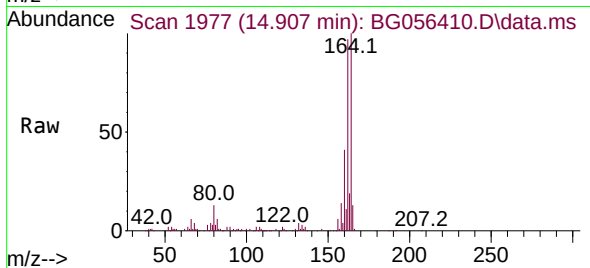

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.645 min Scan# 2443
Delta R.T. -0.008 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion:188 Resp: 257731
Ion Ratio Lower Upper
188 100
94 5.1 4.2 6.2
80 6.0 5.0 7.4


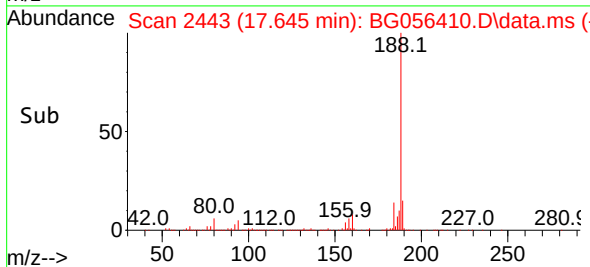
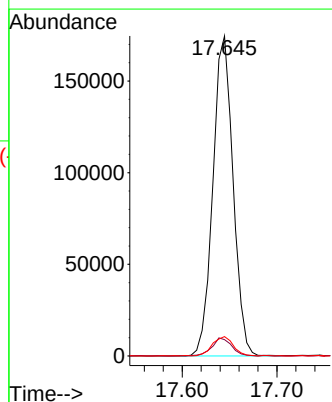
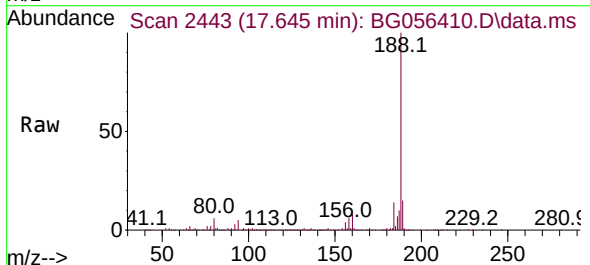




#67
4-Bromophenyl-phenylether
Concen: 3.509 ng
RT: 16.387 min Scan# 21
Delta R.T. -0.443 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51




Instrument :
BNA_G
ClientSampleId :
TP-27


Tgt Ion:248 Resp: 11516
Ion Ratio Lower Upper
248 100
250 210.2 78.2 117.4#
141 421.1 37.6 56.4#

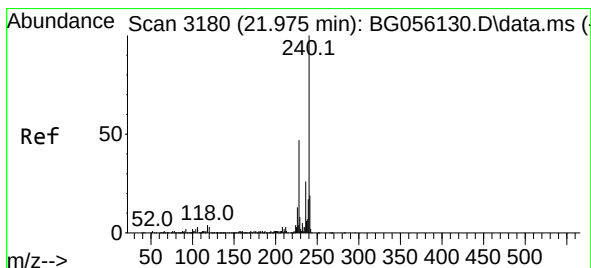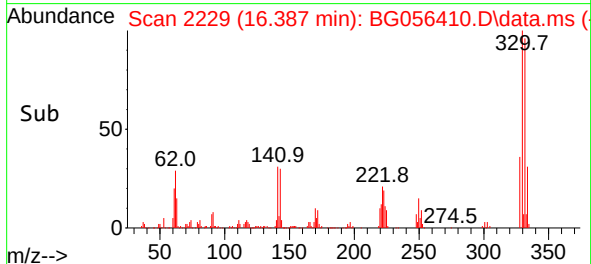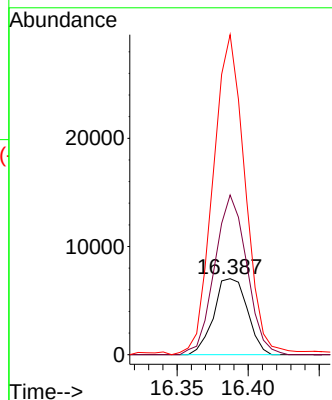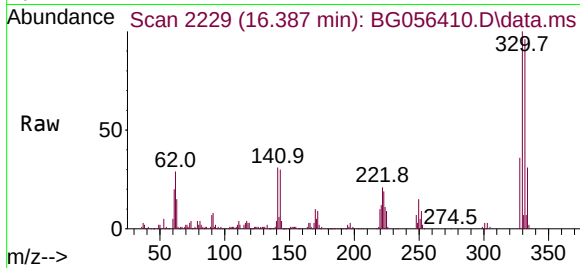

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.934 min Scan# 3173
Delta R.T. -0.008 min
Lab File: BG056410.D
Acq: 24 Jan 2023 19:51

Tgt Ion:240 Resp: 254348
Ion Ratio Lower Upper
240 100
120 4.2 2.6 4.0#
236 24.8 20.8 31.2


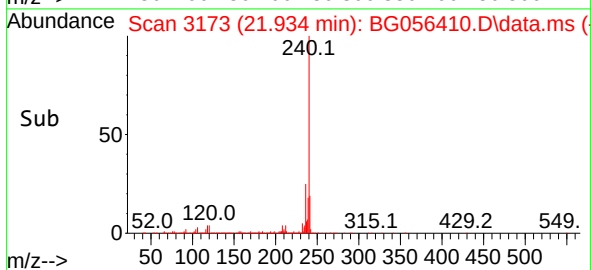
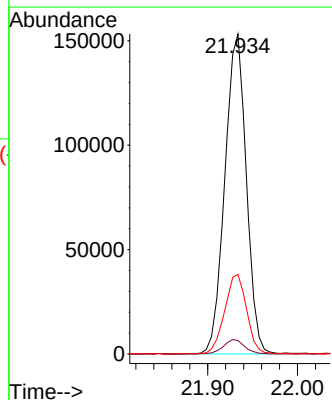
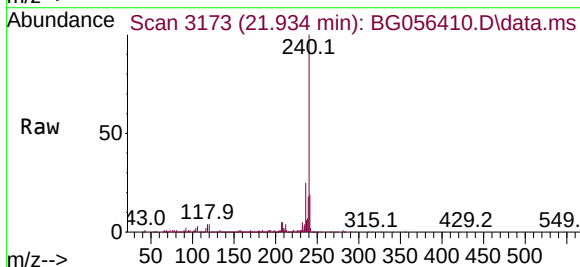




#79
 Terphenyl-d14
 Concen: 69.403 ng
 RT: 20.218 min Scan# 21
 Delta R.T. -0.008 min
 Lab File: BG056410.D
 Acq: 24 Jan 2023 19:51

Instrument :
 BNA_G
 ClientSampleId :
 TP-27

Tgt Ion:244 Resp: 985591
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.7 8.5
 122 5.4 3.5 5.3#

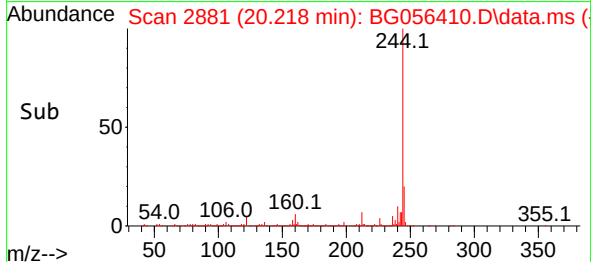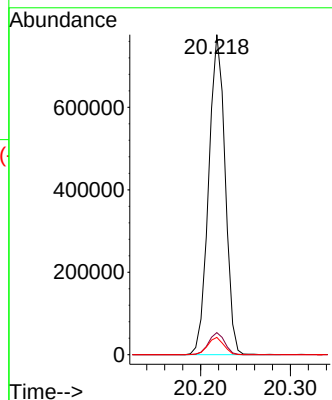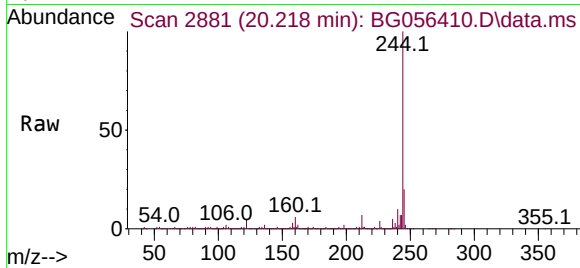

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.353 min Scan# 3755
 Delta R.T. -0.020 min
 Lab File: BG056410.D
 Acq: 24 Jan 2023 19:51

Tgt Ion:264 Resp: 276515
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.6 28.0
 265 23.7 16.7 25.1

