
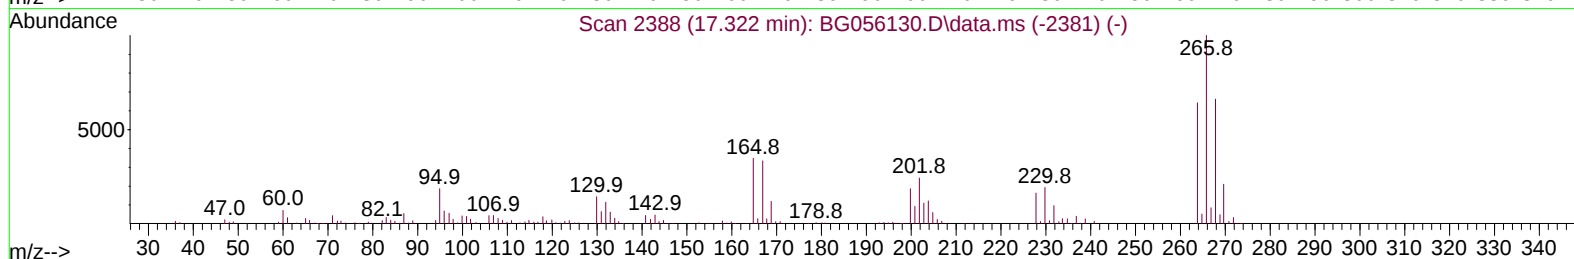
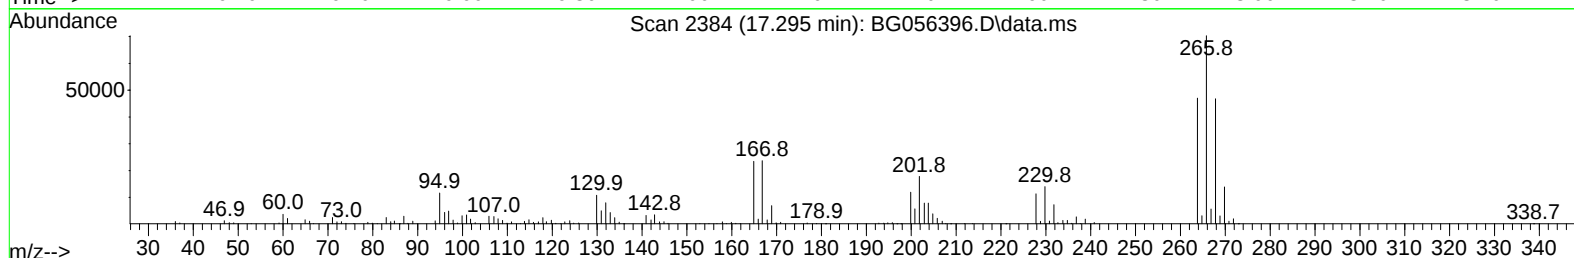


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056396.D
Acq On : 24 Jan 2023 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 08:29:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

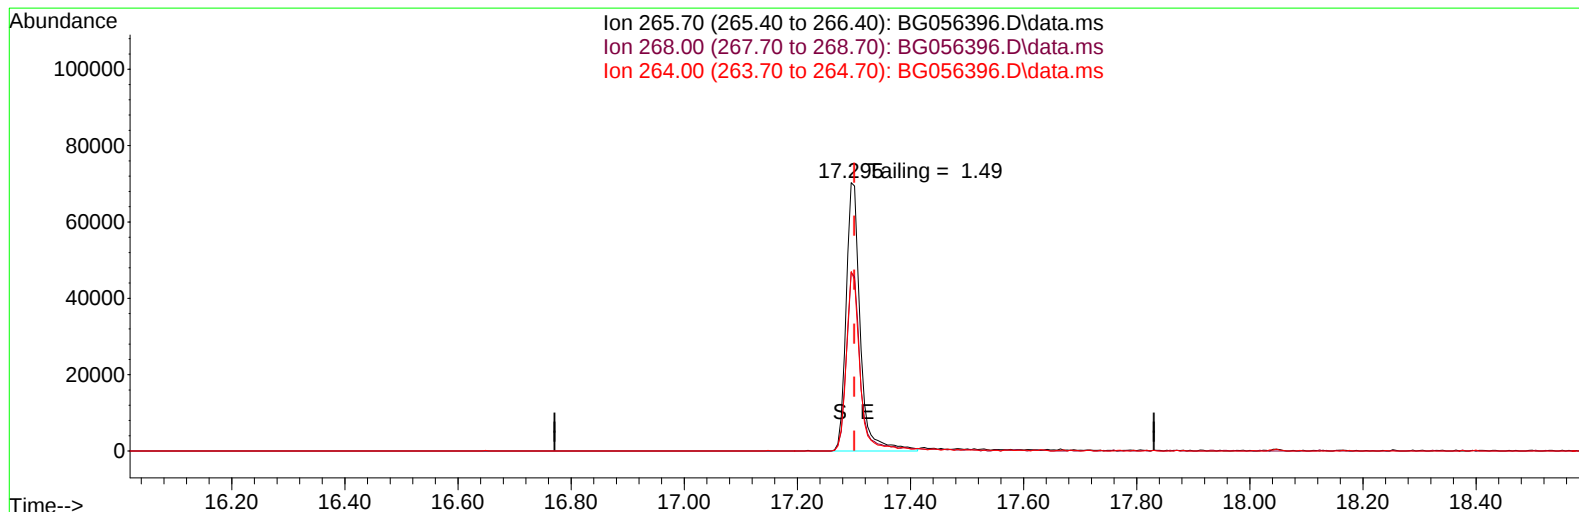

TIC: BG056396.D\data.ms

(70) Pentachlorophenol (C)




17.295min (-0.005) 17798.35 ng

response 122474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.58
264.00	64.30	66.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
 Data File : BG056396.D
 Acq On : 24 Jan 2023 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 08:29:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 04:54:56 2023
 Response via : Initial Calibration

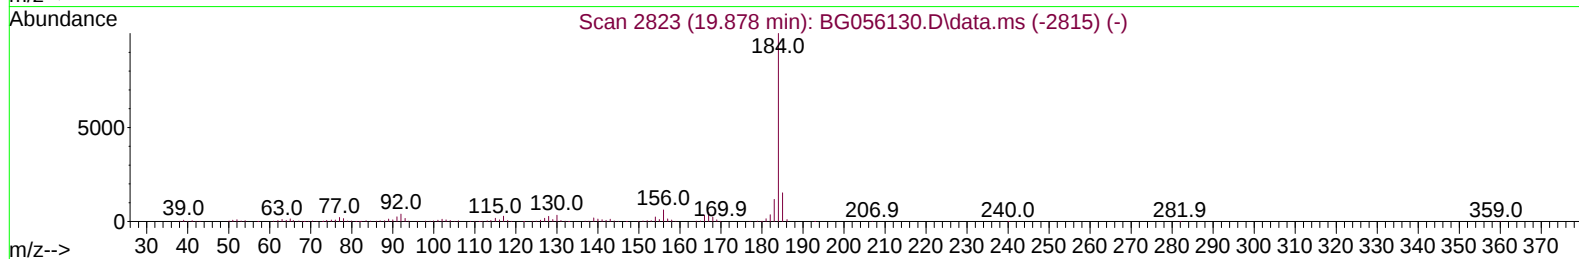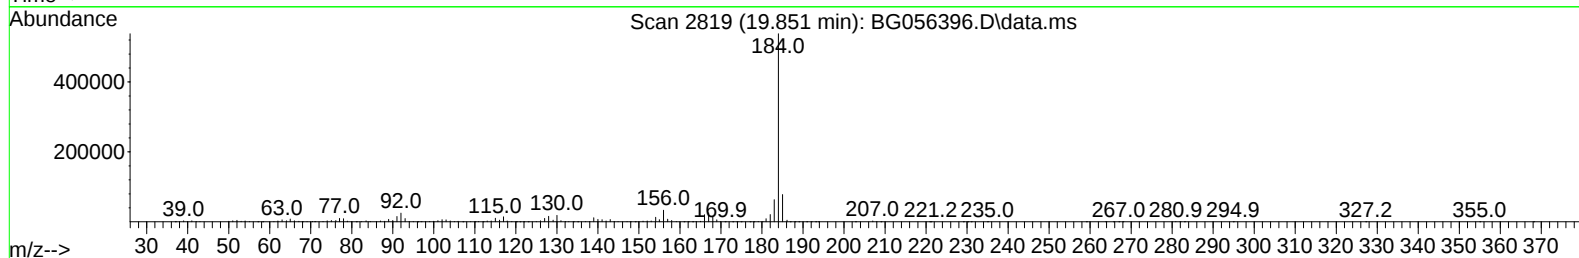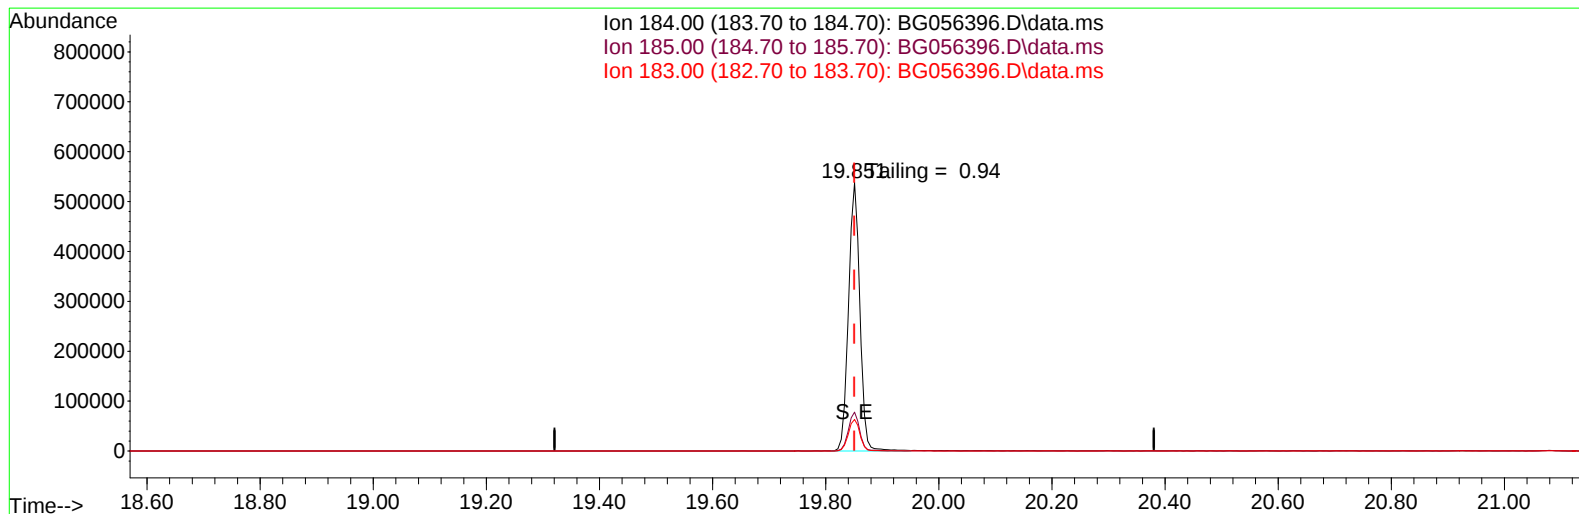

TIC: BG056396.D\data.ms

(77) Benzidine**19.851min (+ 0.001) 274788.40 ng****response 751122**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.49
183.00	11.70	11.75
0.00	0.00	0.00