

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
 Data File : BG056398.D
 Acq On : 24 Jan 2023 11:20
 Operator : CG/JU
 Sample : PB150335BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150335BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.332	342	348	356	rBB	97732	147022	4.56%	1.296%
2	5.814	424	430	440	rBV	410518	661685	20.52%	5.831%
3	7.435	699	706	722	rBV	402495	710345	22.03%	6.260%
4	8.293	845	852	861	rBB	105220	177811	5.52%	1.567%
5	9.468	1045	1052	1063	rBB	242093	432712	13.42%	3.813%
6	11.131	1327	1335	1346	rBB	146560	265604	8.24%	2.341%
7	13.540	1737	1745	1752	rBV	1009205	1587129	49.23%	13.987%
8	14.909	1971	1978	1987	rBB	309888	491159	15.23%	4.329%
9	16.389	2223	2230	2247	rBV	785679	1226192	38.03%	10.806%
10	17.647	2437	2444	2451	rBV	497178	732869	22.73%	6.459%
11	20.220	2876	2882	2888	rBV	2412033	3224077	100.00%	28.414%
12	21.936	3167	3174	3181	rBV	486843	822439	25.51%	7.248%
13	25.367	3744	3758	3769	rVB2	272913	867835	26.92%	7.648%




Sum of corrected areas: 11346879

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056398.D
Acq On : 24 Jan 2023 11:20
Operator : CG/JU
Sample : PB150335BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150335BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

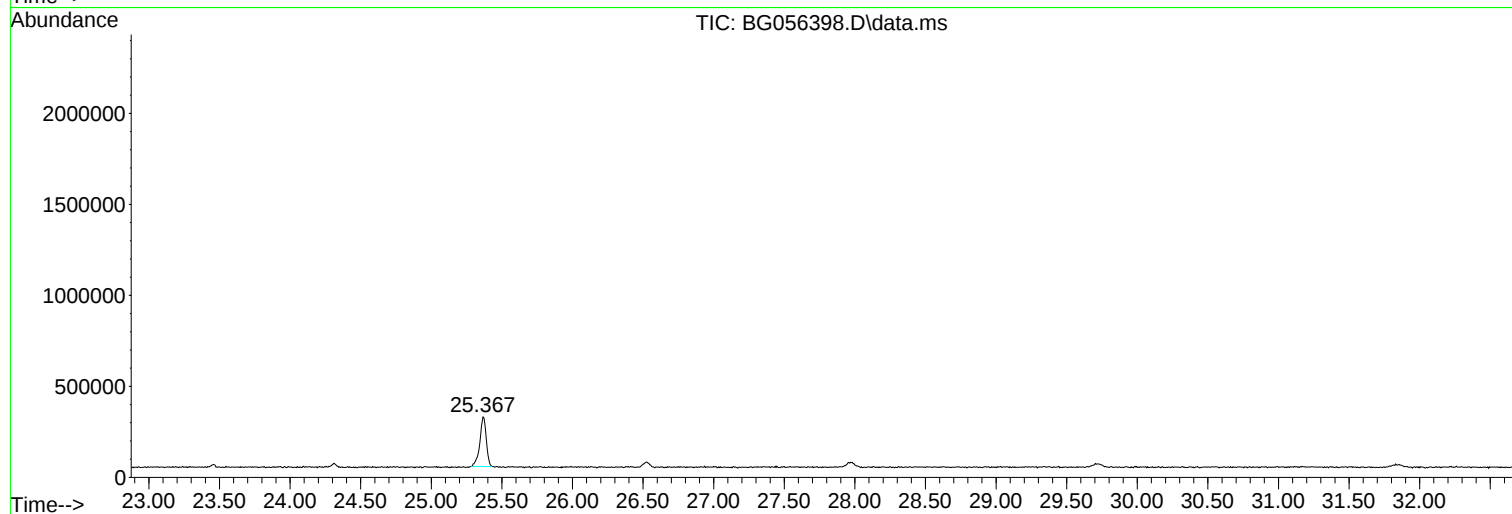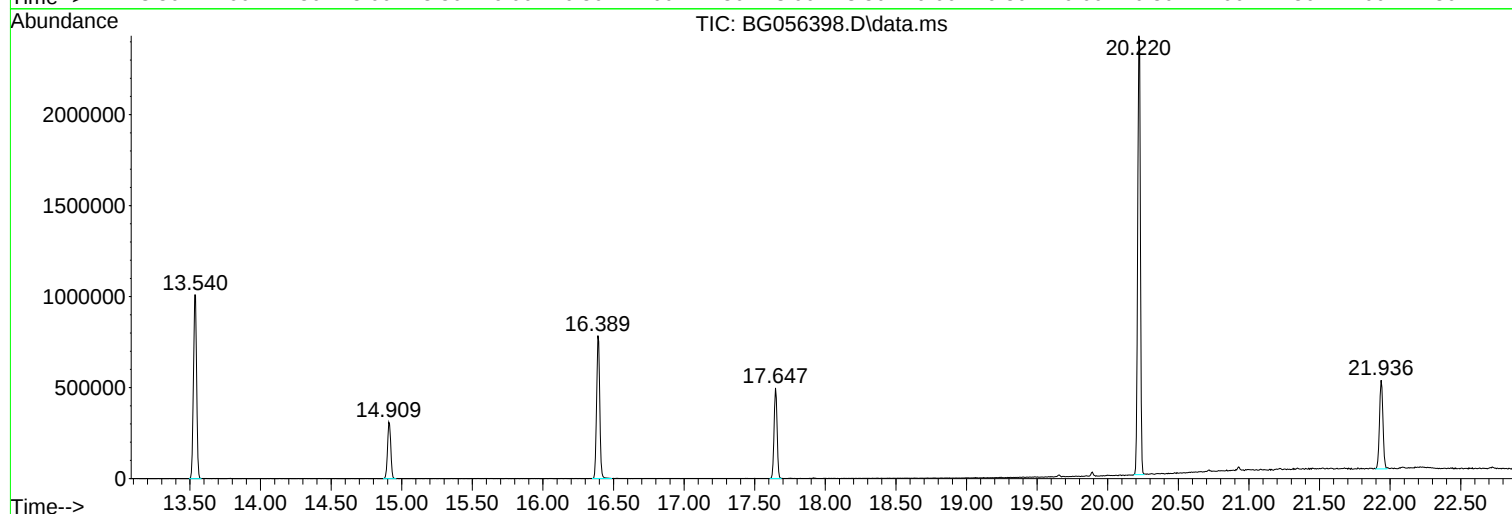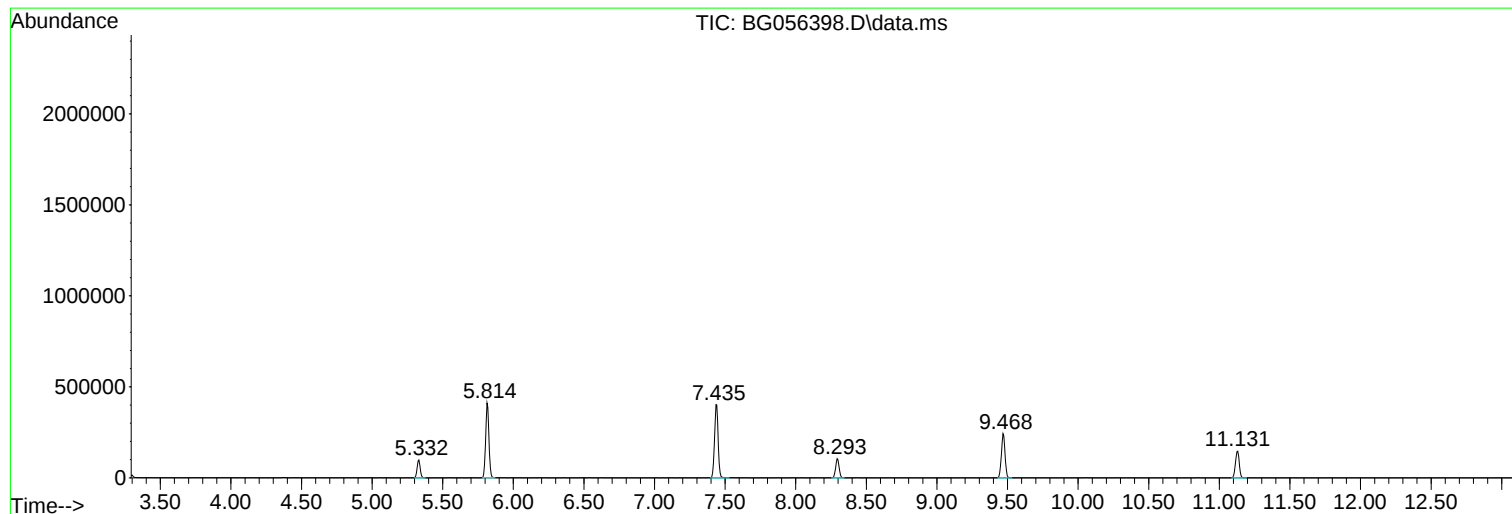

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056398.D
Acq On : 24 Jan 2023 11:20
Operator : CG/JU
Sample : PB150335BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150335BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.332 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.332	16.54 ng	147022	1,4-Dichlorobenzene-d4	8.293

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2		Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	27
3		3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	25
4		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	17
5		Propane, 2-methoxy-	74	C4H10O	000598-53-8	17

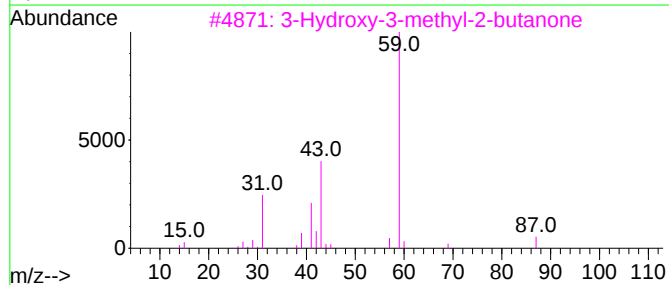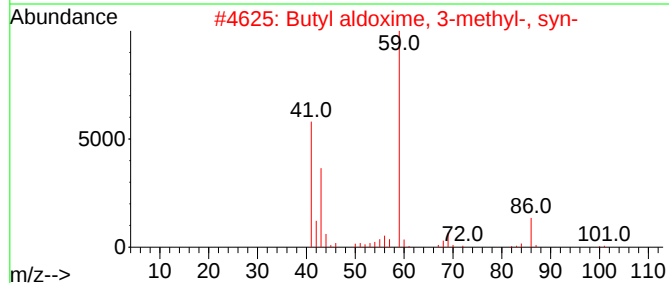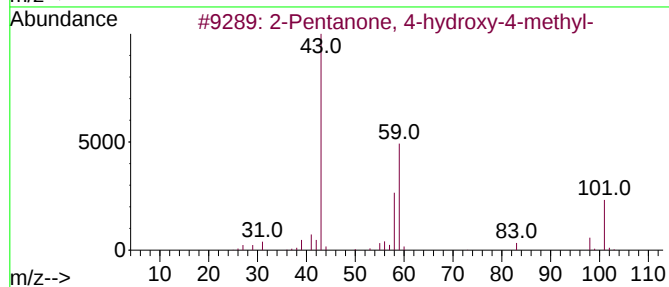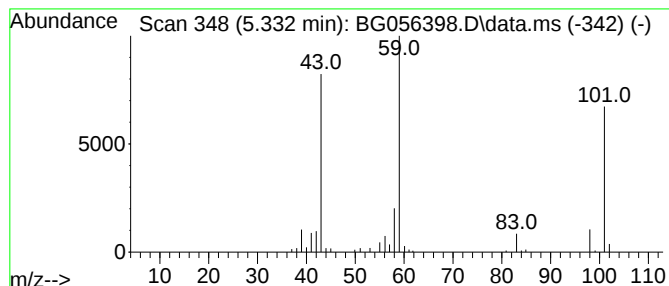

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056398.D
Acq On : 24 Jan 2023 11:20
Operator : CG/JU
Sample : PB150335BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150335BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.332	5.332	16.5	ng	147022	1	8.293	177811	20.0