


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056396.D
Acq On : 24 Jan 2023 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 25 04:54:56 2023

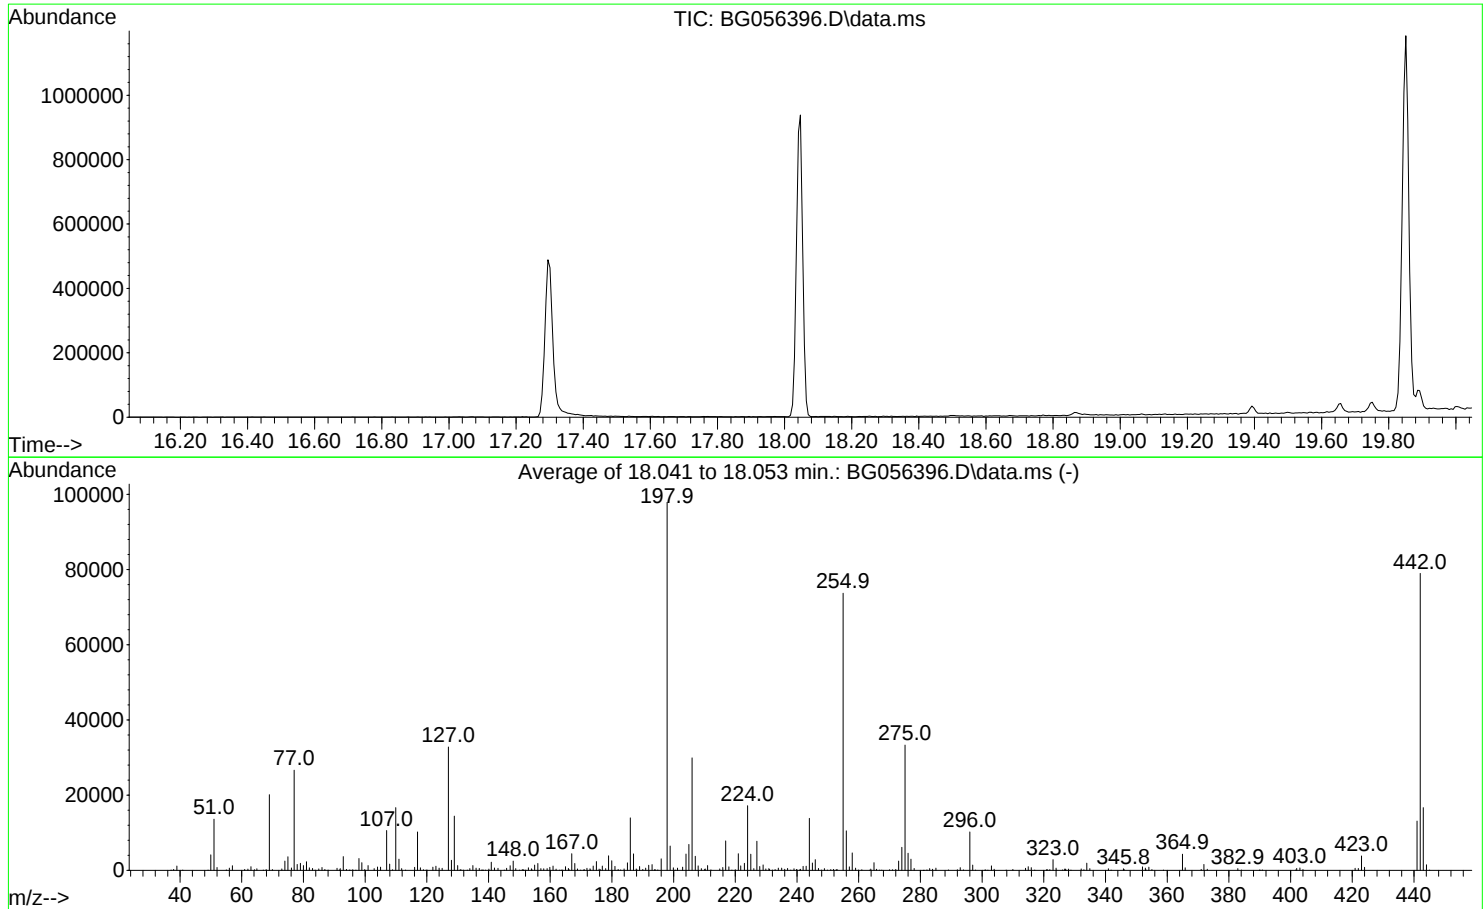




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.9	13616	PASS
68	69	0.00	2	0.9	178	PASS
69	198	0.00	100	20.5	20098	PASS
70	69	0.00	2	0.9	177	PASS
127	198	10	80	33.5	32811	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97843	PASS
199	198	5	9	6.6	6434	PASS
275	198	10	60	34.0	33296	PASS
365	198	1	100	4.4	4291	PASS
441	198	0.01	100	13.4	13090	PASS
442	442	50	100	100.0	78968	PASS
443	442	15	24	21.1	16665	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
 Data File : BG056396.D
 Acq On : 24 Jan 2023 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 08:29:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 04:54:56 2023
 Response via : Initial Calibration

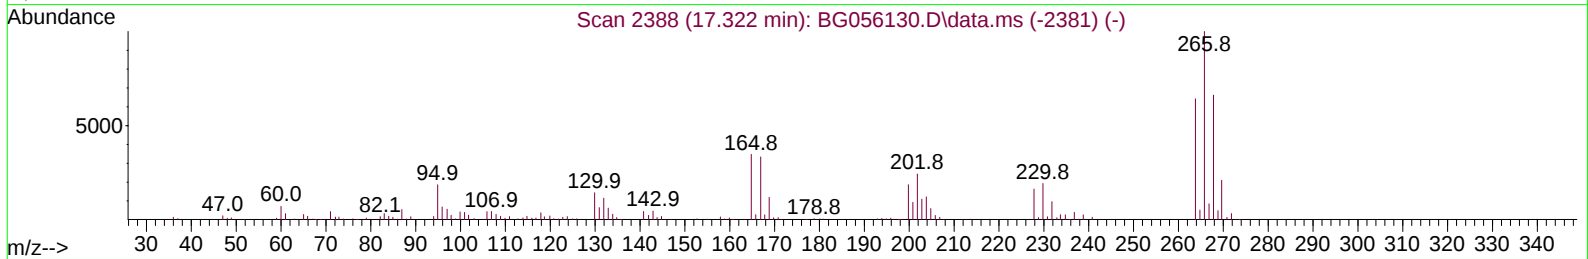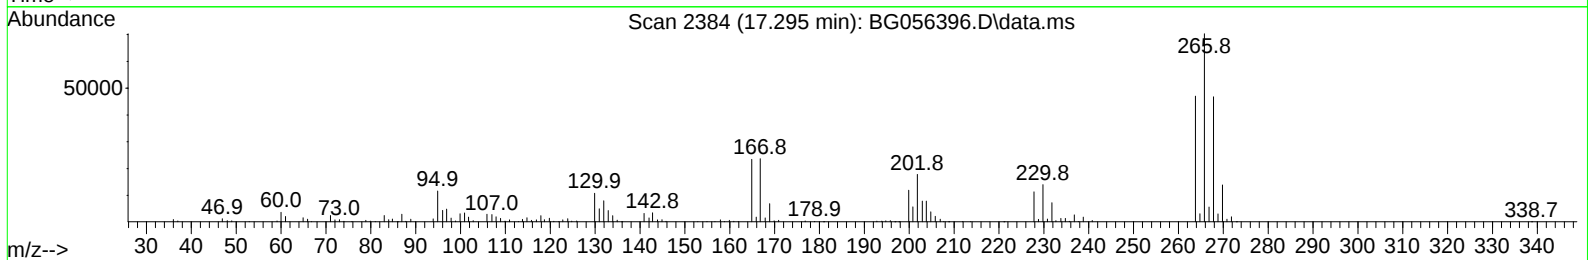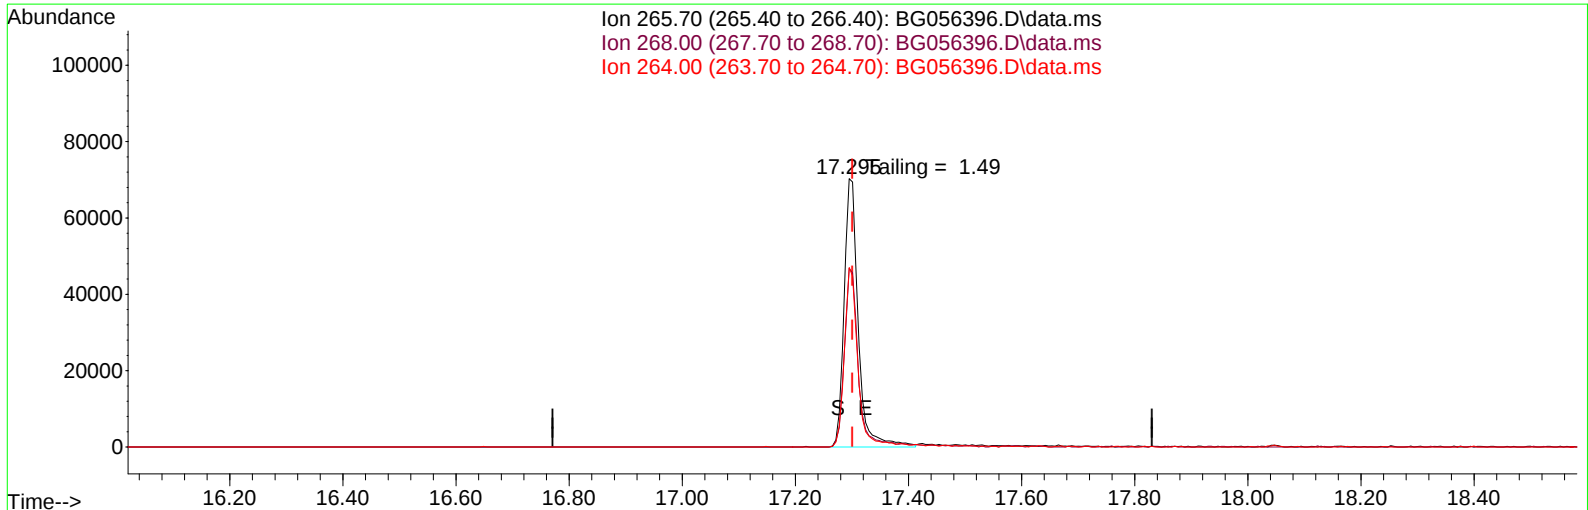

TIC: BG056396.D\data.ms

(70) Pentachlorophenol (C)

17.295min (-0.005) 17798.35 ng




response 122474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.58
264.00	64.30	66.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
 Data File : BG056396.D
 Acq On : 24 Jan 2023 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 08:29:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 04:54:56 2023
 Response via : Initial Calibration

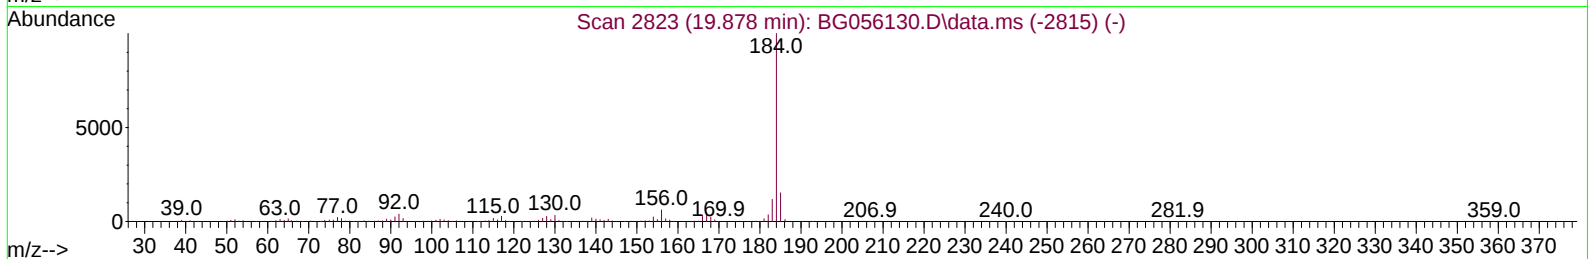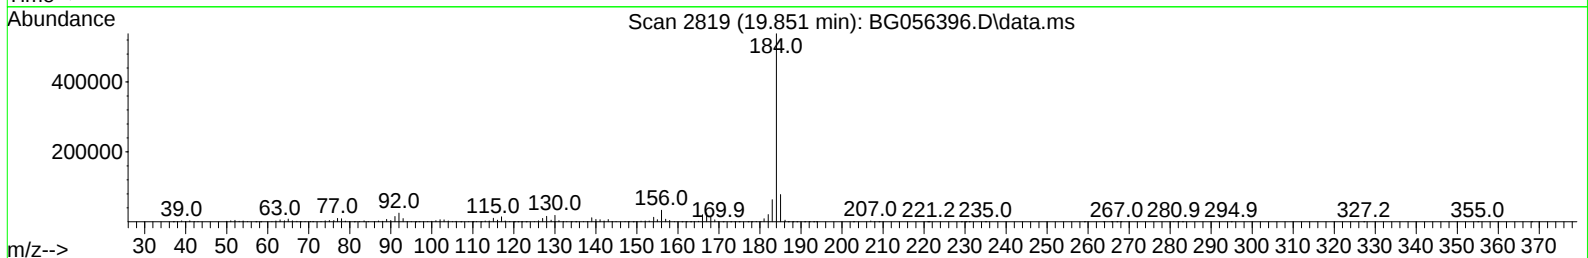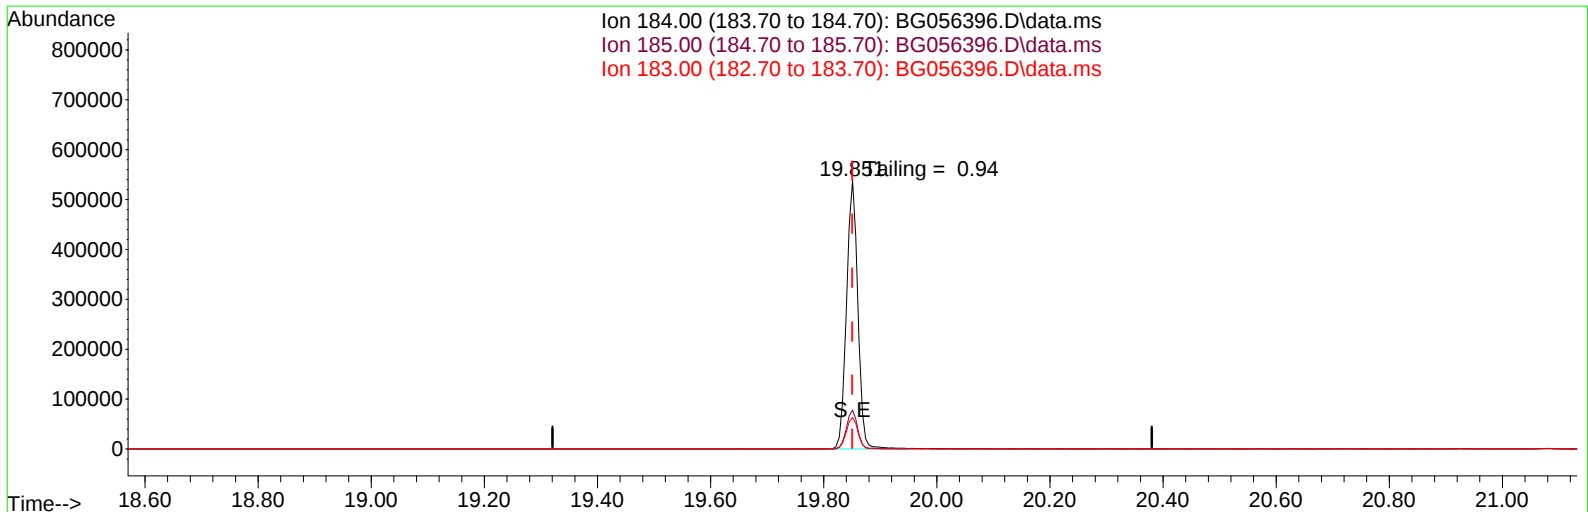

TIC: BG056396.D\data.ms

(77) Benzidine

19.851min (+ 0.001) 274788.40 ng

response 751122

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.49
183.00	11.70	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2023	BNA_G	<u>BG056396.D</u>
Compound Name	Response	Retention Time
DDT	344605	21.079
DDD	17707	20.626
DDE	1514	20.133
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19221	363826	5.28

Instrument :
BNA_G
ClientSampleId :
DFTPP