
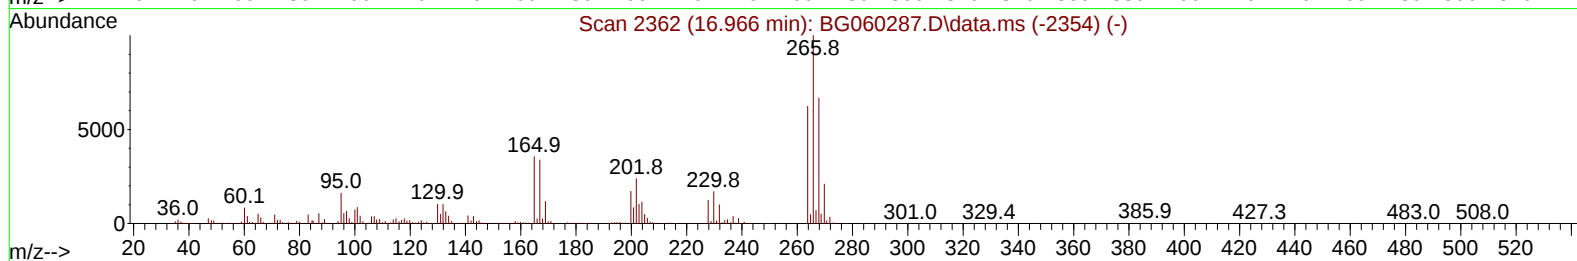
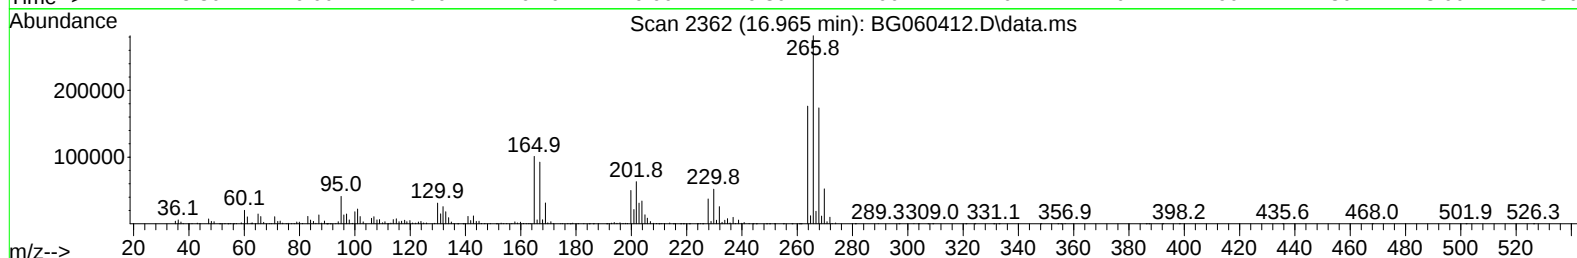


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012424\
Data File : BG060412.D
Acq On : 24 Jan 2024 12:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 16:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

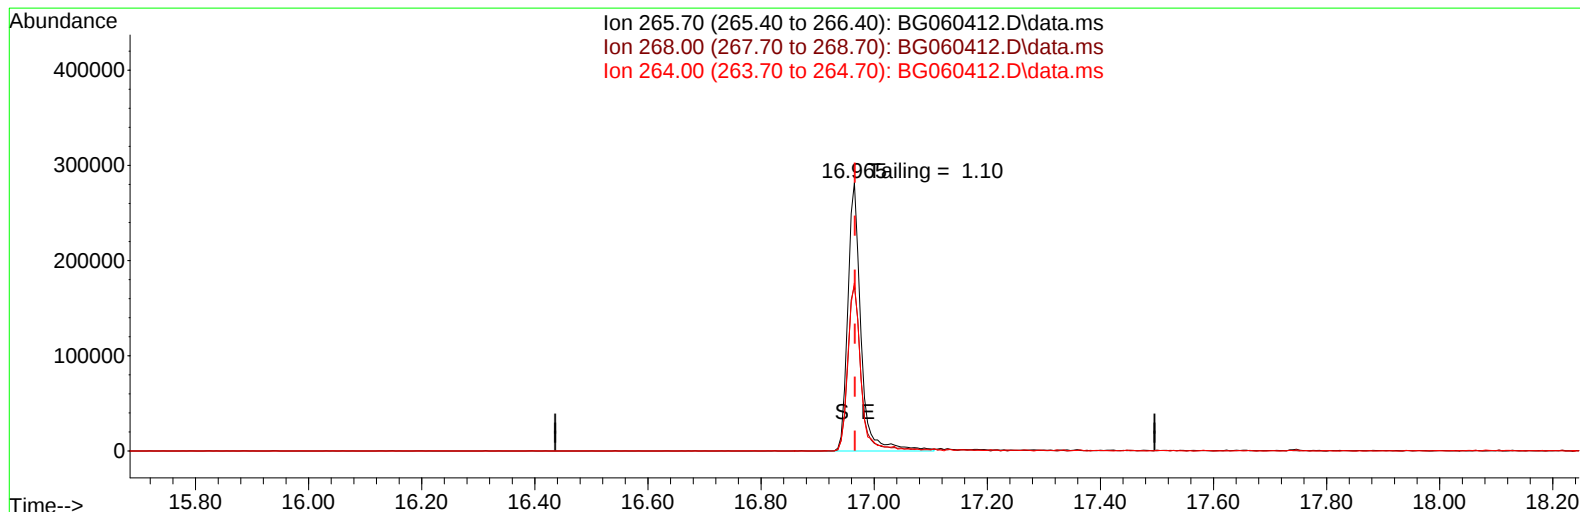

TIC: BG060412.D\data.ms

(70) Pentachlorophenol (C)




16.965min (-0.001) 624113.70 ng

response 455058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	61.60
264.00	62.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012424\
Data File : BG060412.D
Acq On : 24 Jan 2024 12:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 16:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

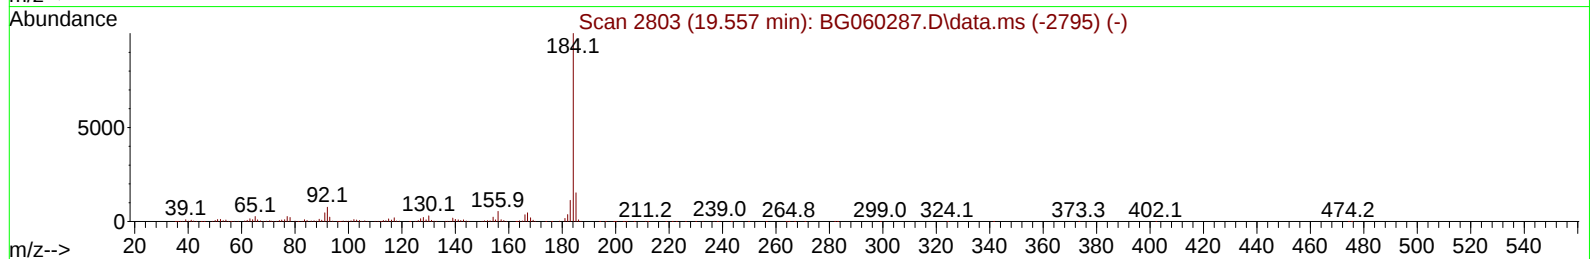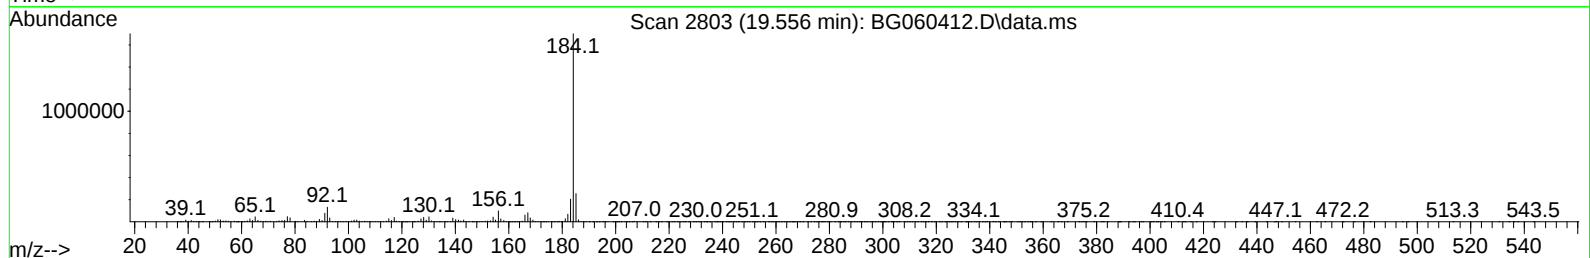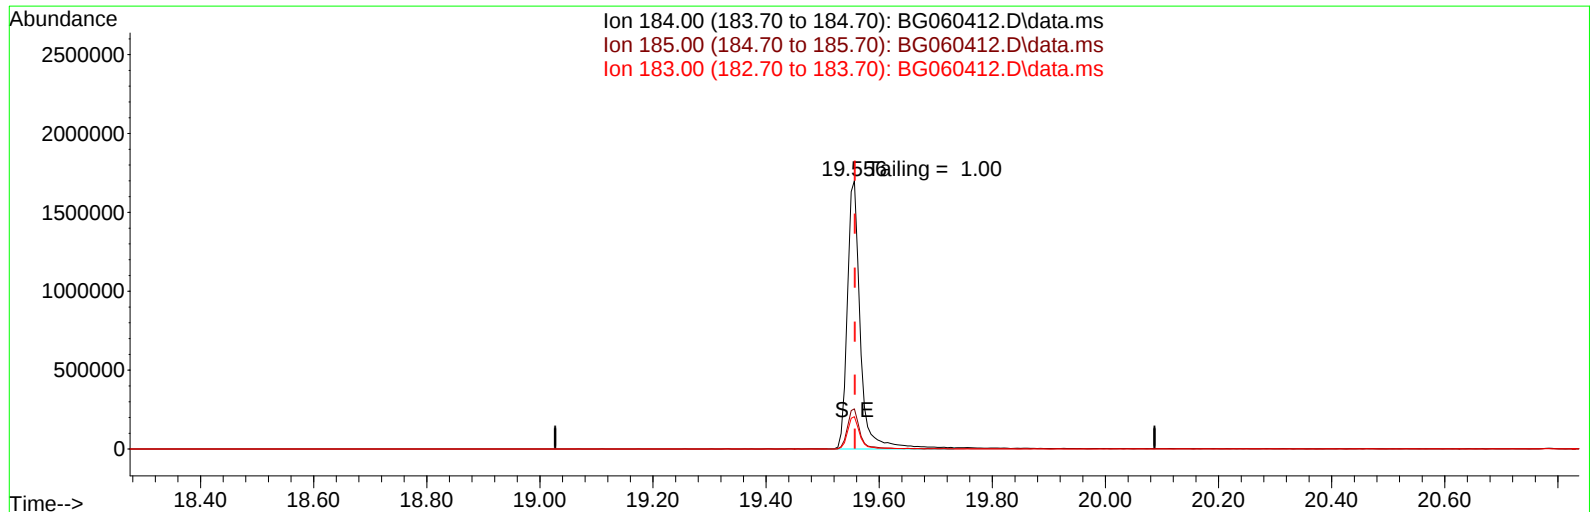

TIC: BG060412.D\data.ms

(77) Benzidine

19.556min (-0.001) 113912.98 ng

response 2655442

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.00
183.00	11.20	12.04
0.00	0.00	0.00