


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012424\
Data File : BG060412.D
Acq On : 24 Jan 2024 12:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

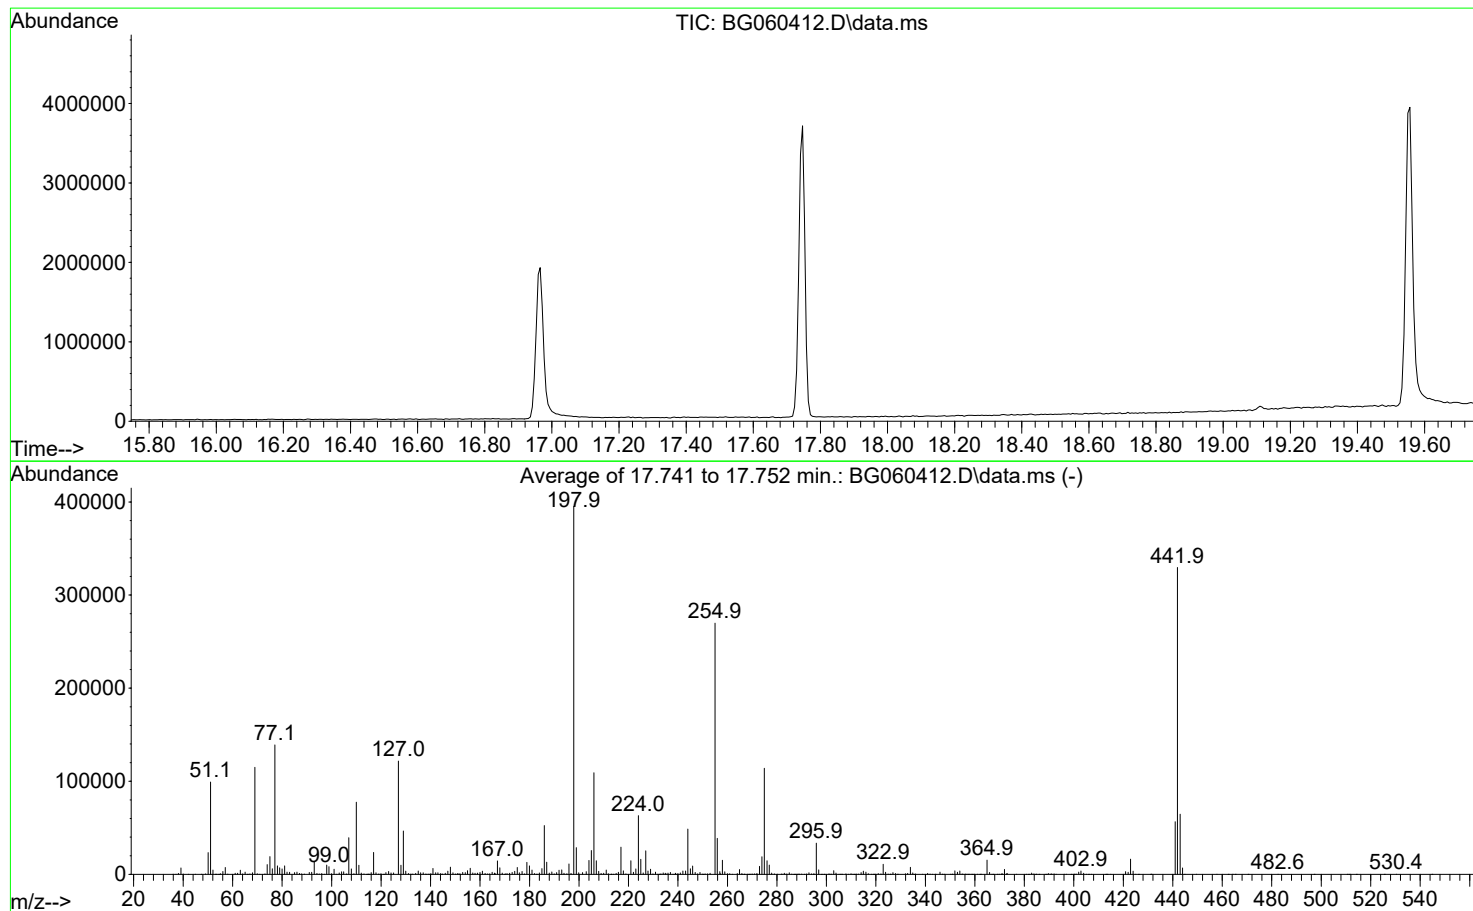

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	25.1	99109	PASS
68	69	0.00	2	1.4	1653	PASS
69	198	0.00	100	29.1	115020	PASS
70	69	0.00	2	0.5	630	PASS
127	198	10	80	30.8	121747	PASS
197	198	0.00	2	0.3	1083	PASS
198	198	100	100	100.0	395115	PASS
199	198	5	9	7.3	28690	PASS
275	198	10	60	28.9	114040	PASS
365	198	1	100	3.9	15248	PASS
441	198	0.01	100	14.3	56608	PASS
442	442	50	100	100.0	329664	PASS
443	442	15	24	19.6	64643	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/24/2024	BNA_G	BG060412.D
Compound Name	Response	Retention Time
DDT	1254663	20.784
DDD	52390	20.343
DDE	14010	19.838
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66400	1321063	5.03

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012424\
Data File : BG060412.D
Acq On : 24 Jan 2024 12:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 24 16:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

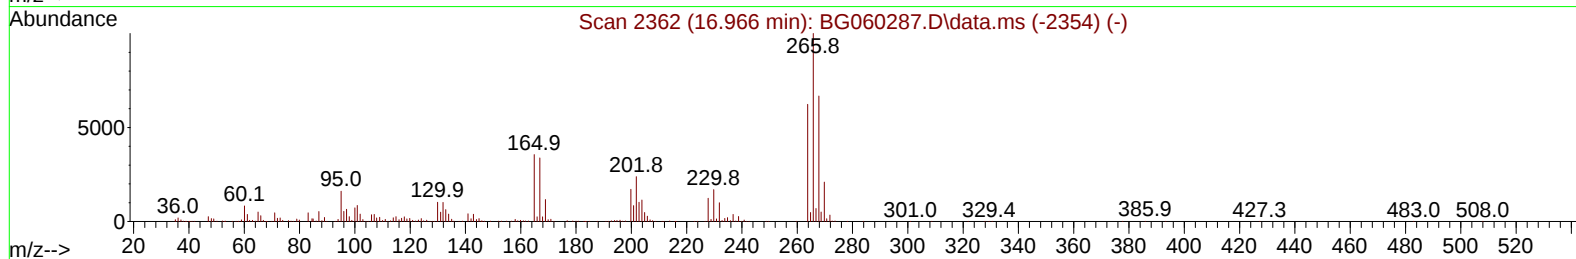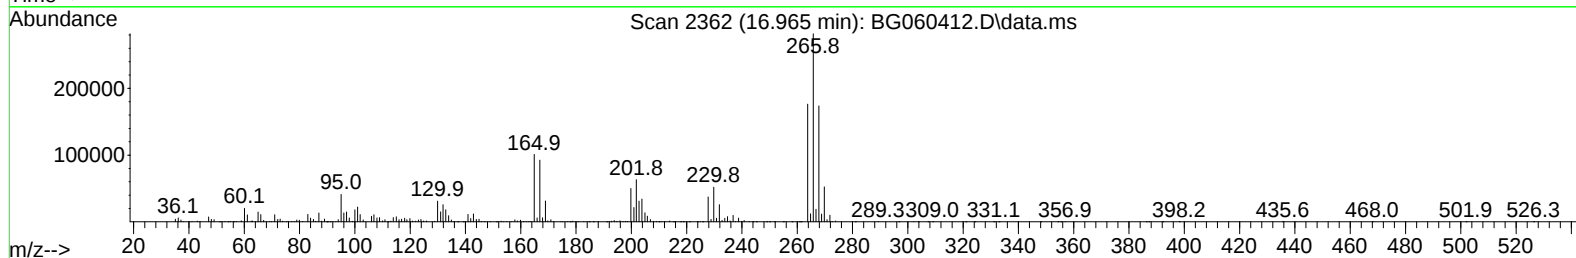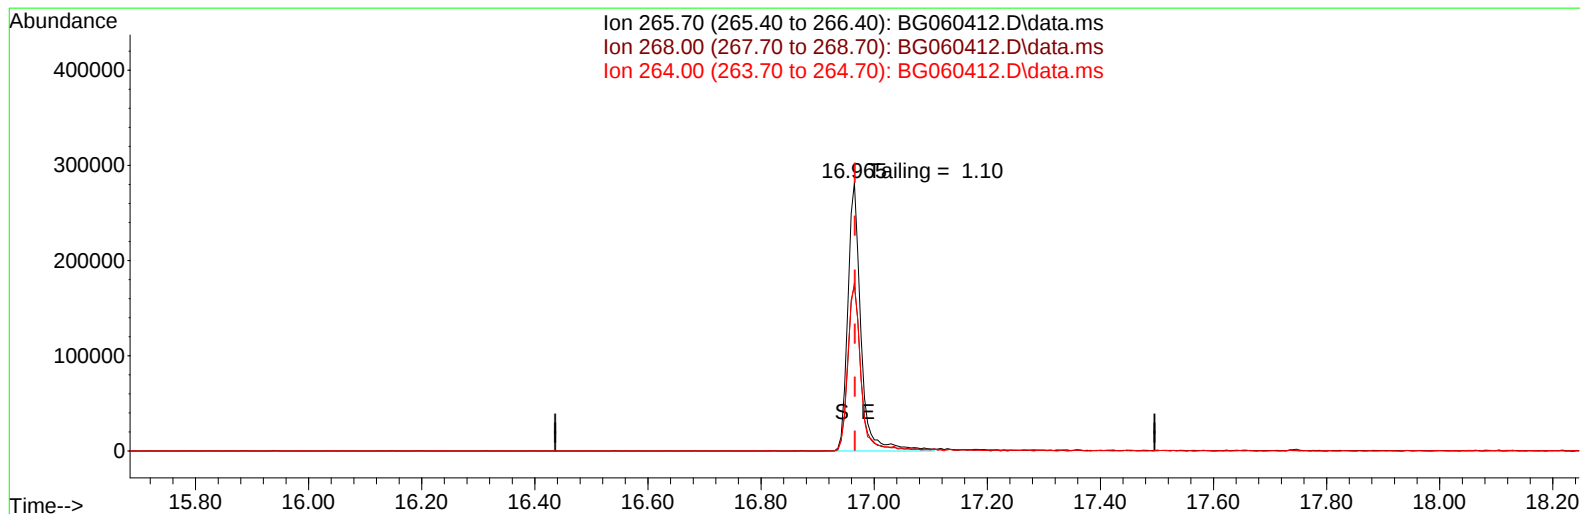

TIC: BG060412.D\data.ms

(70) Pentachlorophenol (C)

16.965min (-0.001) 624113.70 ng




response 455058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	61.60
264.00	62.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012424\
Data File : BG060412.D
Acq On : 24 Jan 2024 12:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 24 16:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

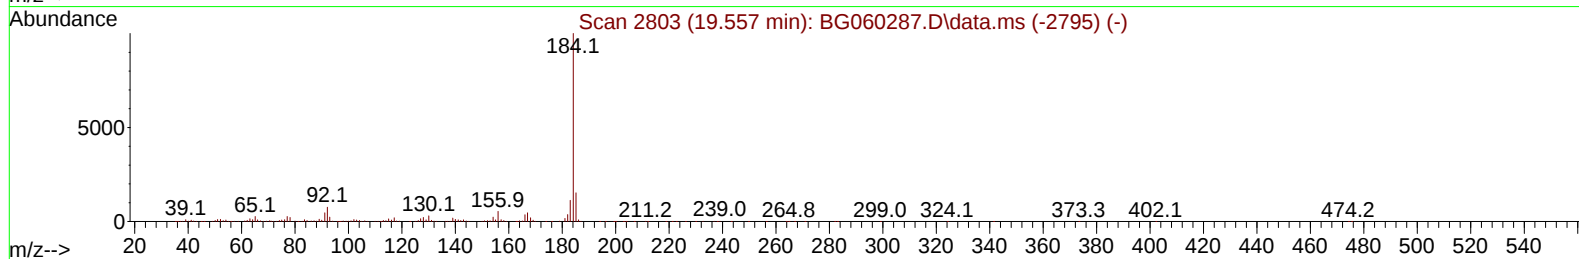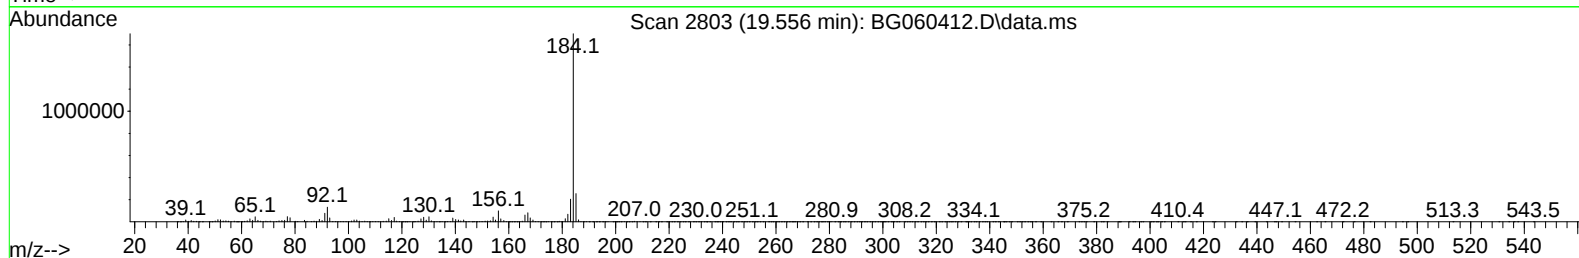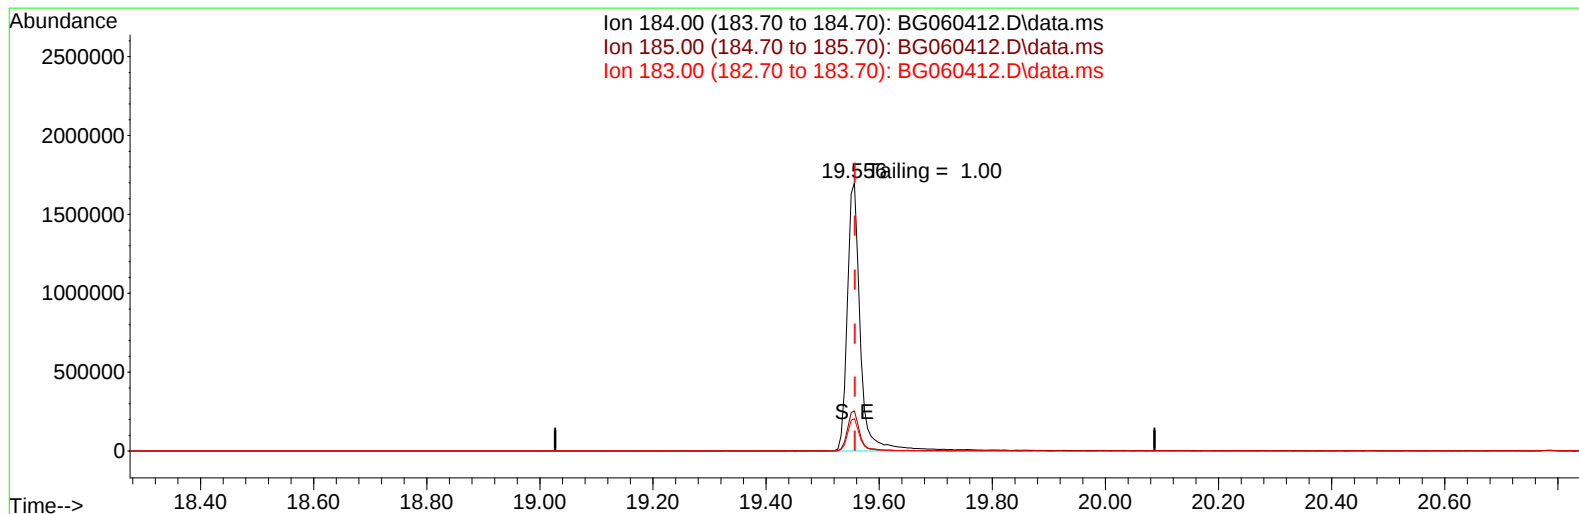

TIC: BG060412.D\data.ms

(77) Benzidine

19.556min (-0.001) 113912.98 ng

response 2655442

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.00
183.00	11.20	12.04
0.00	0.00	0.00