
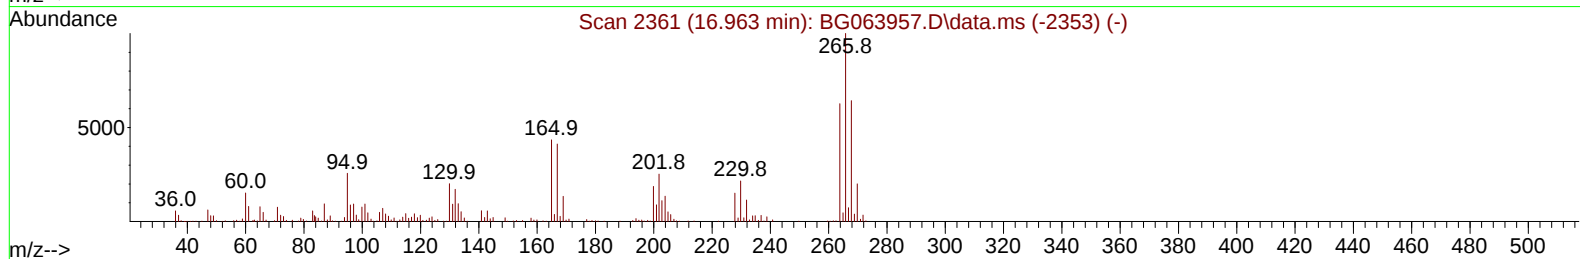
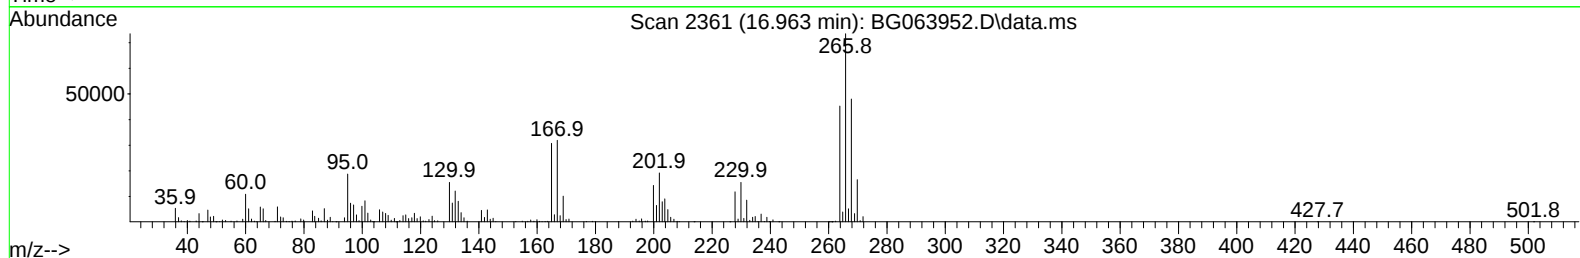


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012425\
Data File : BG063952.D
Acq On : 24 Jan 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 01:39:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 25 00:30:33 2025
Response via : Initial Calibration

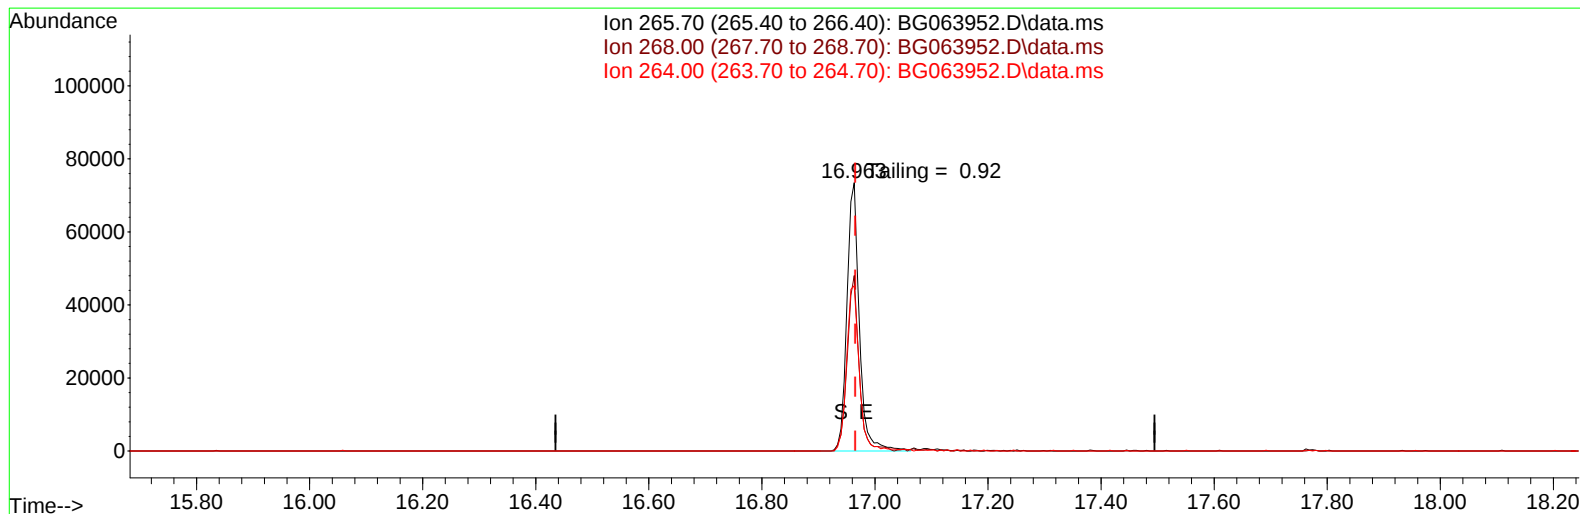

TIC: BG063952.D\data.ms

(70) Pentachlorophenol (C)




16.963min (-0.002) 270033.57 ng

response 112442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.36
264.00	62.60	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012425\
Data File : BG063952.D
Acq On : 24 Jan 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 01:39:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 25 00:30:33 2025
Response via : Initial Calibration

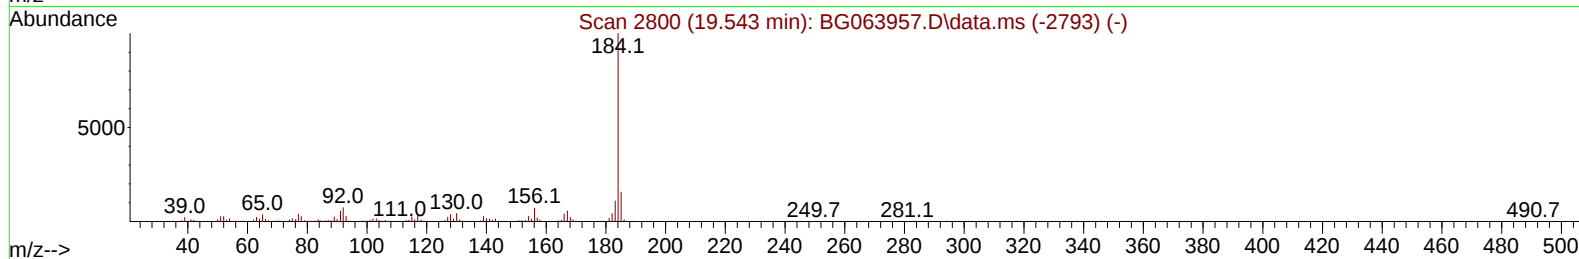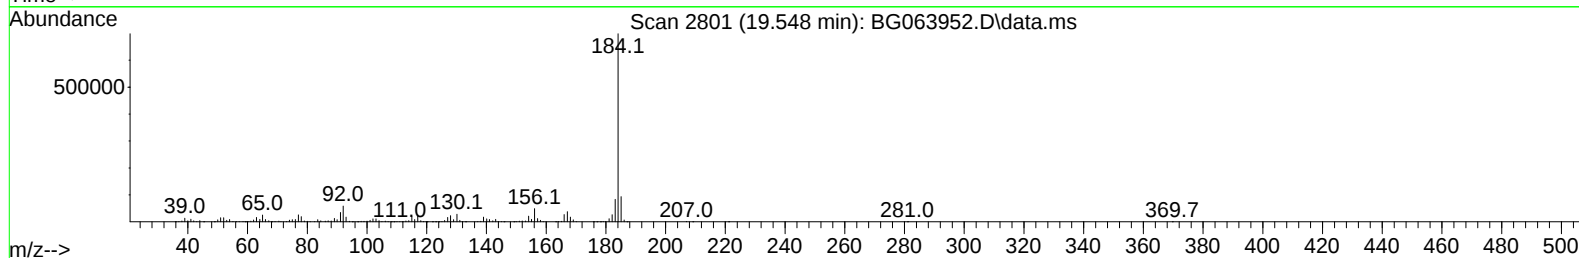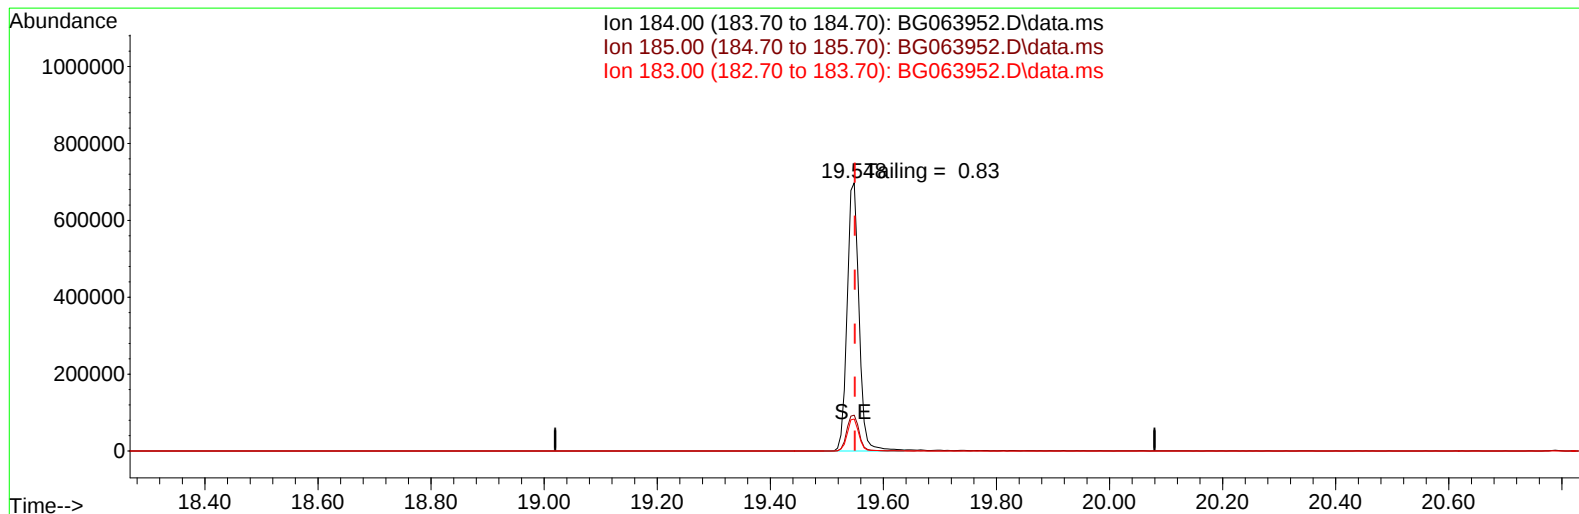

TIC: BG063952.D\data.ms

(77) Benzidine

19.548min (-0.002) 661532.41 ng m

response 1028310

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	13.35
183.00	11.00	11.93
0.00	0.00	0.00