
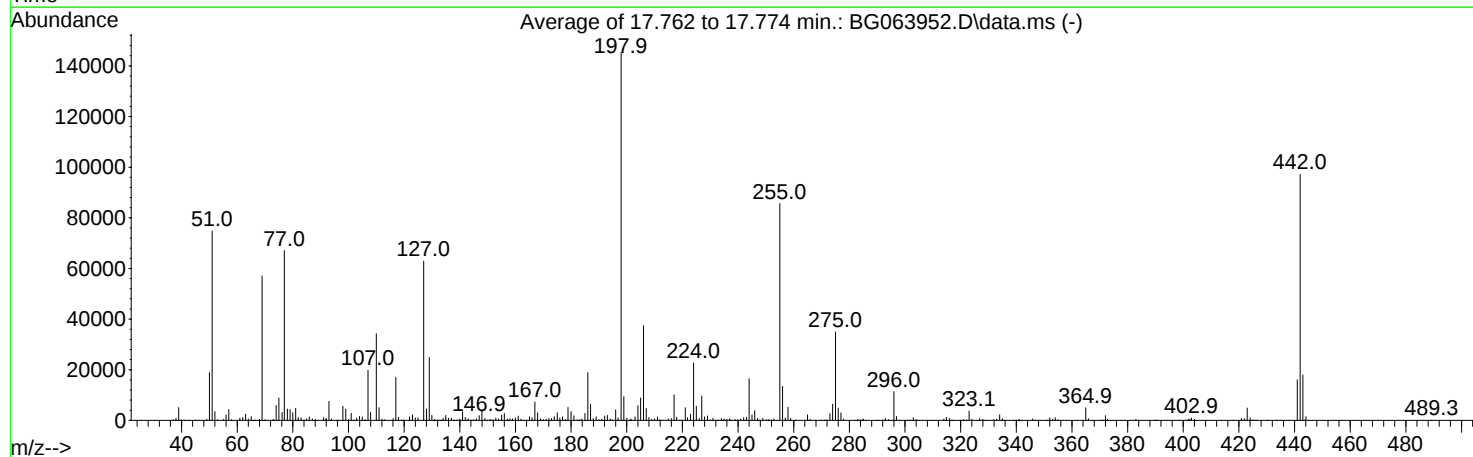


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012425\
Data File : BG063952.D
Acq On : 24 Jan 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jan 27 15:15:32 2025

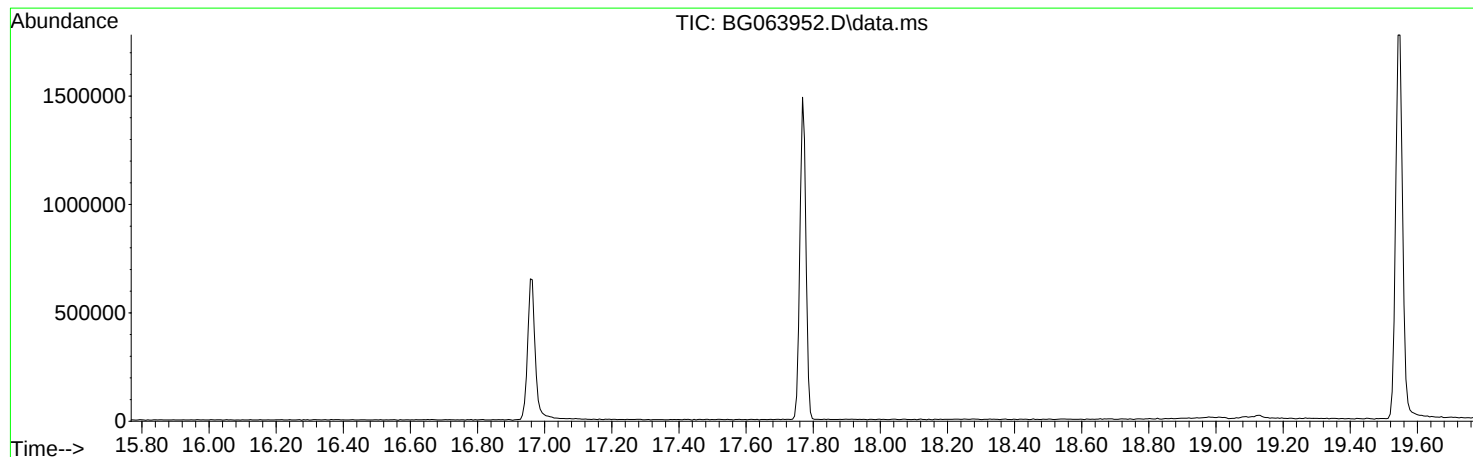




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	51.5	74765	PASS
68	69	0.00	2	0.7	424	PASS
69	198	0.00	100	39.3	57045	PASS
70	69	0.00	2	0.4	232	PASS
127	198	10	80	43.3	62904	PASS
197	198	0.00	2	0.6	939	PASS
198	198	100	100	100.0	145280	PASS
199	198	5	9	6.4	9357	PASS
275	198	10	60	24.1	34963	PASS
365	198	1	100	3.4	4935	PASS
441	198	0.01	100	11.0	16002	PASS
442	442	50	100	100.0	97136	PASS
443	442	15	24	18.4	17921	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012425\
Data File : BG063952.D
Acq On : 24 Jan 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 01:39:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 25 00:30:33 2025
Response via : Initial Calibration

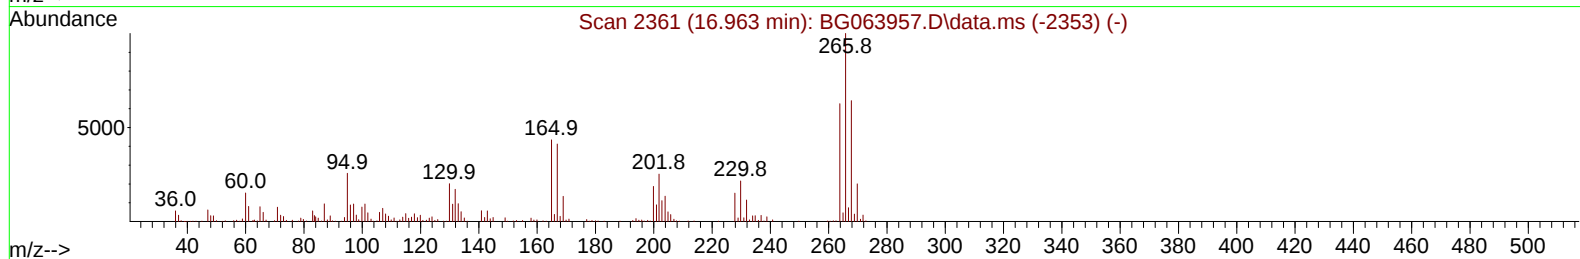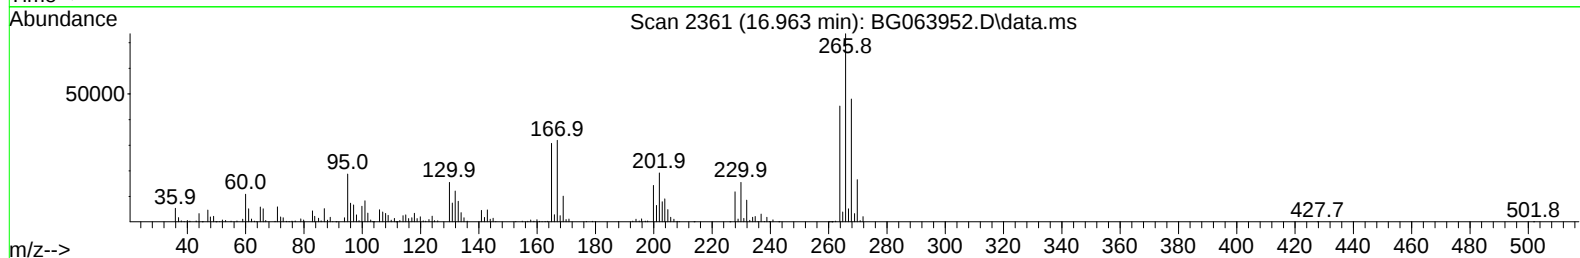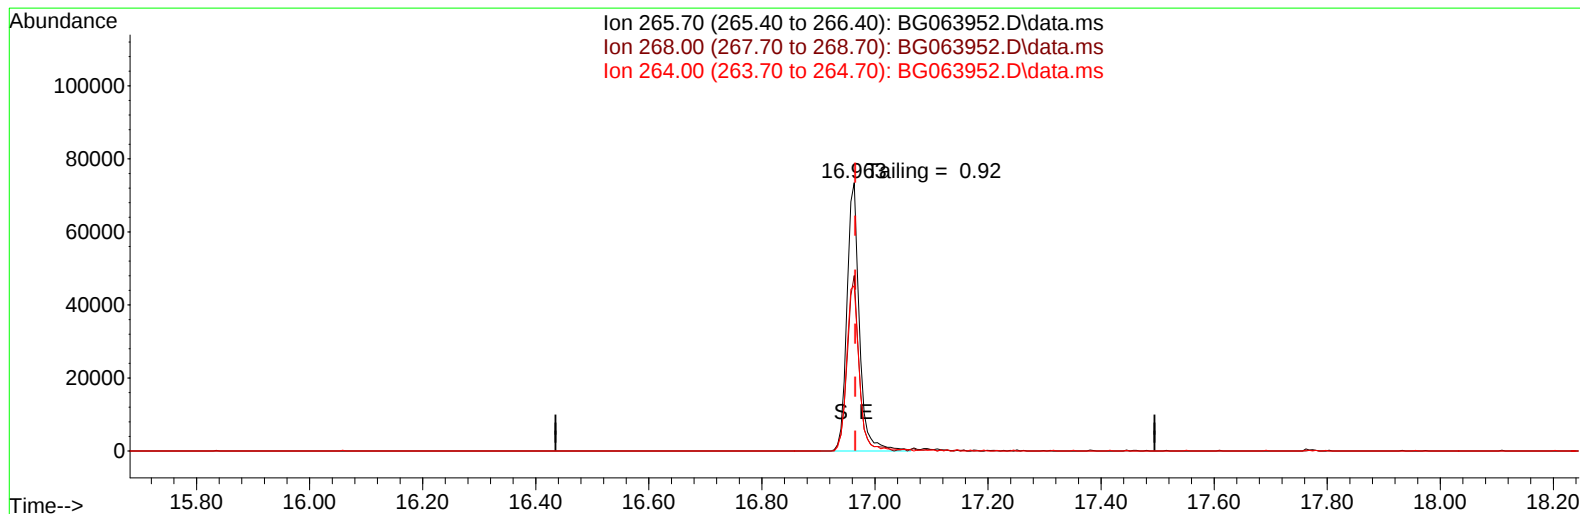

TIC: BG063952.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.002) 270033.57 ng




response 112442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	65.36
264.00	62.60	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012425\
Data File : BG063952.D
Acq On : 24 Jan 2025 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 01:39:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 25 00:30:33 2025
Response via : Initial Calibration

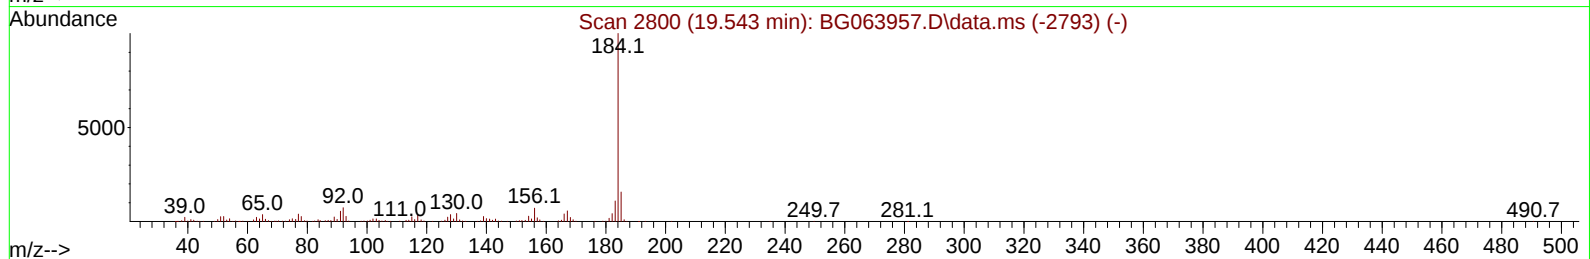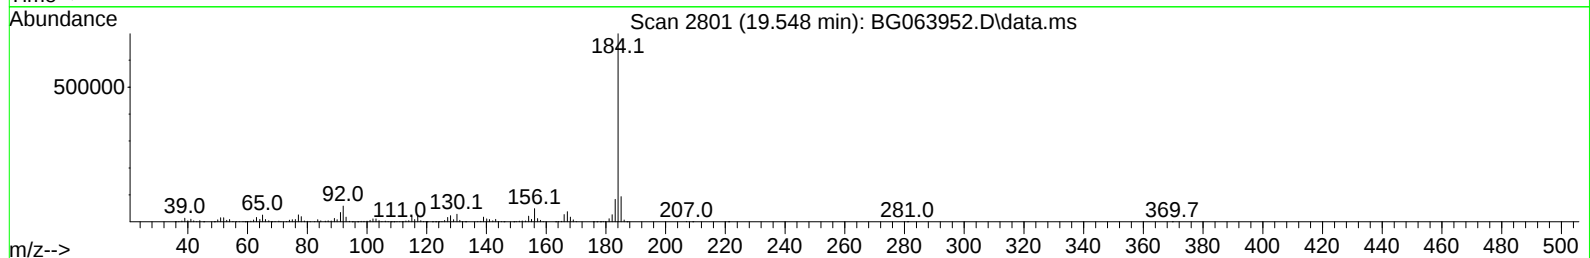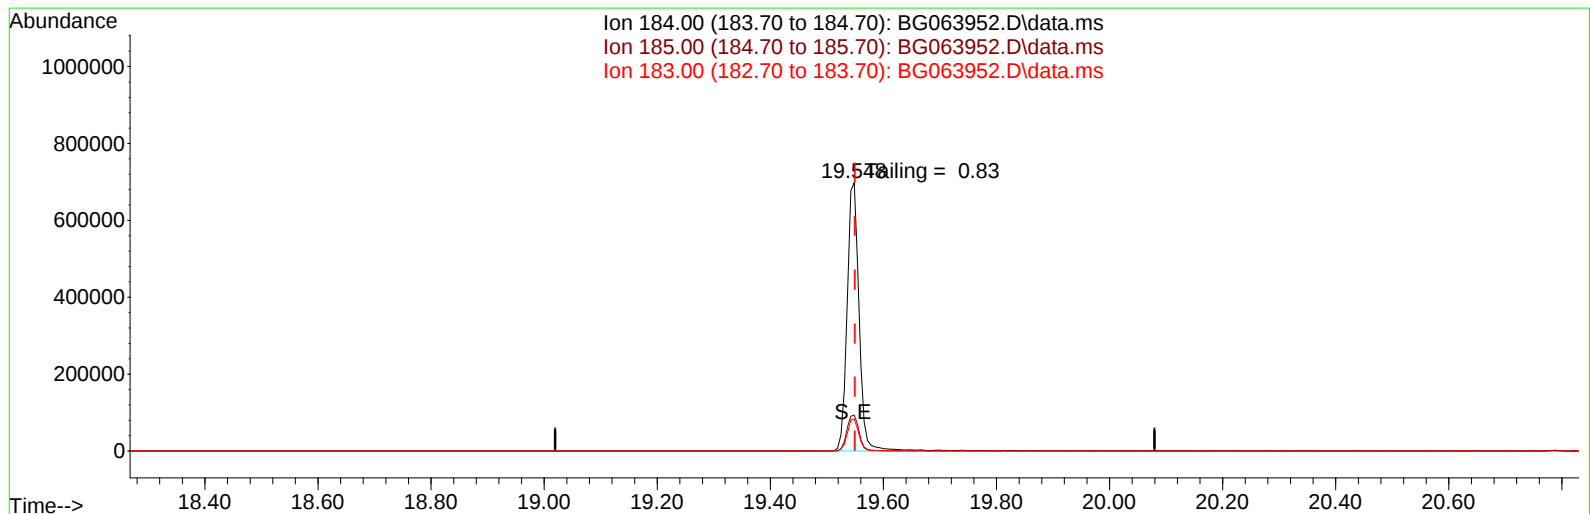

TIC: BG063952.D\data.ms

(77) Benzidine

19.548min (-0.002) 661532.41 ng m

response 1028310

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	13.35
183.00	11.00	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2025	BNA_G	<u>BG063952.D</u>
Compound Name	Response	Retention Time
DDT	210075	20.788
DDD	7331	20.347
DDE	1008	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8339	218414	3.82

Instrument :
BNA_G
ClientSampleId :
DFTPP